

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072320\
 Data File : FF007214.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jul 2020 15:32
 Operator : DD\AJ
 Sample : L3381-10
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 359-GRID-A1-A3

Integration File: autoint1.e
 Quant Time: Jul 24 01:45:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.751	1954635	13.865 ug/ml
Target Compounds			
4) N-TETRADECANE	8.251	421890	2.725 ug/ml
7) N-EICOSANE	12.595f	388518	2.406 ug/ml
8) N-DOCOSANE	13.832	177860	1.097 ug/ml
10) N-TETRACOSANE	14.936	1463438	8.936 ug/ml
12) N-OCTACOSANE	16.937	455842	2.782 ug/ml
13) N-TRIACONTANE	17.823	399852	2.419 ug/ml
14) N-DOTRIACONTANE	18.641	1400472	8.917 ug/ml
15) N-TETRATRIACONTANE	19.480	269652	2.071 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072320\
Data File : FF07214.D
Signal(s) : FID2B.ch
Acq On : 23 Jul 2020 15:32
Operator : DD\AJ
Sample : L3381-10
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
359-GRID-A1-A3

Integration File: autoint1.e
Quant Time: Jul 24 01:45:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

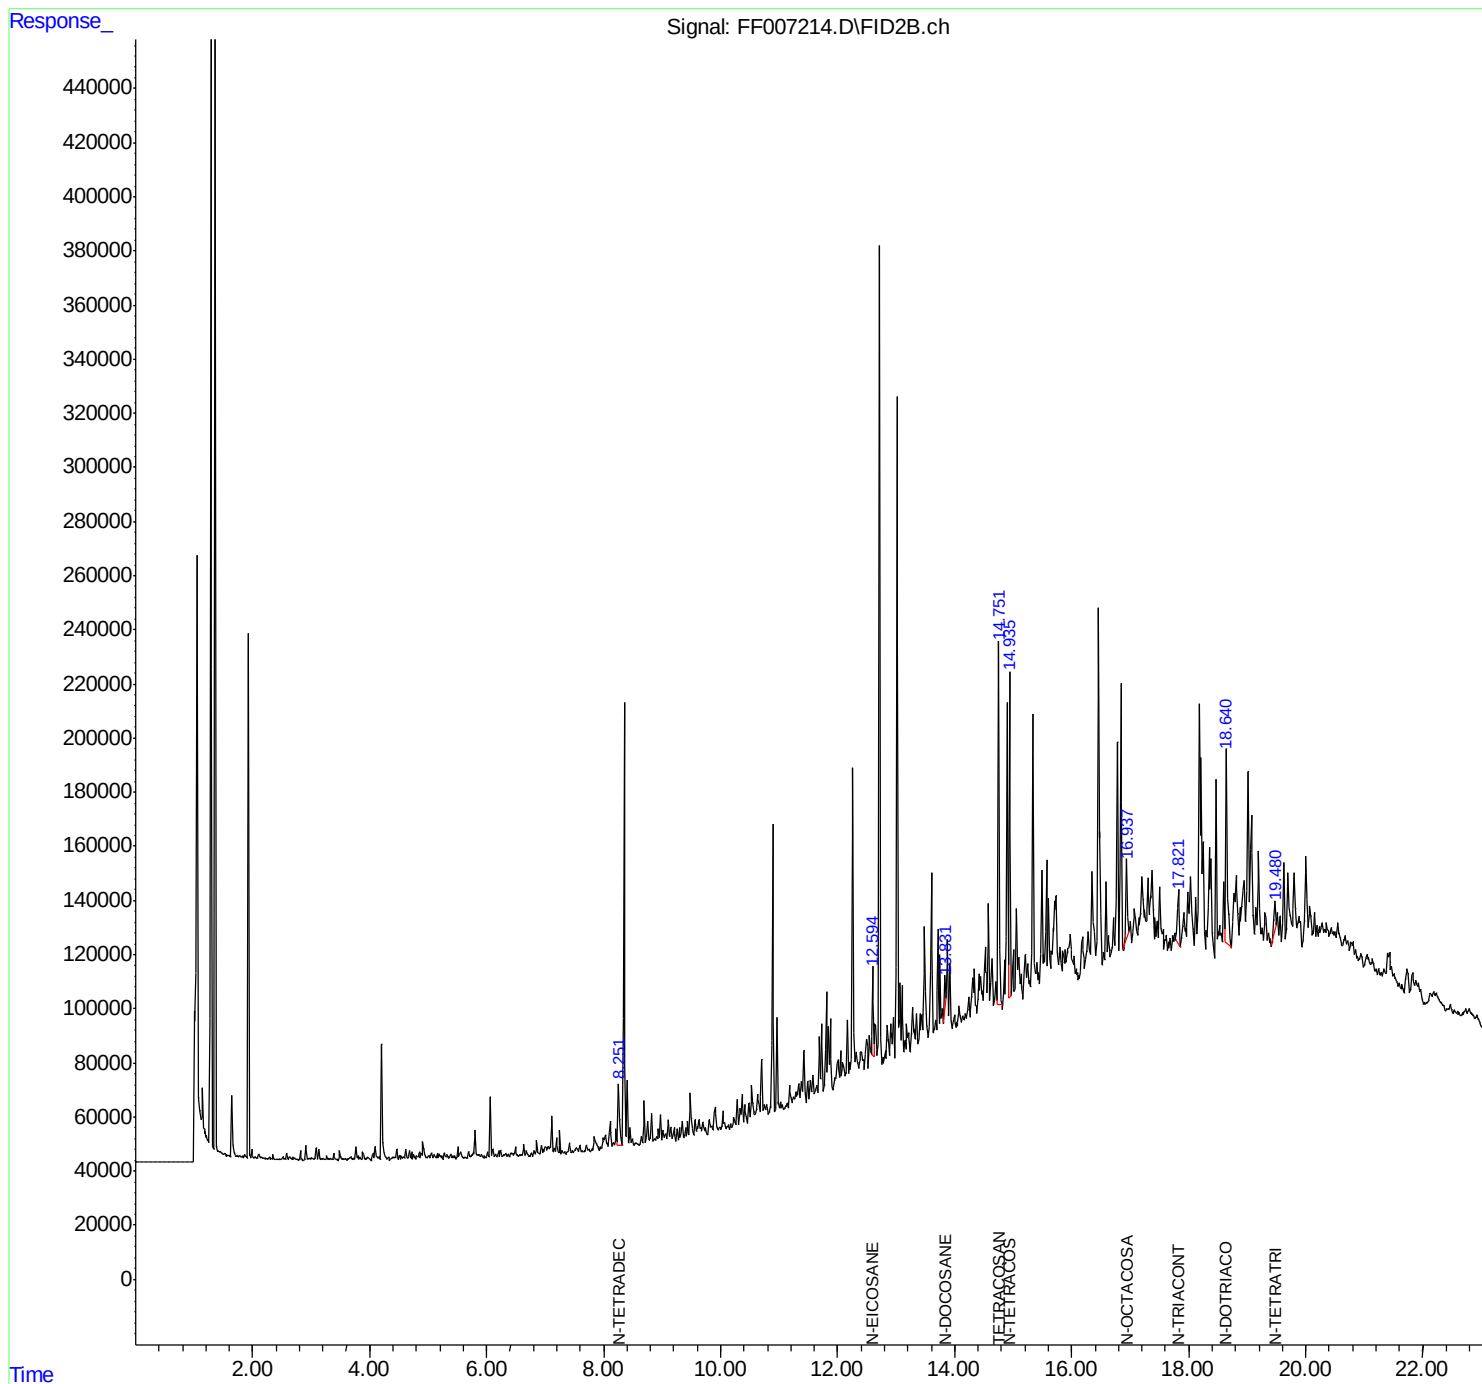


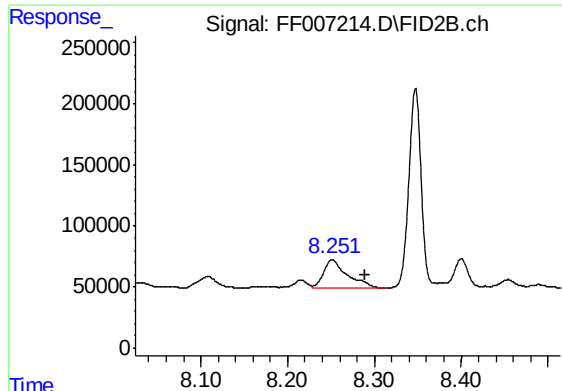

#4 N-TETRADECANE


R.T.: 8.251 min
Delta R.T.: -0.038 min
Response: 421890
Conc: 2.72 ug/ml

Instrument :
FID_B
ClientSampleId :
359-GRID-A1-A3

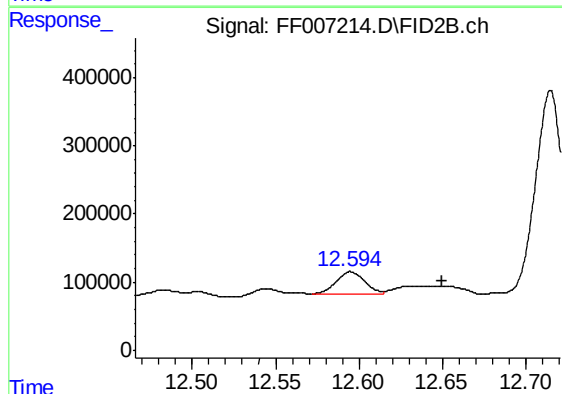


#7 N-EICOSANE

R.T.: 12.595 min
Delta R.T.: -0.055 min
Response: 388518
Conc: 2.41 ug/ml

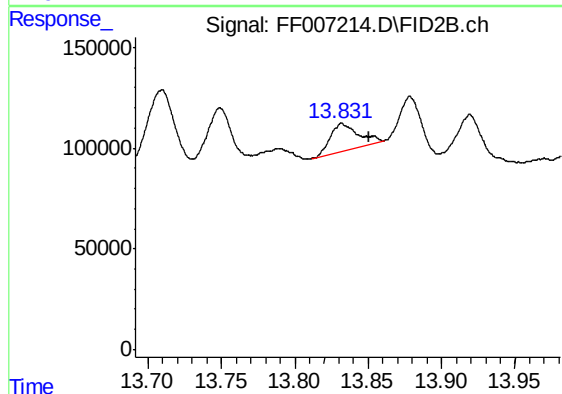


#8 N-DOCOSANE

R.T.: 13.832 min
Delta R.T.: -0.018 min
Response: 177860
Conc: 1.10 ug/ml

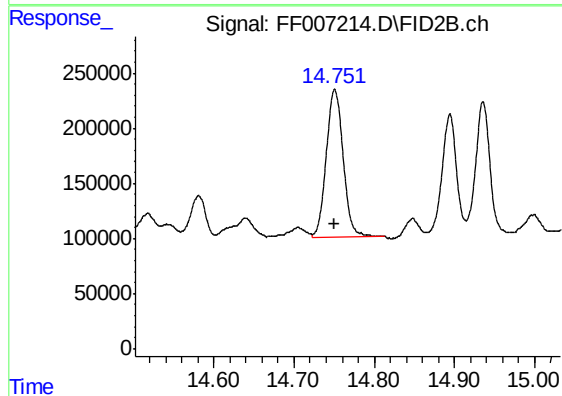

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.751 min
Delta R.T.: 0.000 min
Response: 1954635
Conc: 13.86 ug/ml

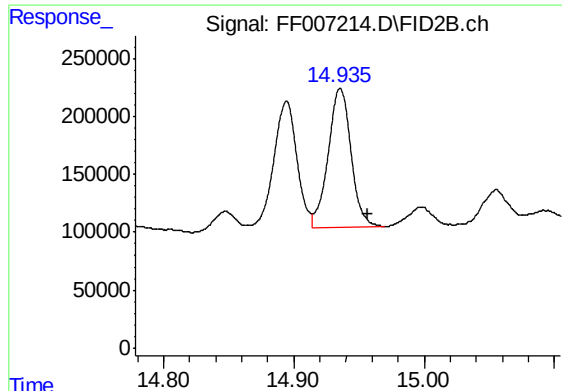

#10 N-TETRACOSANE


R.T.: 14.936 min
Delta R.T.: -0.021 min
Response: 1463438
Conc: 8.94 ug/ml

Instrument :
FID_B
ClientSampleId :
359-GRID-A1-A3

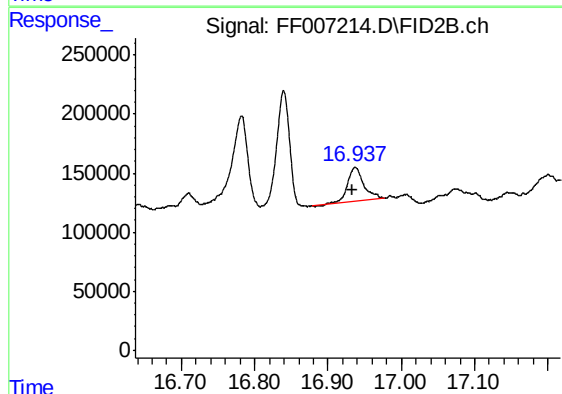


#12 N-OCTACOSANE

R.T.: 16.937 min
Delta R.T.: 0.005 min
Response: 455842
Conc: 2.78 ug/ml

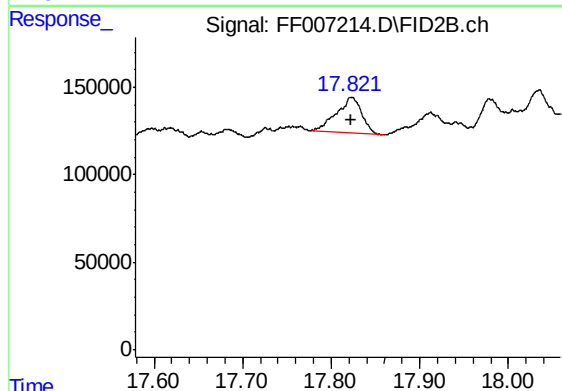


#13 N-TRIACONTANE

R.T.: 17.823 min
Delta R.T.: 0.000 min
Response: 399852
Conc: 2.42 ug/ml

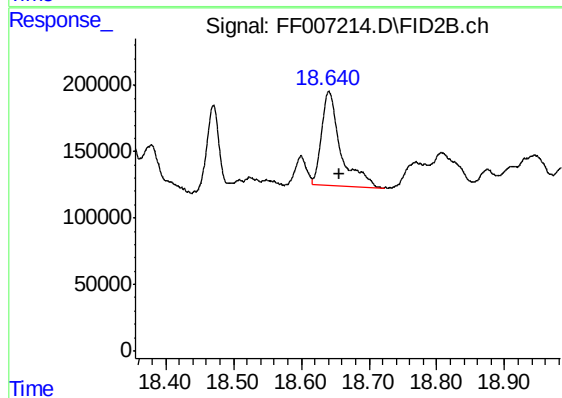

#14 N-DOTRIACONTANE

R.T.: 18.641 min
Delta R.T.: -0.015 min
Response: 1400472
Conc: 8.92 ug/ml

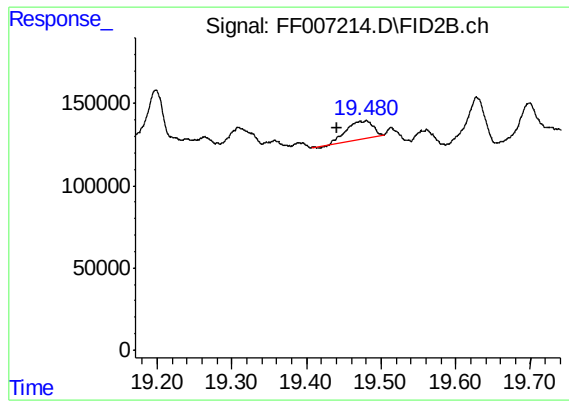

#15 N-TETRATRIACONTANE

R.T.: 19.480 min
Delta R.T.: 0.040 min
Response: 269652
Conc: 2.07 ug/ml

Instrument :
FID_B
ClientSampleId :
359-GRID-A1-A3