

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072418\
 Data File : FB016899.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jul 2018 11:50
 Operator : MJ/SJ
 Sample : J4119-02 MSD
 Misc : 5.04g/5.00ml DI water
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 24 12:15:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
 Quant Title :
 QLast Update : Mon Jul 09 13:06:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.116	161783	18.556 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.965	371346	25.562 ng/ml
2) t 2,2,4-Trimethylpentane	7.732	349633	25.137 ng/ml
3) t n-Heptane	8.068	108248	7.989 ng/ml
4) t Benzene	8.211	161373	8.696 ng/ml
6) t Toluene	10.963	381533	26.127 ng/ml
7) t Ethylbenzene	13.413	120418	8.198 ng/ml
8) t m-Xylene	13.545	246189	15.805 ng/ml
9) t O-Xylene	14.277	259393	15.671 ng/ml
10) t 1,2,4-Trimethylbenzene	16.559	305395	15.616 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072418\
Data File : FB016899.D
Signal(s) : FID2B.CH
Acq On : 24 Jul 2018 11:50
Operator : MJ/SJ
Sample : J4119-02 MSD
Misc : 5.04g/5.00ml DI water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 24 12:15:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
Quant Title :
QLast Update : Mon Jul 09 13:06:15 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

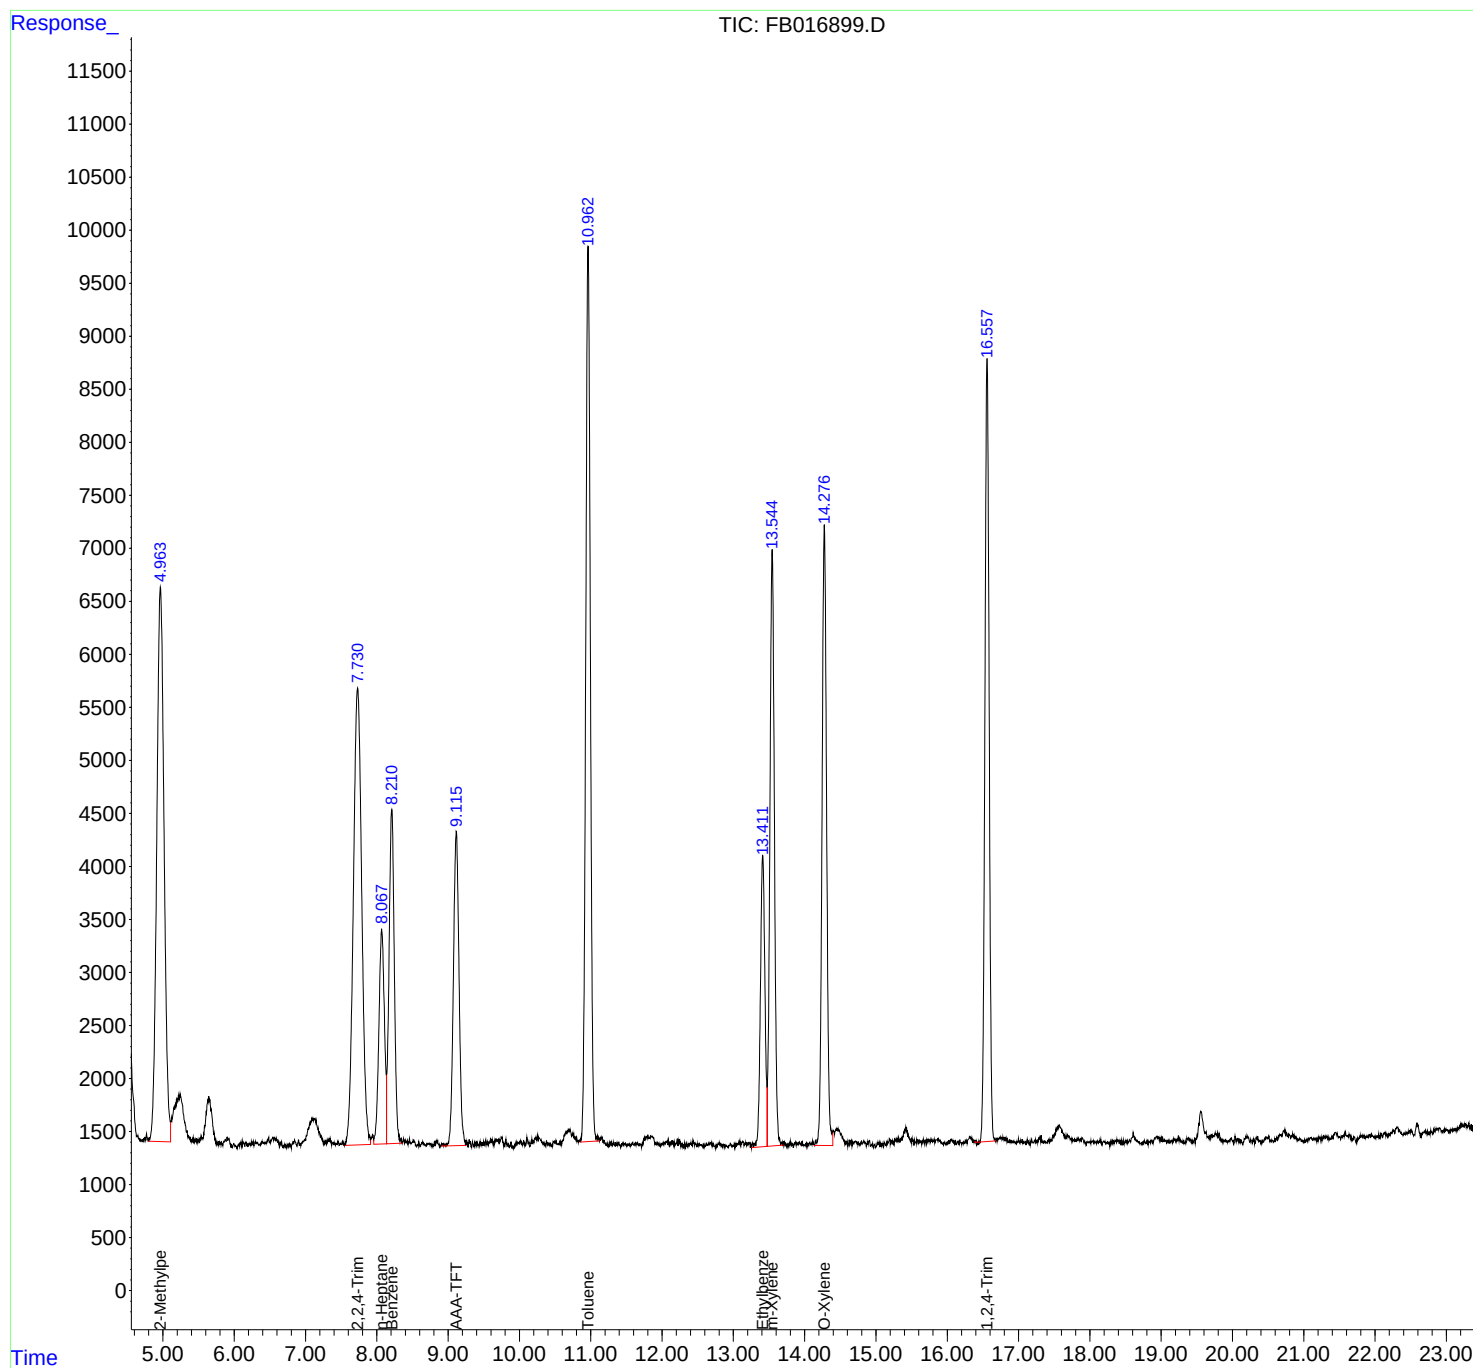

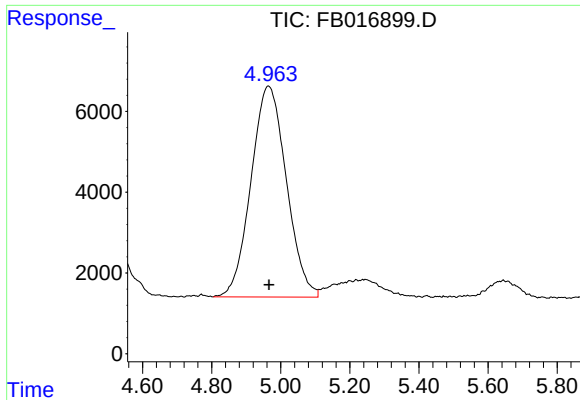


#1 2-Methylpentane

R.T.: 4.965 min
Delta R.T.: -0.001 min
Response: 371346
Conc: 25.56 ng/ml

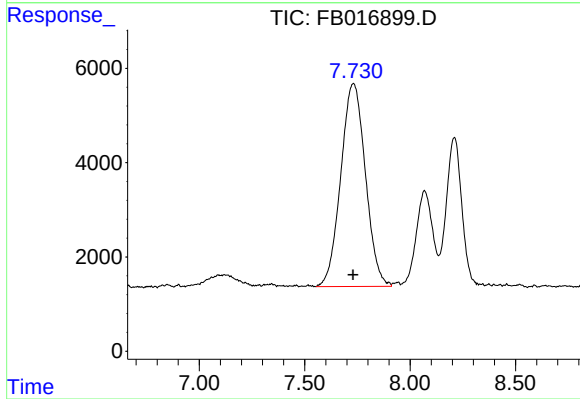


#2 2,2,4-Trimethylpentane

R.T.: 7.732 min
Delta R.T.: 0.003 min
Response: 349633
Conc: 25.14 ng/ml

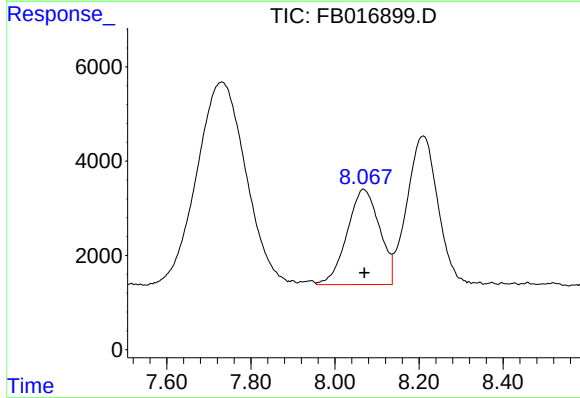


#3 n-Heptane

R.T.: 8.068 min
Delta R.T.: -0.002 min
Response: 108248
Conc: 7.99 ng/ml

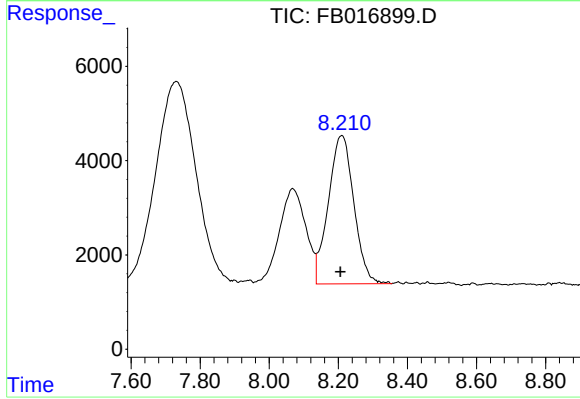


#4 Benzene

R.T.: 8.211 min
Delta R.T.: 0.005 min
Response: 161373
Conc: 8.70 ng/ml

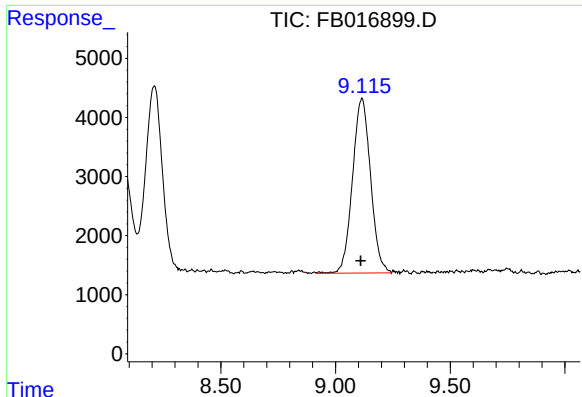


#5 AAA-TFT

R.T.: 9.116 min
Delta R.T.: 0.006 min
Response: 161783
Conc: 18.56 ng/ml

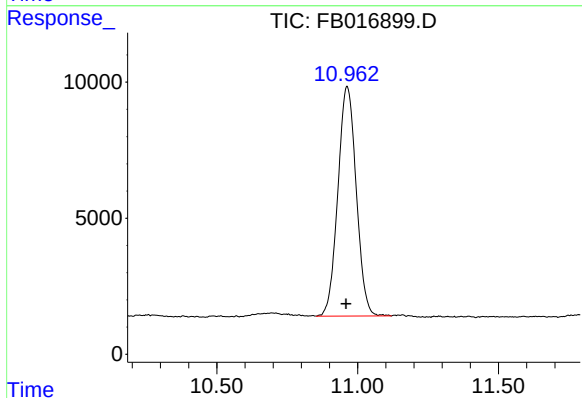


#6 Toluene

R.T.: 10.963 min
Delta R.T.: 0.003 min
Response: 381533
Conc: 26.13 ng/ml

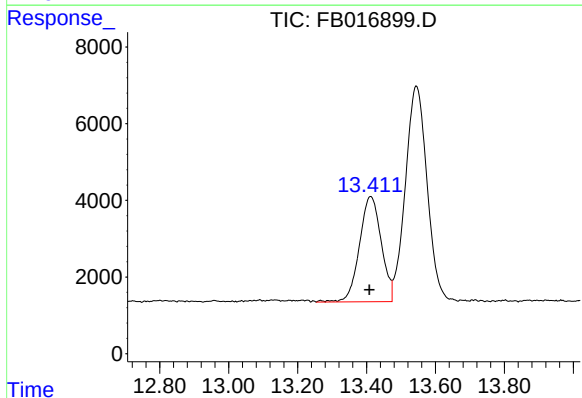


#7 Ethylbenzene

R.T.: 13.413 min
Delta R.T.: 0.004 min
Response: 120418
Conc: 8.20 ng/ml

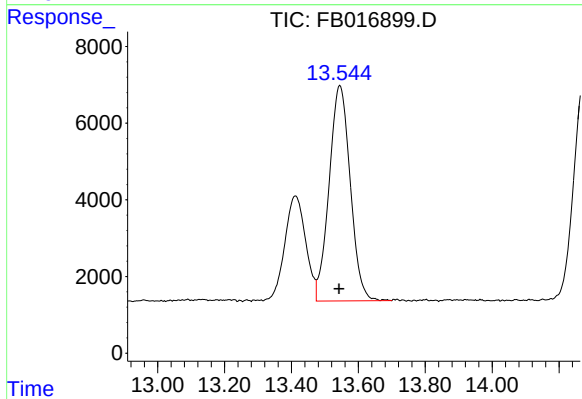


#8 m-Xylene

R.T.: 13.545 min
Delta R.T.: 0.003 min
Response: 246189
Conc: 15.81 ng/ml

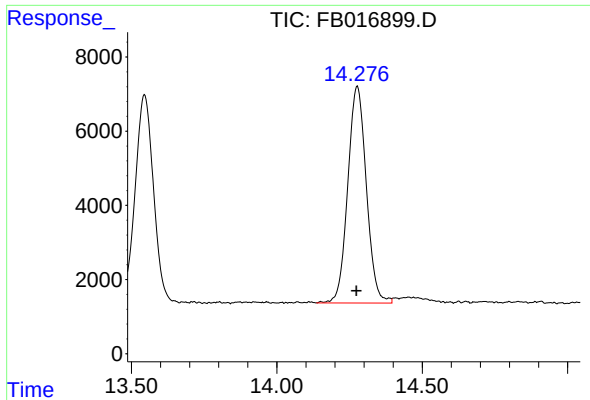

#9 O-Xylene

R.T.: 14.277 min
Delta R.T.: 0.003 min
Response: 259393
Conc: 15.67 ng/ml

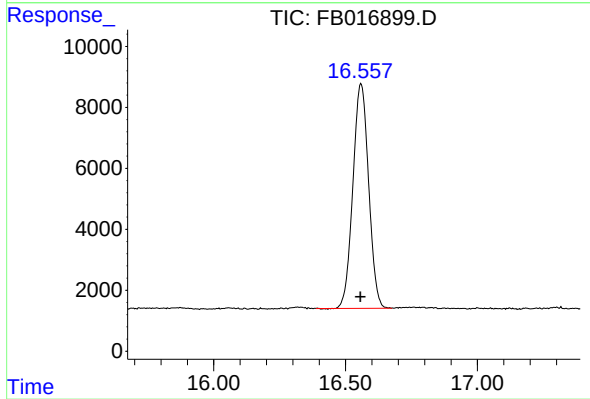

#10 1,2,4-Trimethylbenzene

R.T.: 16.559 min
Delta R.T.: 0.003 min
Response: 305395
Conc: 15.62 ng/ml