

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072419\
 Data File : FB021801.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jul 2019 9:56
 Operator : DD/AJ
 Sample : BSF0724S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 25 01:04:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.987	283958	20.808 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.861	757841	27.482 ng/ml
2) t	2,2,4-Trimethylpentane	7.608	738550	27.939 ng/ml
3) t	n-Heptane	7.947	226097	9.119 ng/ml
4) t	Benzene	8.081	302779	10.364 ng/ml
6) t	Toluene	10.828	658348	31.995 ng/ml
7) t	Ethylbenzene	13.273	230212	11.065 ng/ml
8) t	m-Xylene	13.406	491680	22.133 ng/ml
9) t	O-Xylene	14.135	495631	21.547 ng/ml
10) t	1,2,4-Trimethylbenzene	16.414	492588	20.893 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072419\
Data File : FB021801.D
Signal(s) : FID2B.CH
Acq On : 24 Jul 2019 9:56
Operator : DD/AJ
Sample : BSF0724S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 25 01:04:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

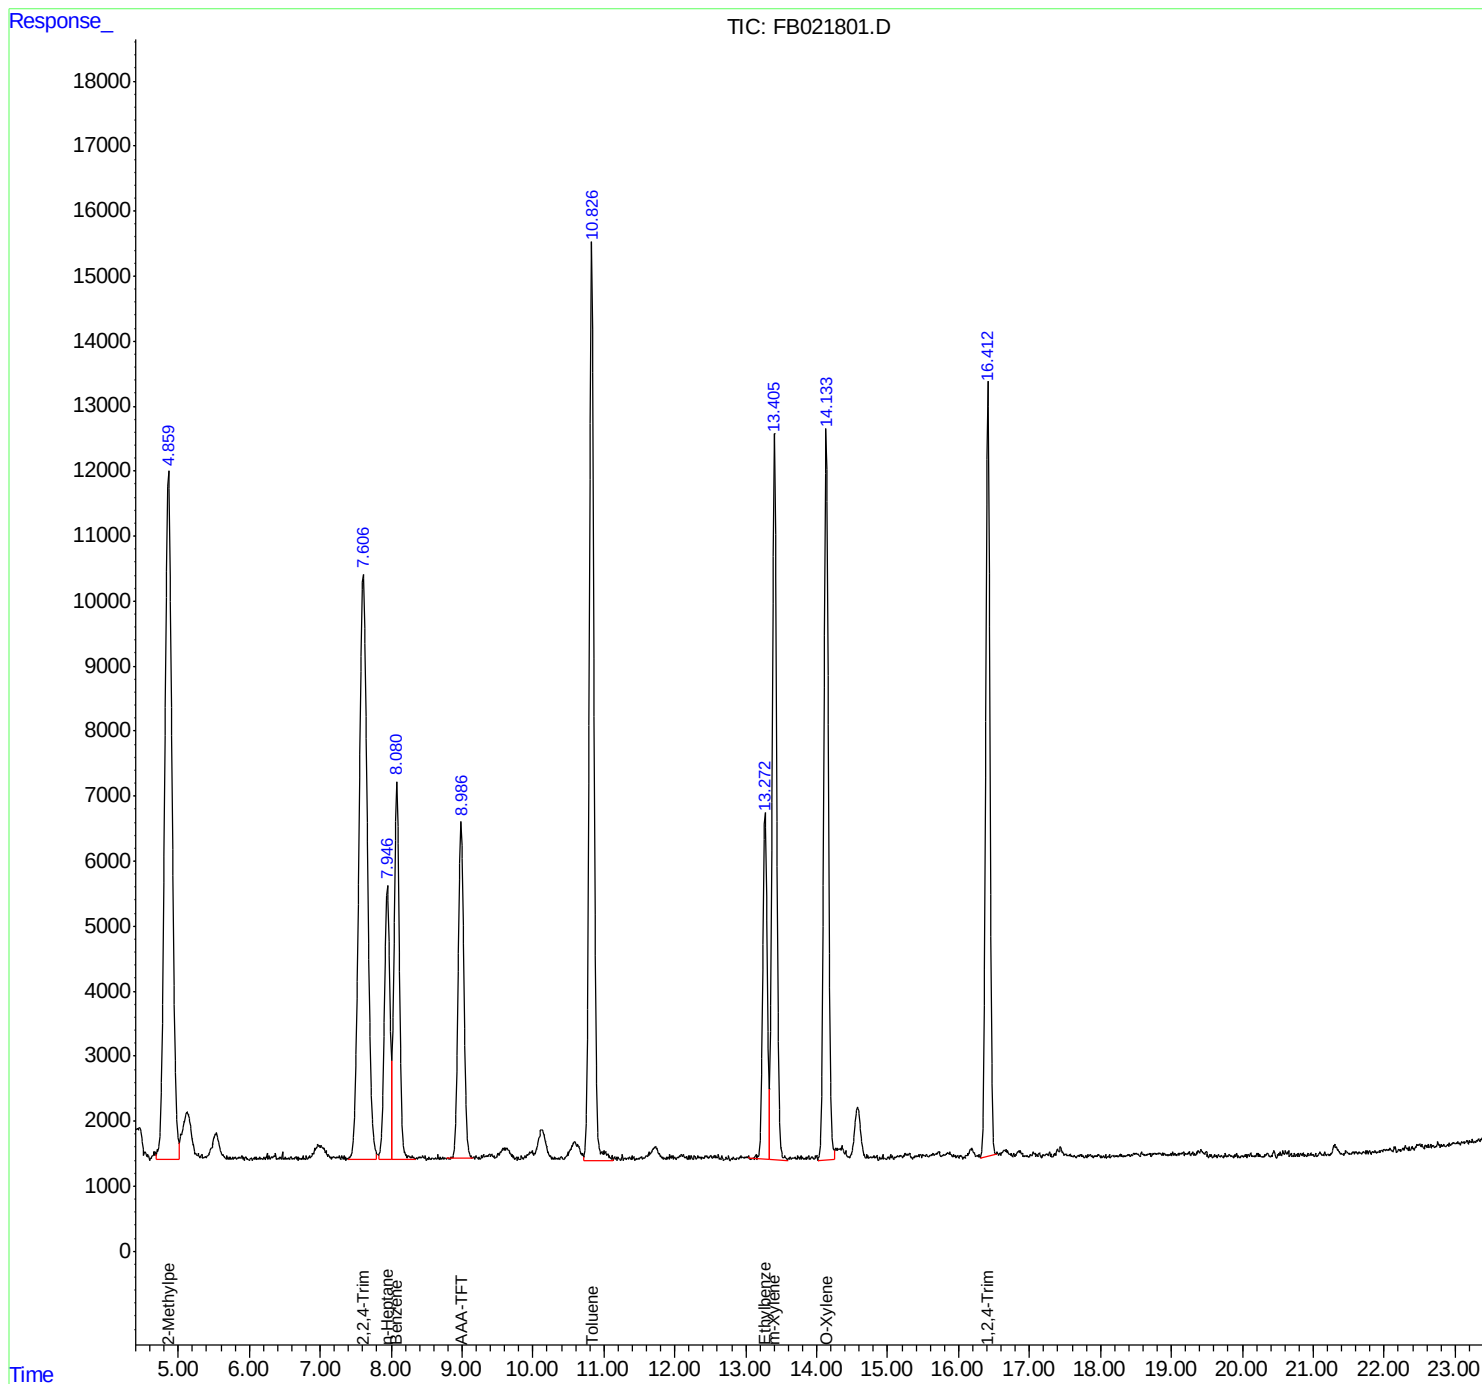

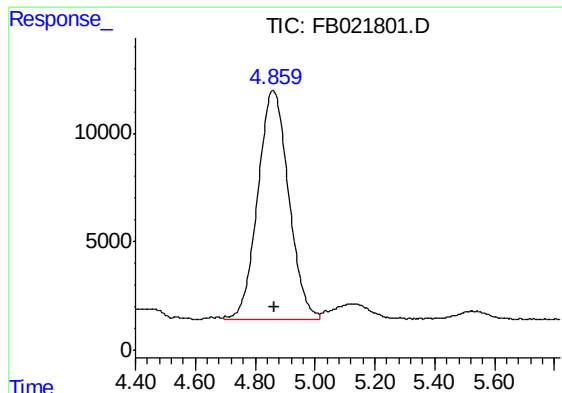


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 757841
Conc: 27.48 ng/ml

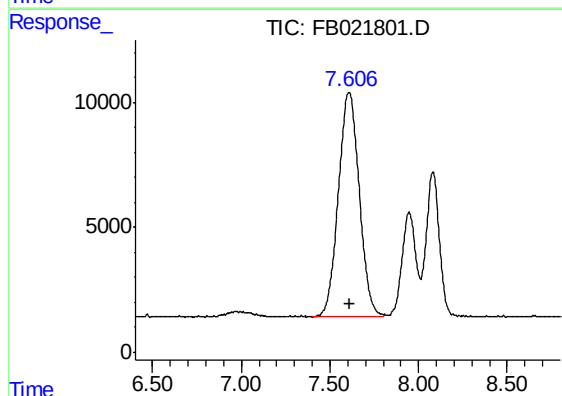


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: -0.005 min
Response: 738550
Conc: 27.94 ng/ml

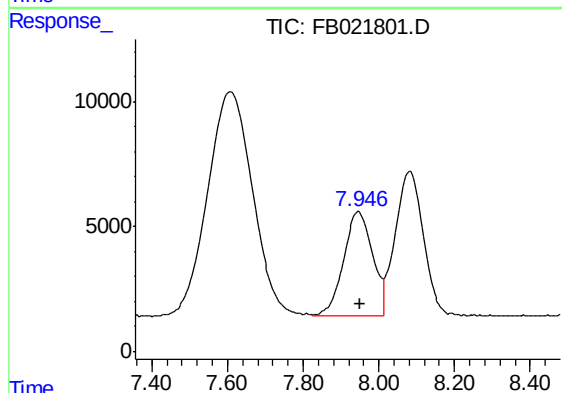


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: -0.004 min
Response: 226097
Conc: 9.12 ng/ml

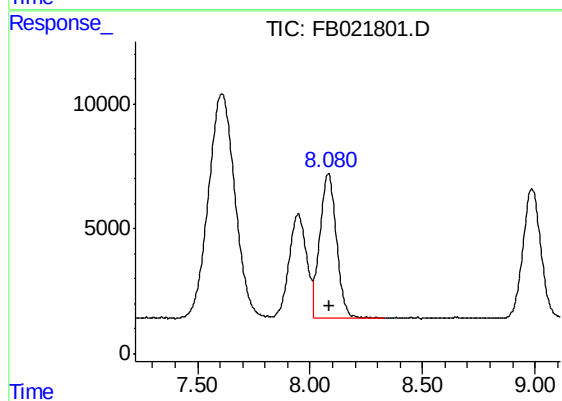


#4 Benzene

R.T.: 8.081 min
Delta R.T.: -0.005 min
Response: 302779
Conc: 10.36 ng/ml

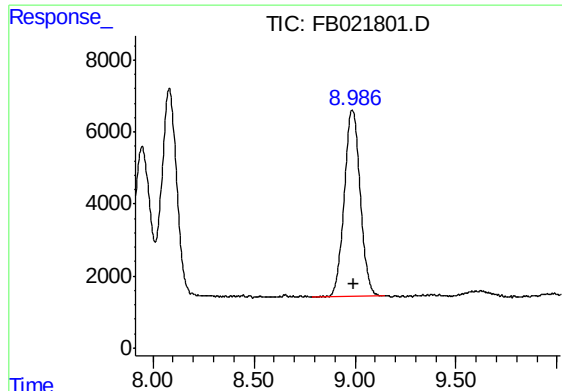


#5 AAA-TFT

R.T.: 8.987 min
Delta R.T.: -0.005 min
Response: 283958
Conc: 20.81 ng/ml

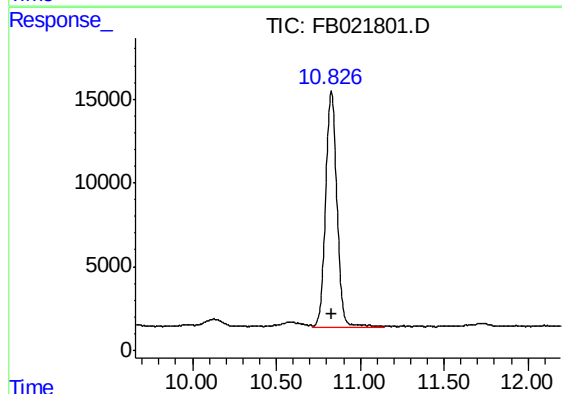


#6 Toluene

R.T.: 10.828 min
Delta R.T.: -0.005 min
Response: 658348
Conc: 32.00 ng/ml

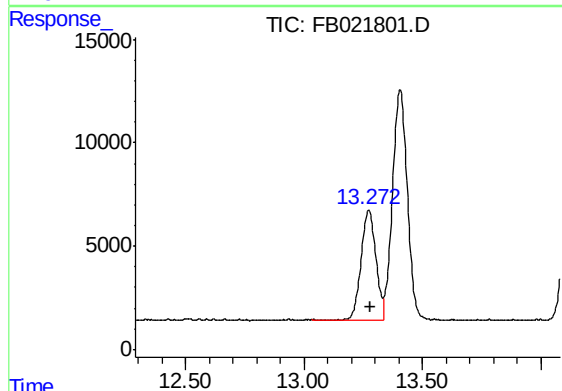


#7 Ethylbenzene

R.T.: 13.273 min
Delta R.T.: -0.005 min
Response: 230212
Conc: 11.07 ng/ml

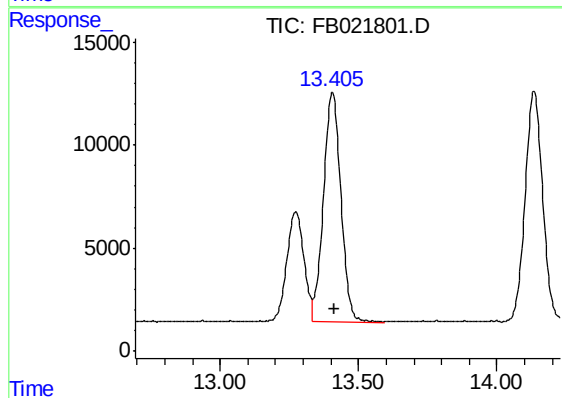


#8 m-Xylene

R.T.: 13.406 min
Delta R.T.: -0.005 min
Response: 491680
Conc: 22.13 ng/ml

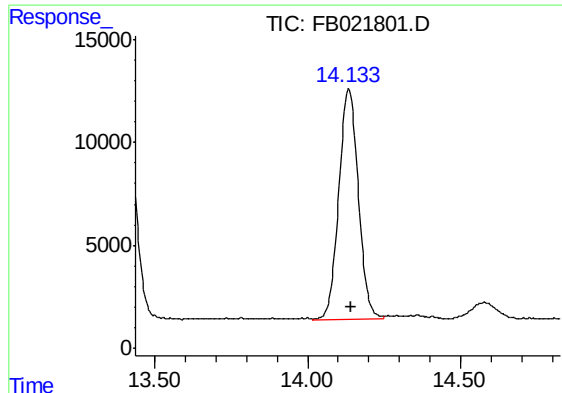

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: -0.006 min
Response: 495631
Conc: 21.55 ng/ml

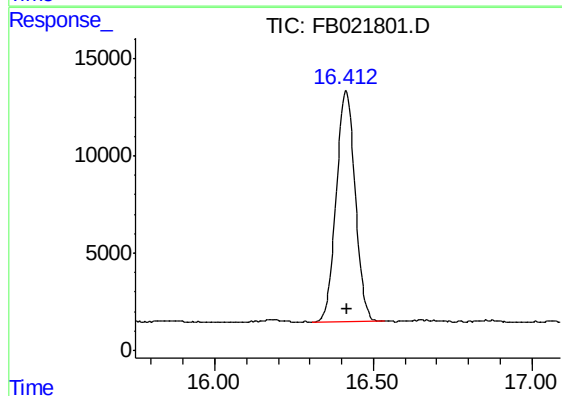

#10 1,2,4-Trimethylbenzene

R.T.: 16.414 min
Delta R.T.: -0.005 min
Response: 492588
Conc: 20.89 ng/ml