

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072419\
 Data File : FB021803.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jul 2019 10:57
 Operator : DD/AJ
 Sample : K3618-07MS
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 25 01:05:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.988	296498	21.727 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	650383	23.585 ng/ml
2) t 2,2,4-Trimethylpentane	7.607	619789	23.446 ng/ml
3) t n-Heptane	7.944	192140	7.749 ng/ml
4) t Benzene	8.081	288796	9.885 ng/ml
6) t Toluene	10.828	632649	30.746 ng/ml
7) t Ethylbenzene	13.274	225479	10.838 ng/ml
8) t m-Xylene	13.406	472394	21.264 ng/ml
9) t O-Xylene	14.135	477588	20.762 ng/ml
10) t 1,2,4-Trimethylbenzene	16.415	461282	19.565 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072419\
Data File : FB021803.D
Signal(s) : FID2B.CH
Acq On : 24 Jul 2019 10:57
Operator : DD/AJ
Sample : K3618-07MS
Misc : 5.02/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 25 01:05:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

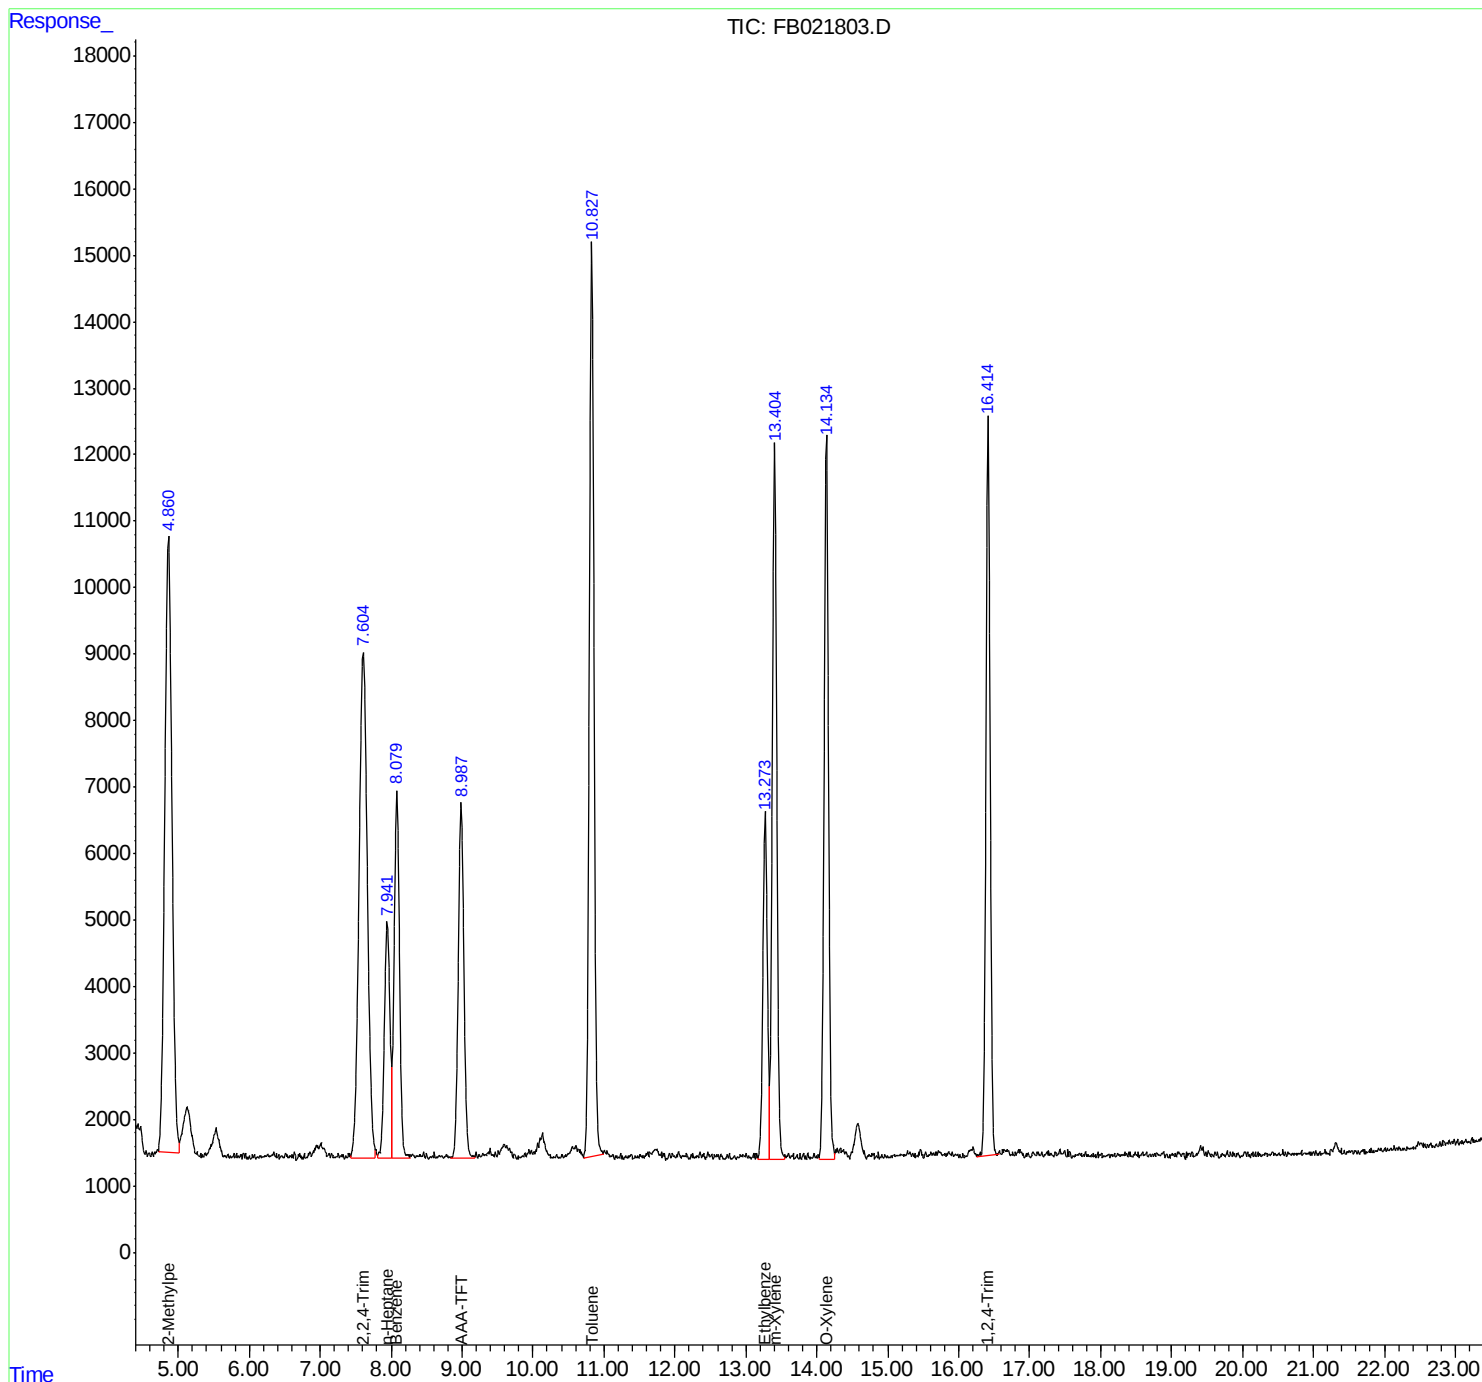

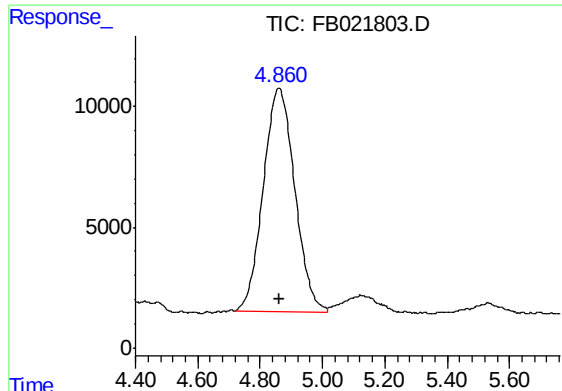


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 650383
Conc: 23.59 ng/ml

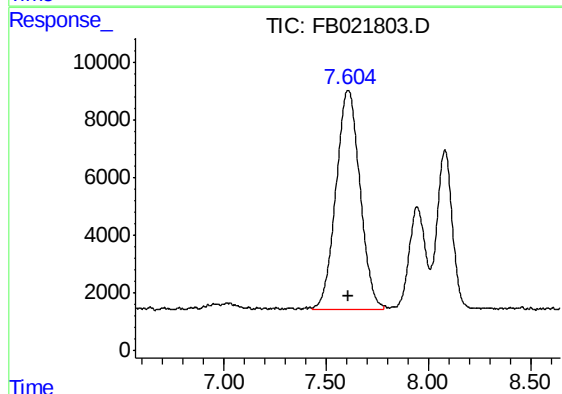


#2 2,2,4-Trimethylpentane

R.T.: 7.607 min
Delta R.T.: -0.005 min
Response: 619789
Conc: 23.45 ng/ml

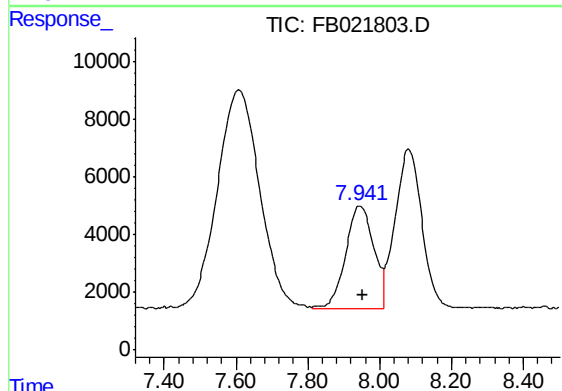


#3 n-Heptane

R.T.: 7.944 min
Delta R.T.: -0.007 min
Response: 192140
Conc: 7.75 ng/ml

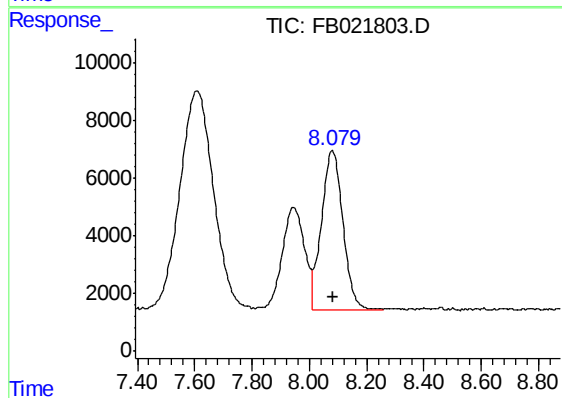


#4 Benzene

R.T.: 8.081 min
Delta R.T.: -0.005 min
Response: 288796
Conc: 9.89 ng/ml

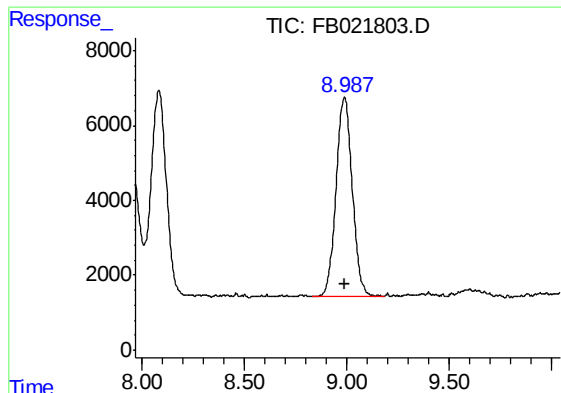


#5 AAA-TFT

R.T.: 8.988 min
Delta R.T.: -0.004 min
Response: 296498
Conc: 21.73 ng/ml

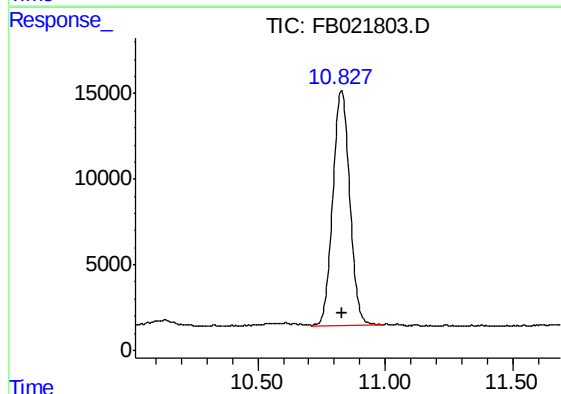


#6 Toluene

R.T.: 10.828 min
Delta R.T.: -0.005 min
Response: 632649
Conc: 30.75 ng/ml

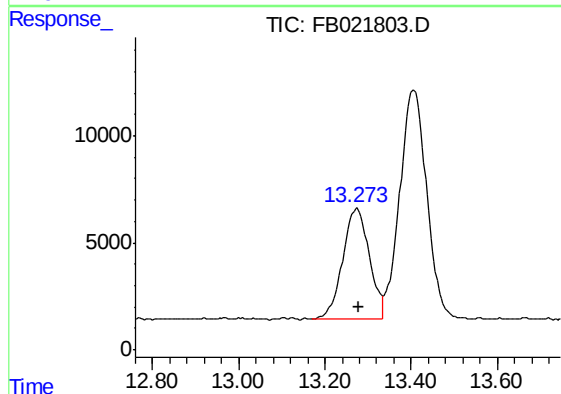


#7 Ethylbenzene

R.T.: 13.274 min
Delta R.T.: -0.004 min
Response: 225479
Conc: 10.84 ng/ml

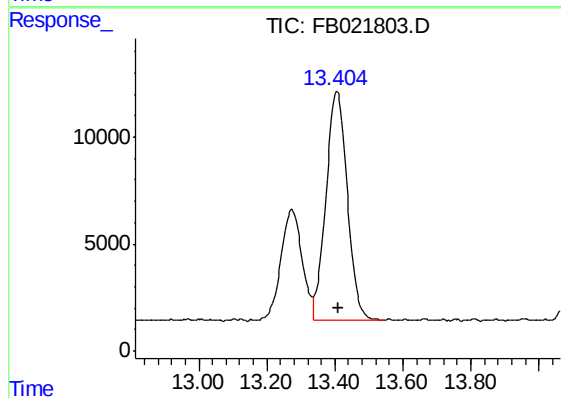


#8 m-Xylene

R.T.: 13.406 min
Delta R.T.: -0.005 min
Response: 472394
Conc: 21.26 ng/ml

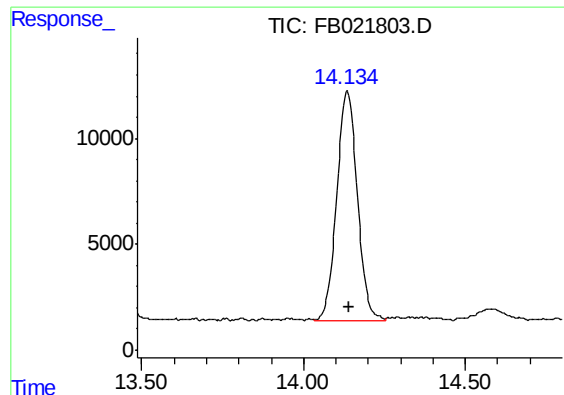

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: -0.005 min
Response: 477588
Conc: 20.76 ng/ml

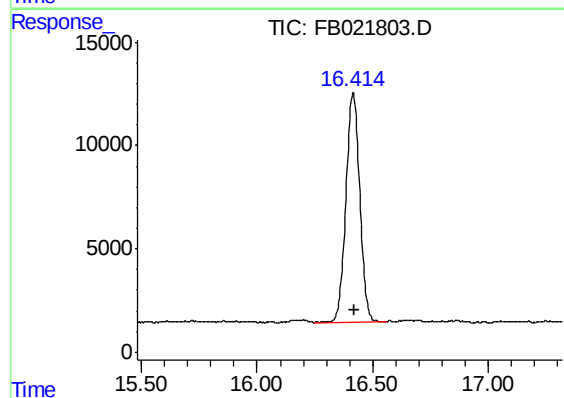

#10 1,2,4-Trimethylbenzene

R.T.: 16.415 min
Delta R.T.: -0.004 min
Response: 461282
Conc: 19.57 ng/ml