

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072419\
 Data File : FB021804.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jul 2019 11:28
 Operator : DD/AJ
 Sample : K3618-07MSD
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 25 01:05:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	314209	23.025 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.863	684669	24.828 ng/ml
2) t 2,2,4-Trimethylpentane	7.611	583368	22.069 ng/ml
3) t n-Heptane	7.949	184973	7.460 ng/ml
4) t Benzene	8.082	308339	10.554 ng/ml
6) t Toluene	10.830	632711	30.749 ng/ml
7) t Ethylbenzene	13.275	219213	10.537 ng/ml
8) t m-Xylene	13.407	460173	20.714 ng/ml
9) t O-Xylene	14.137	471649	20.504 ng/ml
10) t 1,2,4-Trimethylbenzene	16.416	449718	19.075 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072419\
Data File : FB021804.D
Signal(s) : FID2B.CH
Acq On : 24 Jul 2019 11:28
Operator : DD/AJ
Sample : K3618-07MSD
Misc : 5.03/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 25 01:05:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

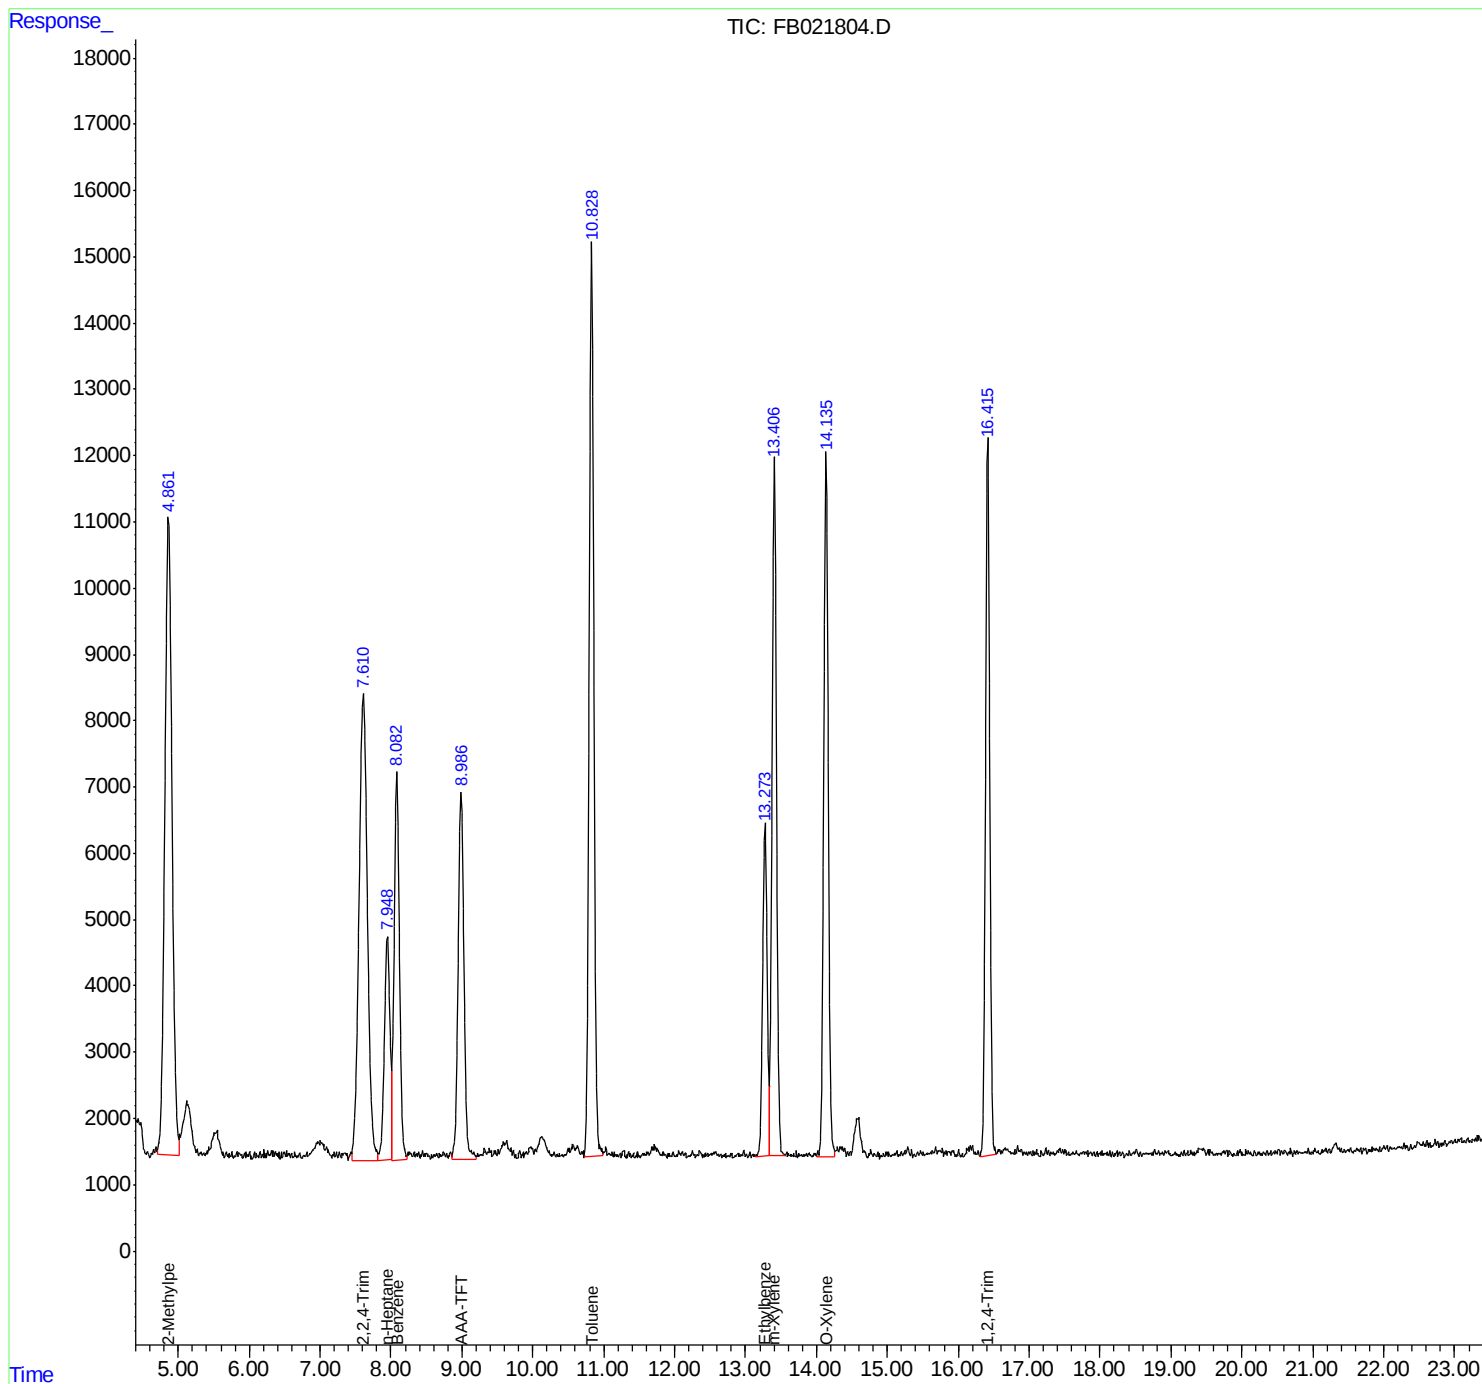

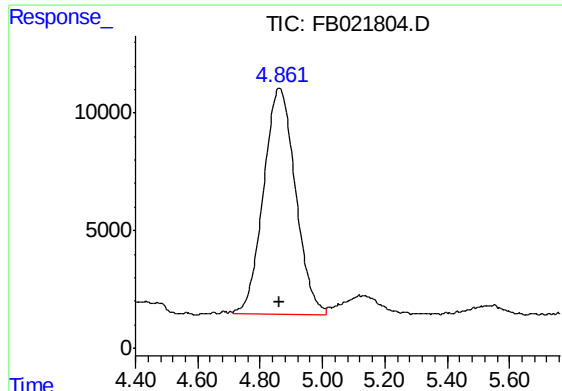


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 684669
Conc: 24.83 ng/ml

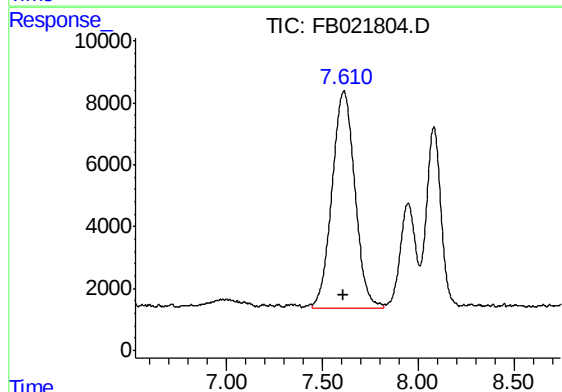


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.001 min
Response: 583368
Conc: 22.07 ng/ml

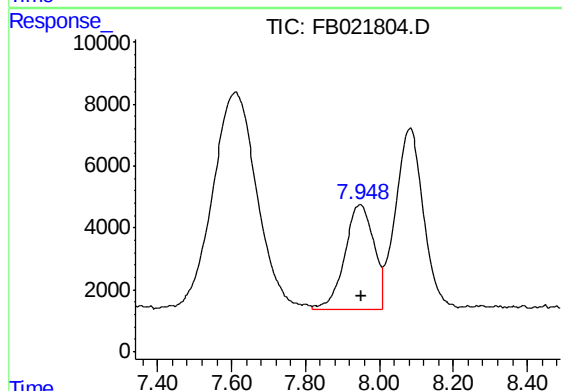


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.003 min
Response: 184973
Conc: 7.46 ng/ml

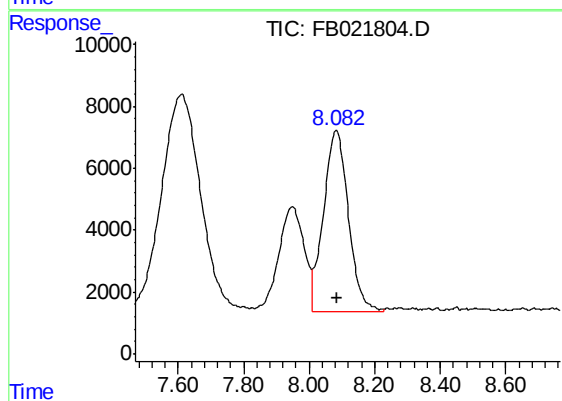


#4 Benzene

R.T.: 8.082 min
Delta R.T.: -0.003 min
Response: 308339
Conc: 10.55 ng/ml

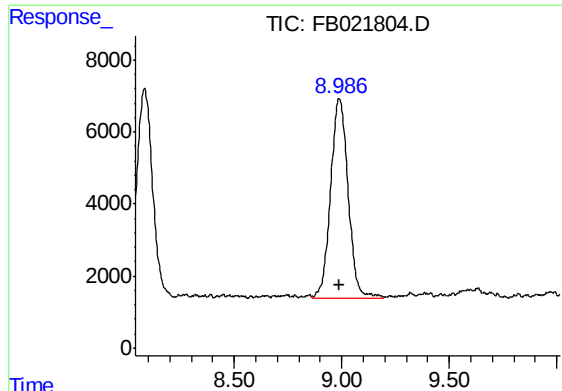


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.004 min
Response: 314209
Conc: 23.02 ng/ml

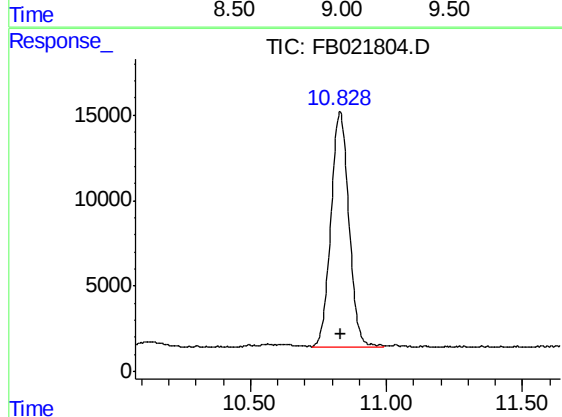


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.004 min
Response: 632711
Conc: 30.75 ng/ml

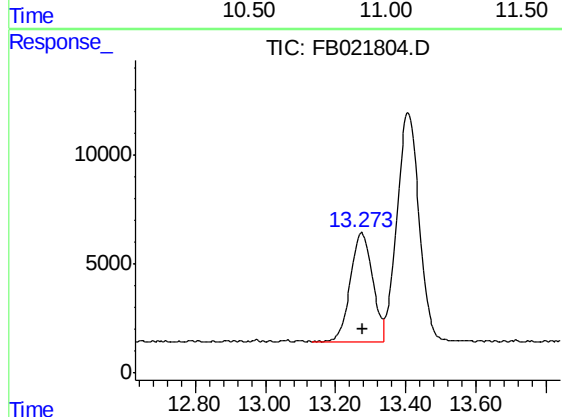


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: -0.003 min
Response: 219213
Conc: 10.54 ng/ml

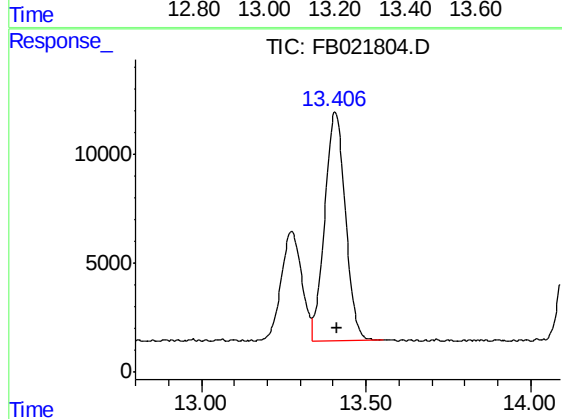


#8 m-Xylene

R.T.: 13.407 min
Delta R.T.: -0.004 min
Response: 460173
Conc: 20.71 ng/ml

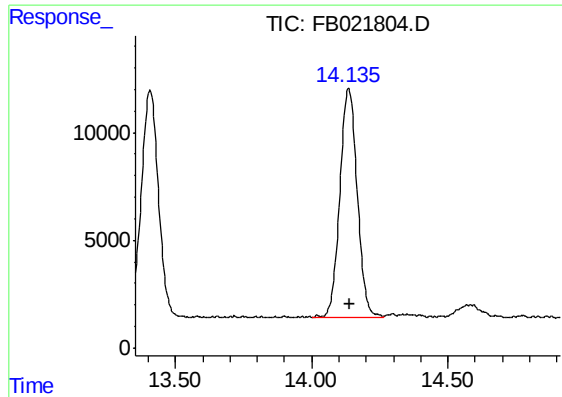

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: -0.004 min
Response: 471649
Conc: 20.50 ng/ml

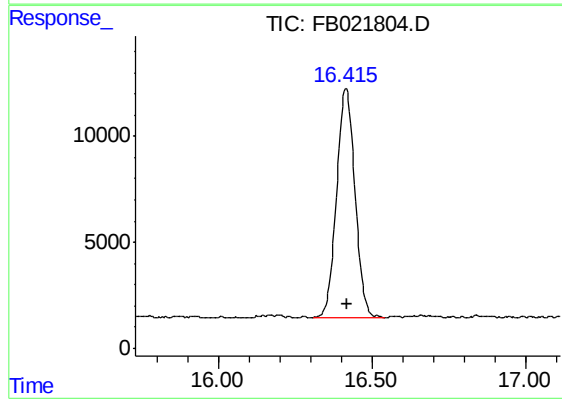

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: -0.004 min
Response: 449718
Conc: 19.07 ng/ml