

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072423\
 Data File : FB030193.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jul 2023 17:50
 Operator : YP/AJ
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 24 17:57:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Mon Jul 24 17:24:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.793	612743	59.990 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.710	1244667	80.852 ng/ml
2) t	2,2,4-Trimethylpentane	7.422	1421990	83.436 ng/ml
3) t	n-Heptane	7.752	484687	27.378 ng/ml
4) t	Benzene	7.888	592881	27.028 ng/ml
6) t	Toluene	10.621	1734117	82.228 ng/ml
7) t	Ethylbenzene	13.057	541459	27.361 ng/ml
8) t	m-Xylene	13.190	1053767	54.053 ng/ml
9) t	O-Xylene	13.916	1002422	53.713 ng/ml
10) t	1,2,4-Trimethylbenzene	16.191	918854	52.682 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072423\
Data File : FB030193.D
Signal(s) : FID2B.CH
Acq On : 24 Jul 2023 17:50
Operator : YP/AJ
Sample : 50 GRO STD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 24 17:57:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Mon Jul 24 17:24:10 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

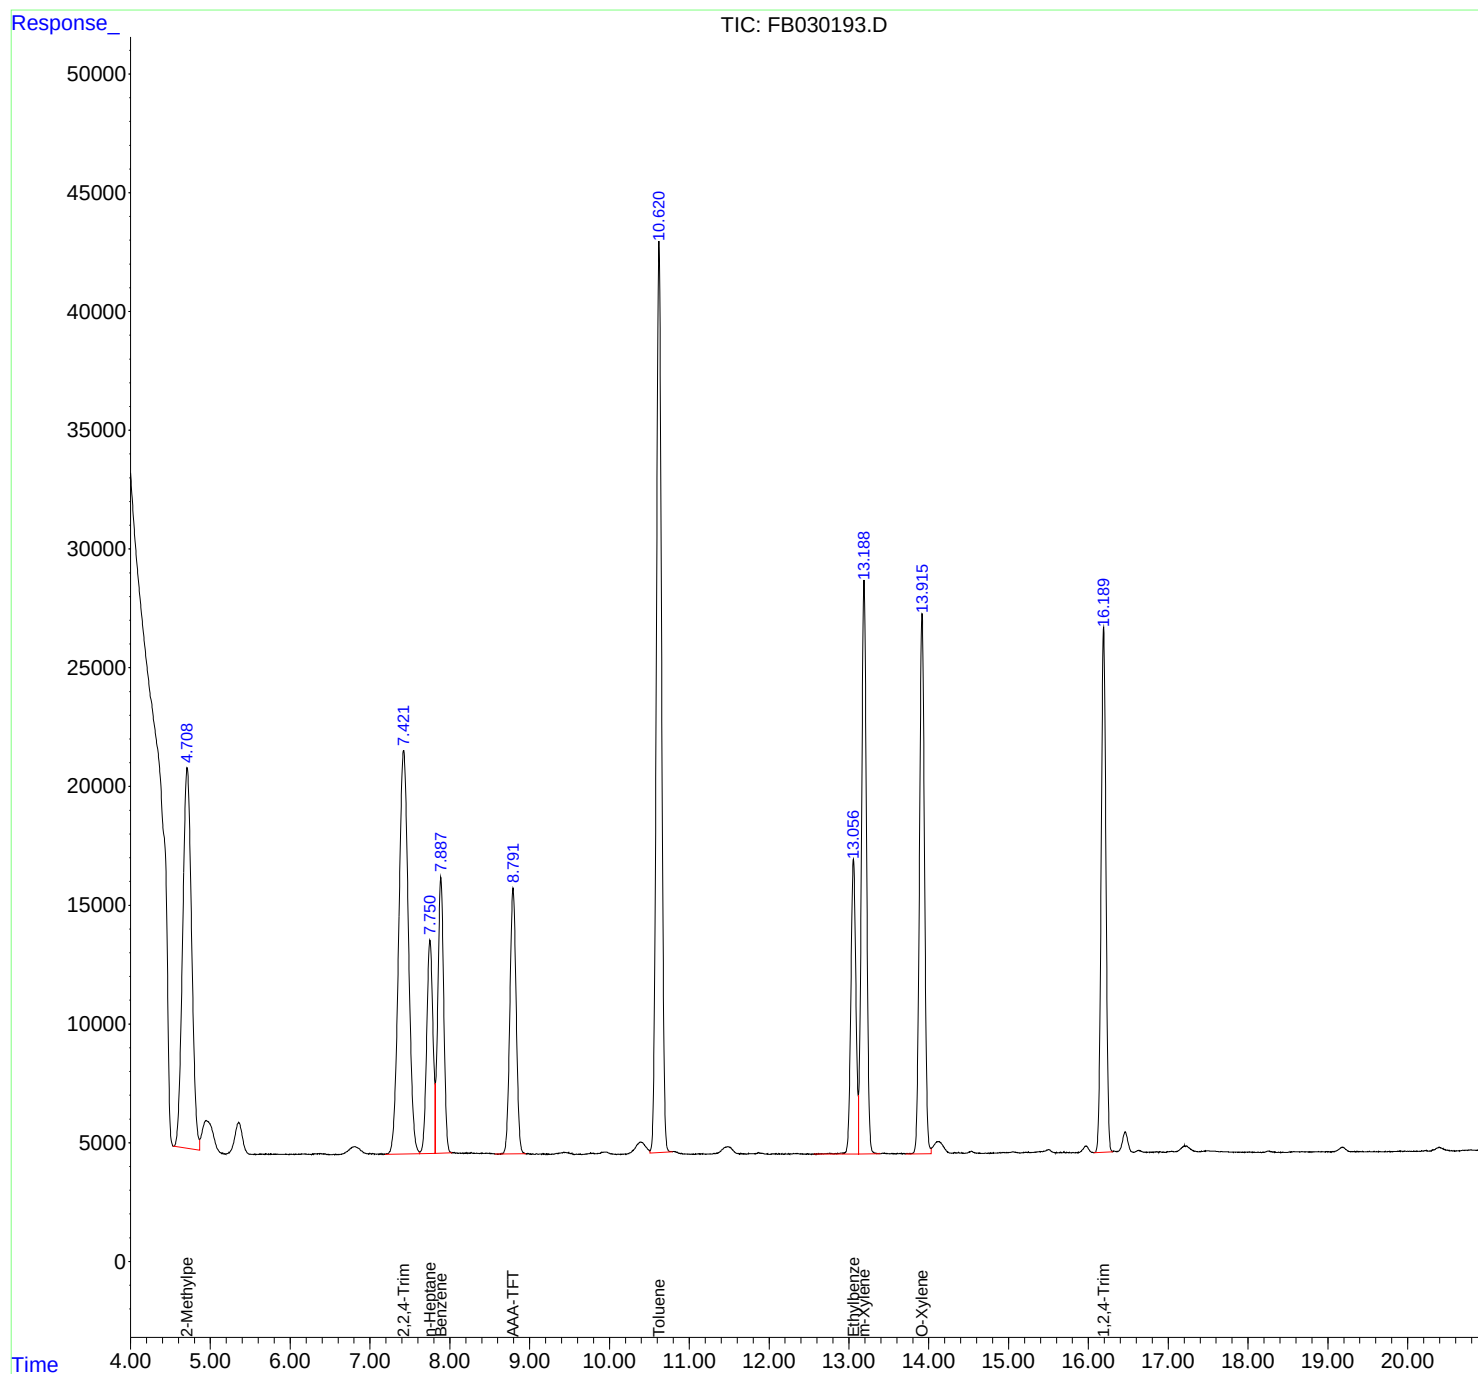

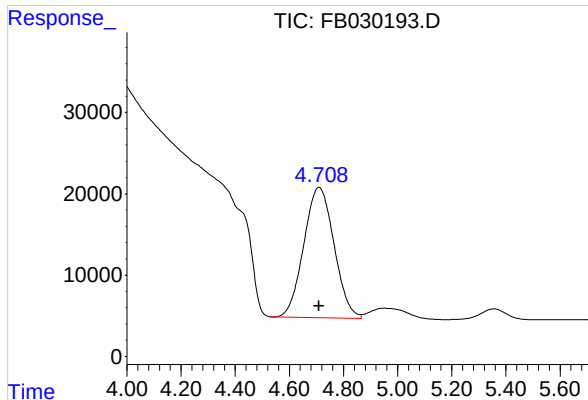


#1 2-Methylpentane

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 1244667
Conc: 80.85 ng/ml

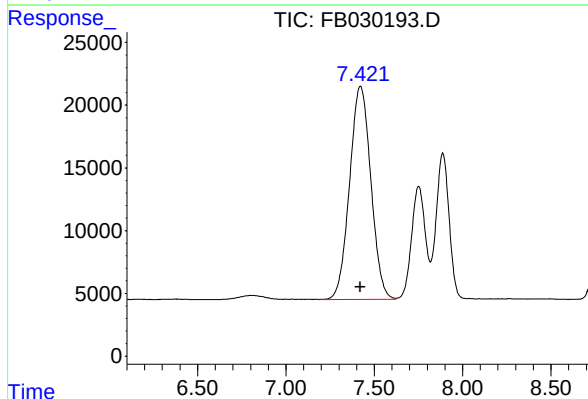


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 1421990
Conc: 83.44 ng/ml

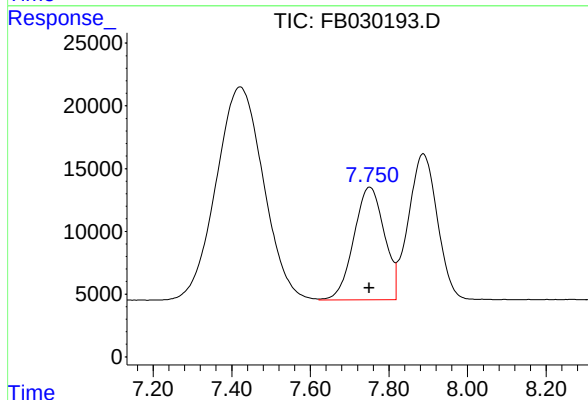


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.001 min
Response: 484687
Conc: 27.38 ng/ml

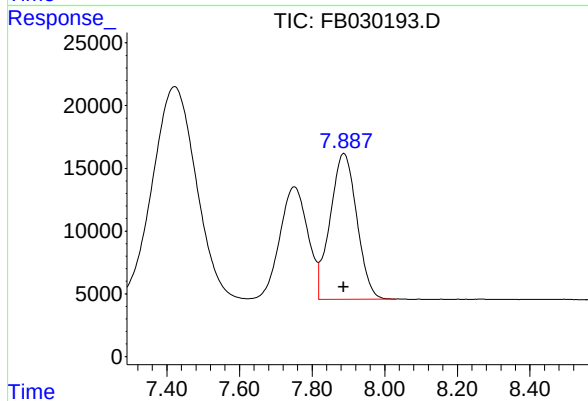


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 592881
Conc: 27.03 ng/ml

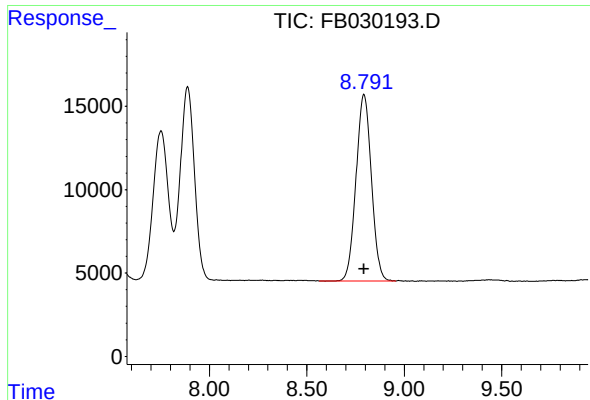


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 612743
Conc: 59.99 ng/ml

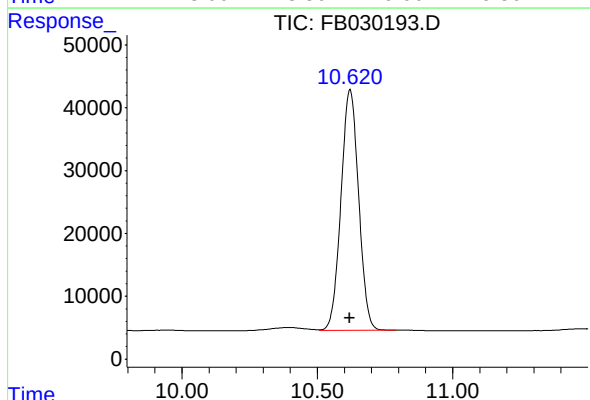


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 1734117
Conc: 82.23 ng/ml

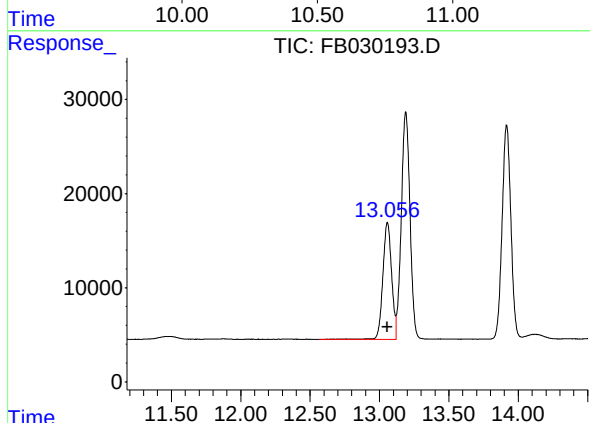


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 541459
Conc: 27.36 ng/ml

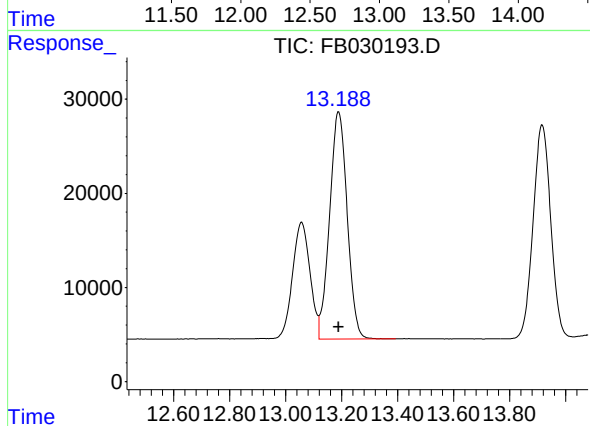


#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 1053767
Conc: 54.05 ng/ml

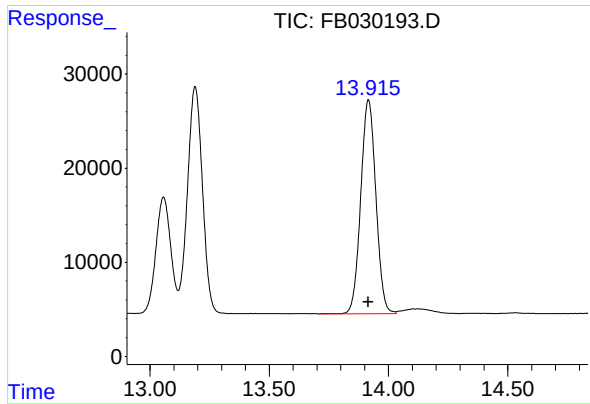

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 1002422
Conc: 53.71 ng/ml

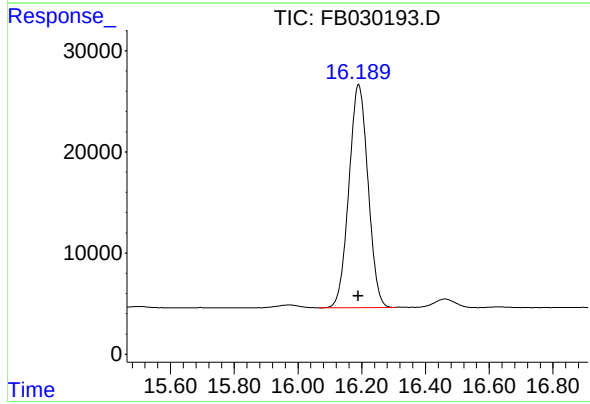

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 918854
Conc: 52.68 ng/ml