

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072424\
 Data File : FB030824.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jul 2024 12:44
 Operator : YP/AJ
 Sample : BSF0724S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0724S1

Integration File: Calibration.e
 Quant Time: Jul 25 03:15:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070324.M
 Quant Title :
 QLast Update : Wed Jul 03 12:25:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	230937	21.634 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	478375	27.671 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	483119	27.849 ng/ml
3) t n-Heptane	7.747	173213	9.039 ng/ml
4) t Benzene	7.883	208591	9.351 ng/ml
6) t Toluene	10.615	605988	28.032 ng/ml
7) t Ethylbenzene	13.052	189348	9.503 ng/ml
8) t m-Xylene	13.184	376318	18.839 ng/ml
9) t O-Xylene	13.911	364189	19.049 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	360062	18.371 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072424\
Data File : FB030824.D
Signal(s) : FID2B.CH
Acq On : 24 Jul 2024 12:44
Operator : YP/AJ
Sample : BSF0724S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0724S1

Integration File: Calibration.e
Quant Time: Jul 25 03:15:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070324.M
Quant Title :
QLast Update : Wed Jul 03 12:25:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

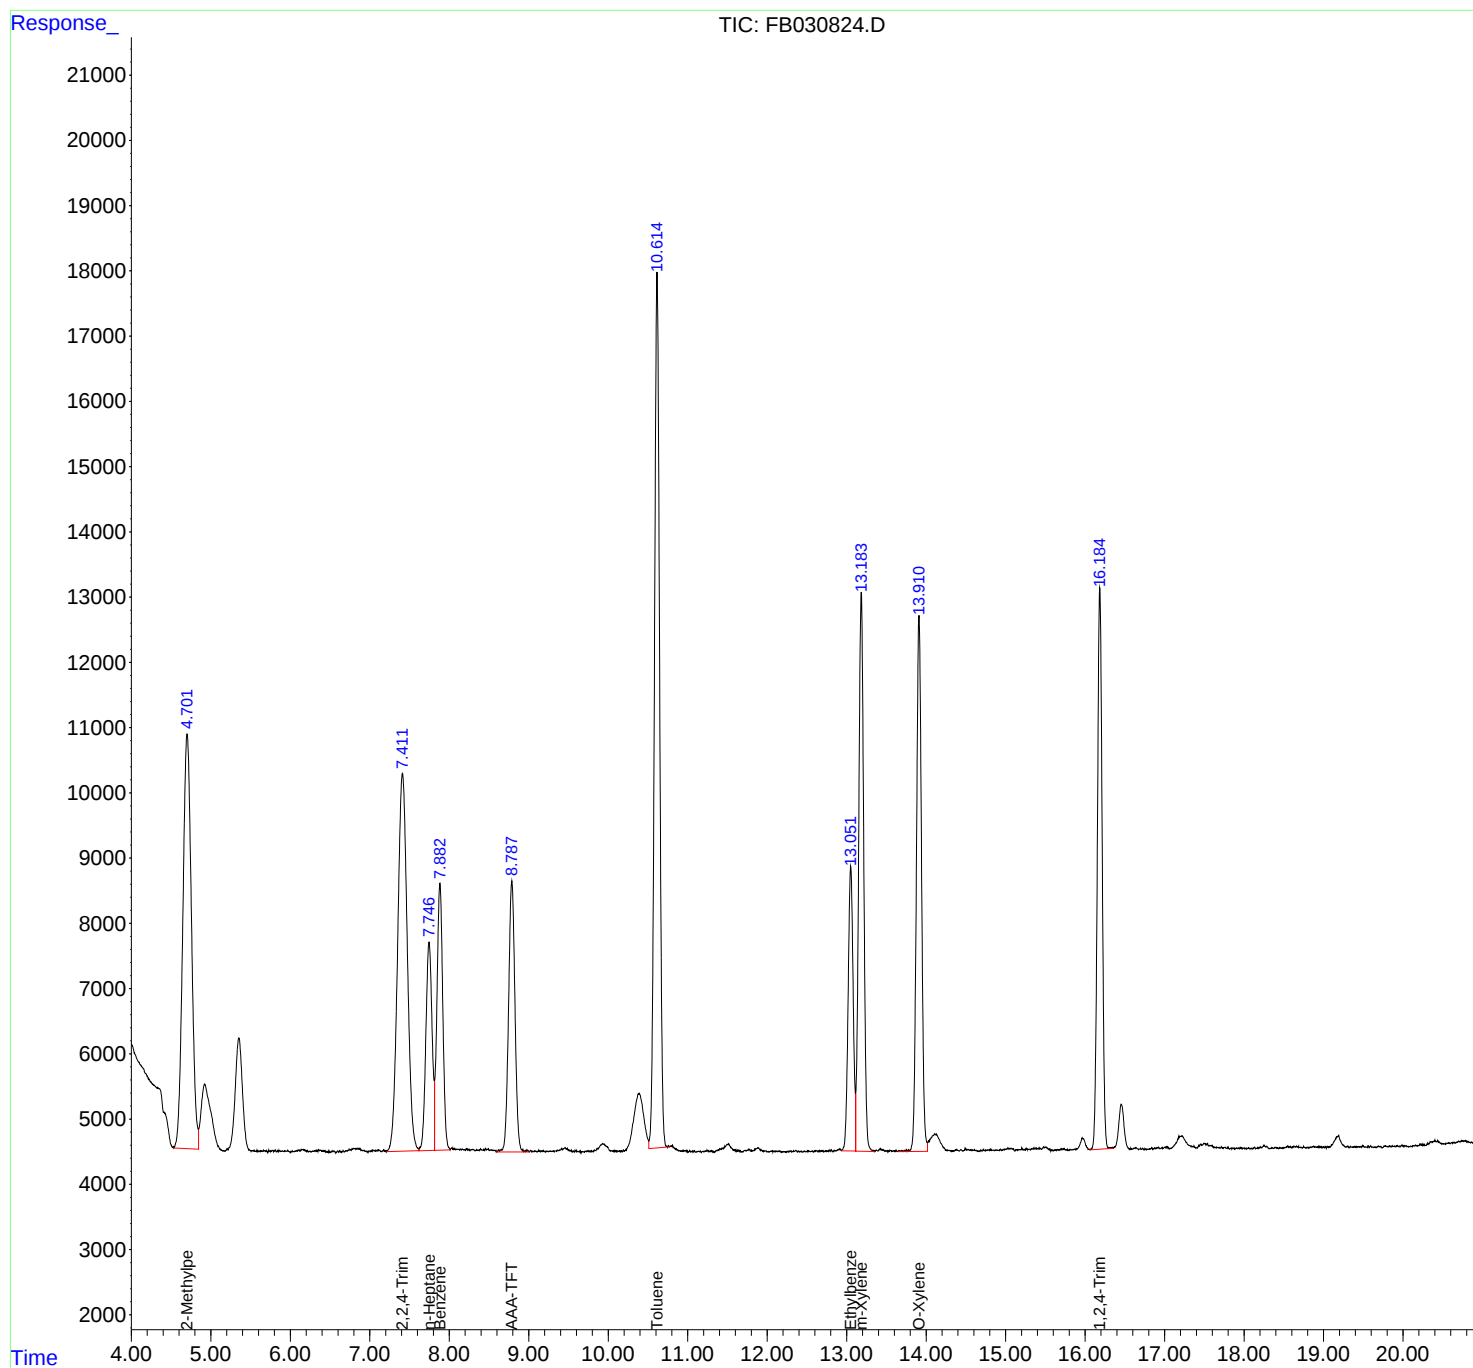


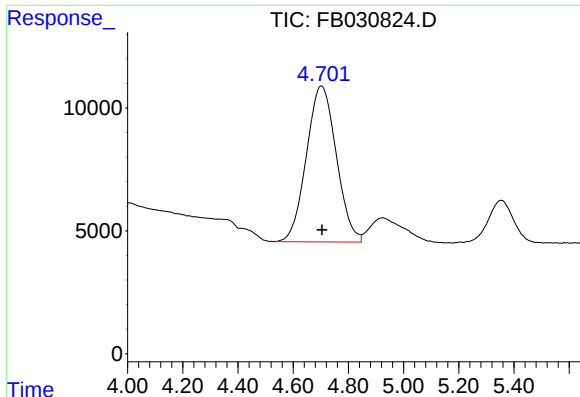

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.003 min
Response: 478375
Conc: 27.67 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0724S1

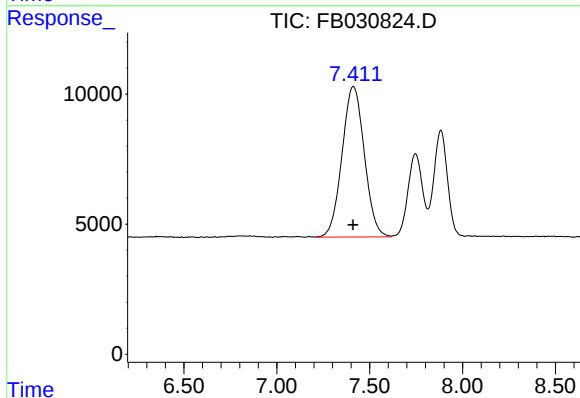


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: 0.000 min
Response: 483119
Conc: 27.85 ng/ml

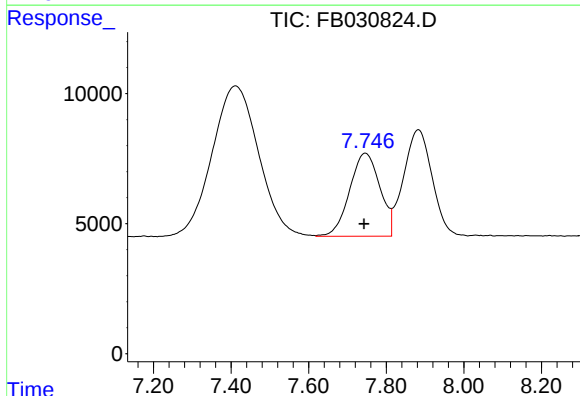


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.004 min
Response: 173213
Conc: 9.04 ng/ml

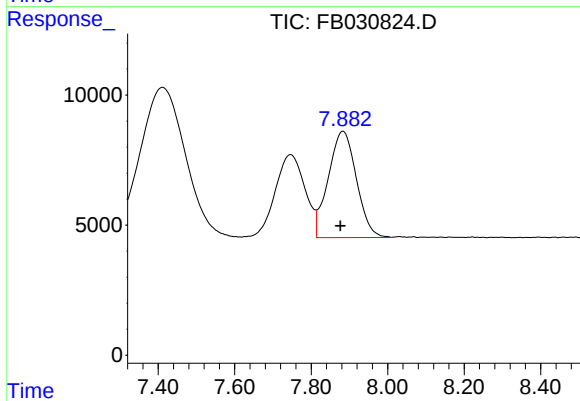

#4 Benzene


R.T.: 7.883 min
Delta R.T.: 0.007 min
Response: 208591
Conc: 9.35 ng/ml

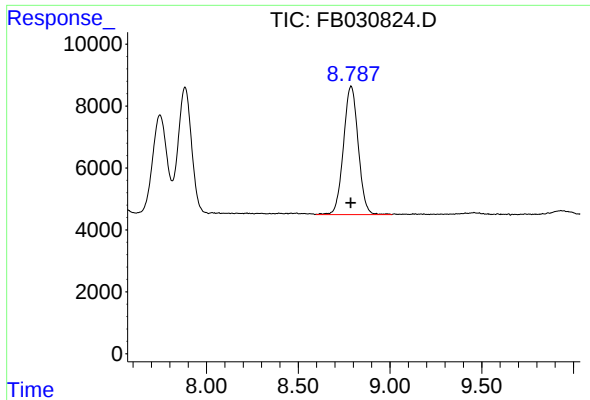

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.002 min
Response: 230937
Conc: 21.63 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0724S1

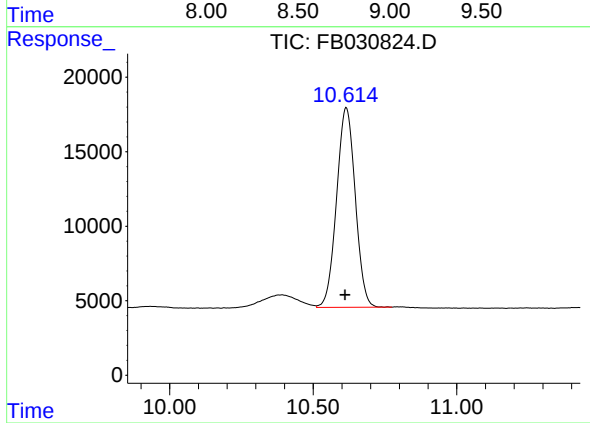


#6 Toluene

R.T.: 10.615 min
Delta R.T.: 0.004 min
Response: 605988
Conc: 28.03 ng/ml

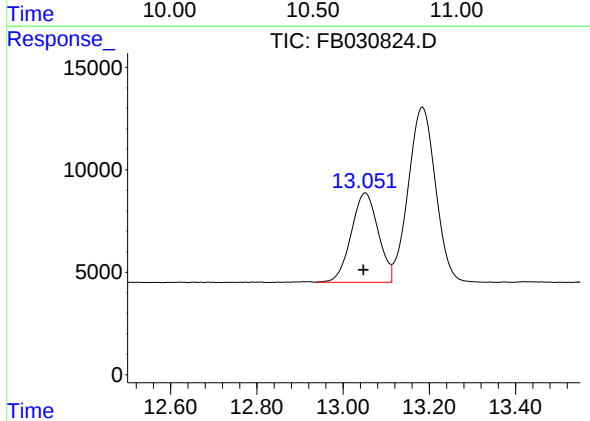


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: 0.004 min
Response: 189348
Conc: 9.50 ng/ml

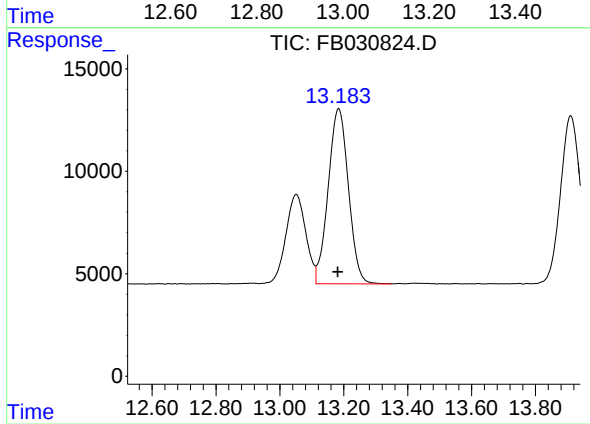

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: 0.003 min
Response: 376318
Conc: 18.84 ng/ml

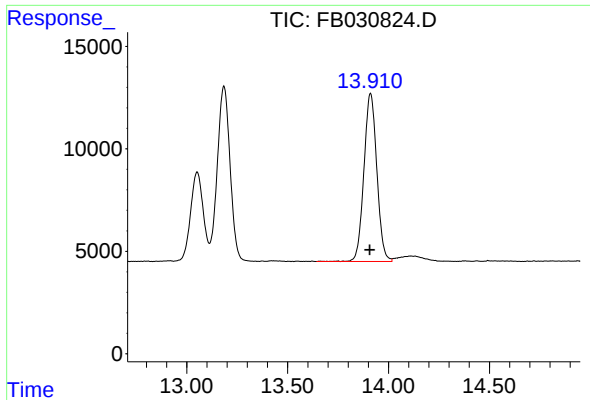

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: 0.004 min
Response: 364189
Conc: 19.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0724S1

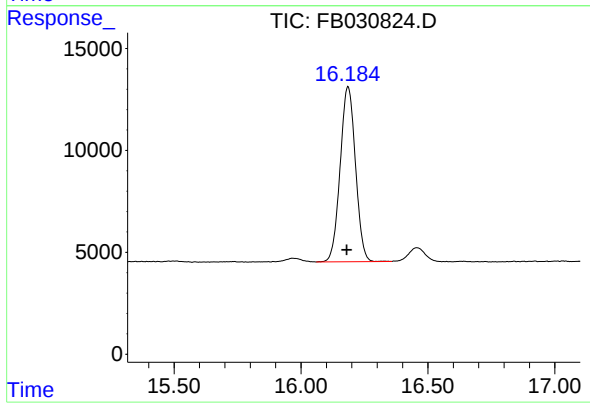

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: 0.005 min
Response: 360062
Conc: 18.37 ng/ml