

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072424\
 Data File : FB030827.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jul 2024 14:41
 Operator : YP/AJ
 Sample : P3341-01MS
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-05-072324MS

Integration File: Calibration.e
 Quant Time: Jul 25 03:16:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070324.M
 Quant Title :
 QLast Update : Wed Jul 03 12:25:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	255437	23.929 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	428318	24.776 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	485941	28.011 ng/ml
3) t n-Heptane	7.745	165196	8.621 ng/ml
4) t Benzene	7.882	218267	9.785 ng/ml
6) t Toluene	10.616	622637	28.802 ng/ml
7) t Ethylbenzene	13.053	192903	9.681 ng/ml
8) t m-Xylene	13.185	380291	19.038 ng/ml
9) t O-Xylene	13.912	371478	19.431 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	343479	17.525 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072424\
 Data File : FB030827.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jul 2024 14:41
 Operator : YP/AJ
 Sample : P3341-01MS
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-05-072324MS

Integration File: Calibration.e
 Quant Time: Jul 25 03:16:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070324.M
 Quant Title :
 QLast Update : Wed Jul 03 12:25:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

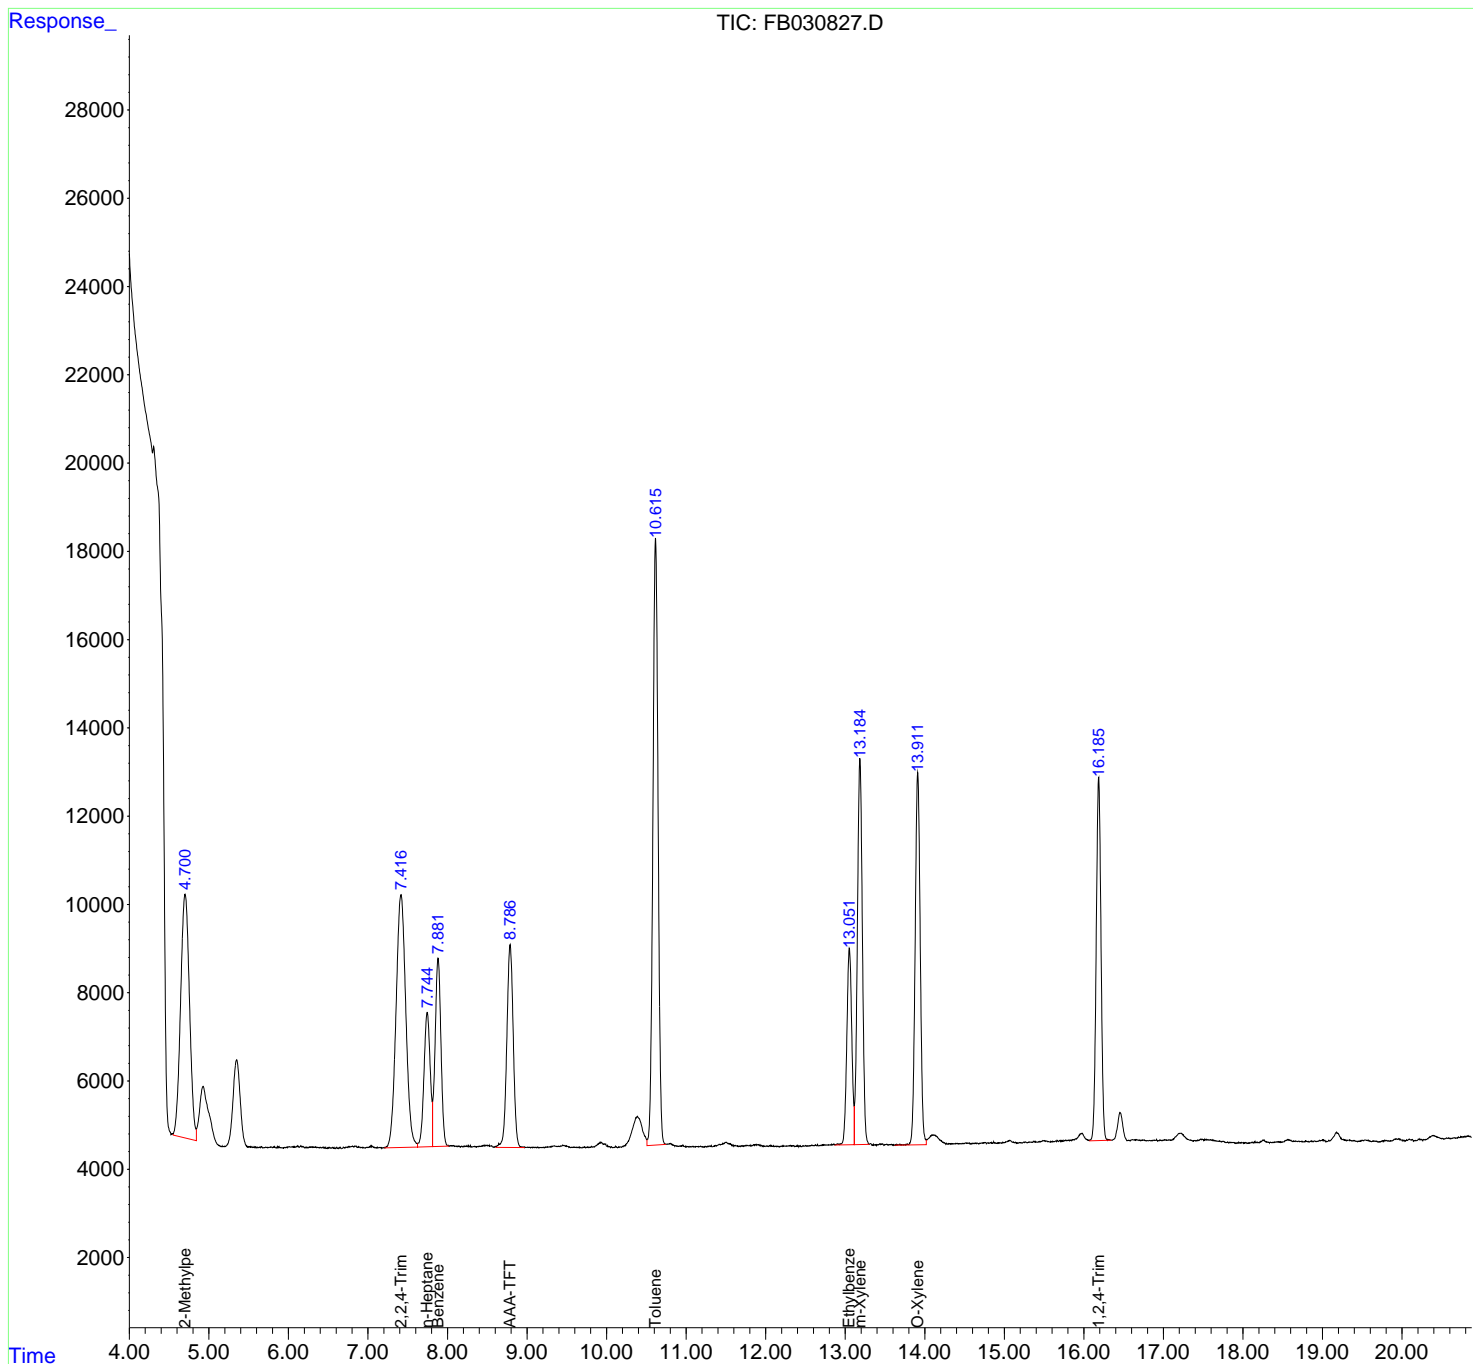


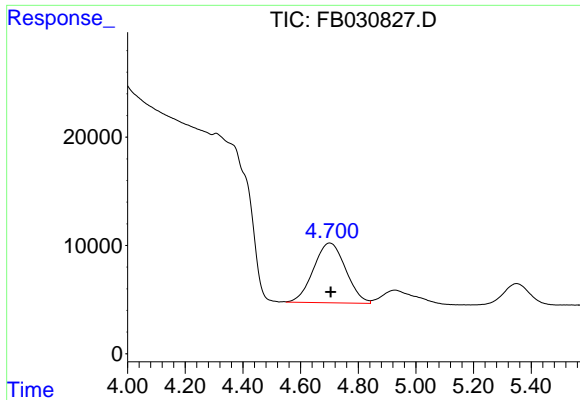

#1 2-Methylpentane


R.T.: 4.701 min
 Delta R.T.: -0.004 min
 Response: 428318
 Conc: 24.78 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 AU-05-072324MS

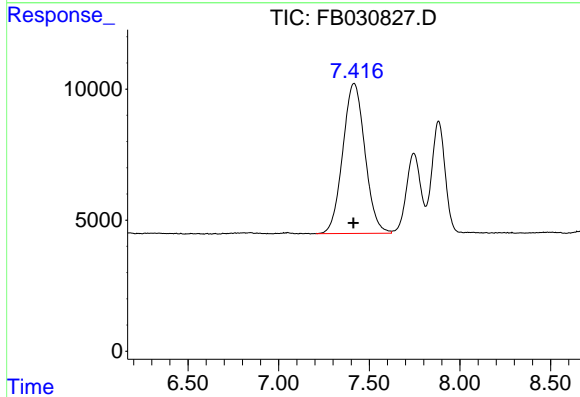


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
 Delta R.T.: 0.005 min
 Response: 485941
 Conc: 28.01 ng/ml

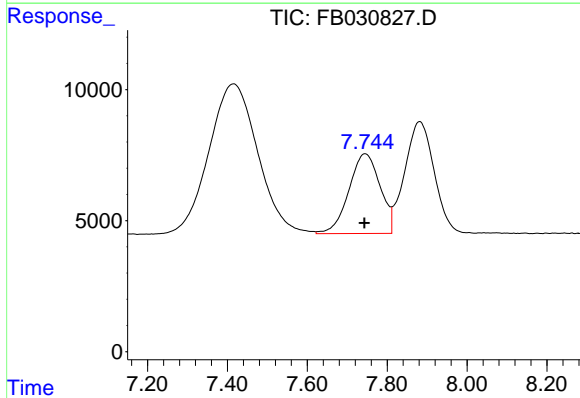


#3 n-Heptane

R.T.: 7.745 min
 Delta R.T.: 0.002 min
 Response: 165196
 Conc: 8.62 ng/ml

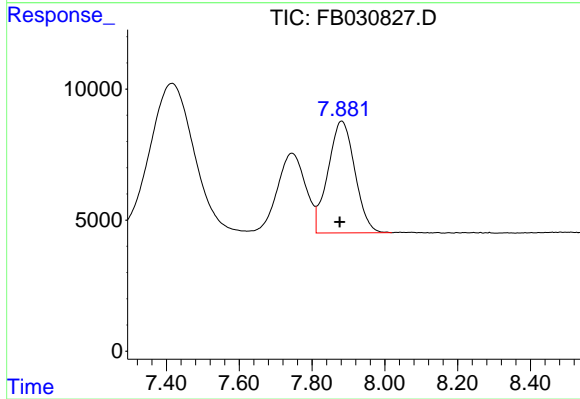

#4 Benzene


R.T.: 7.882 min
 Delta R.T.: 0.005 min
 Response: 218267
 Conc: 9.78 ng/ml

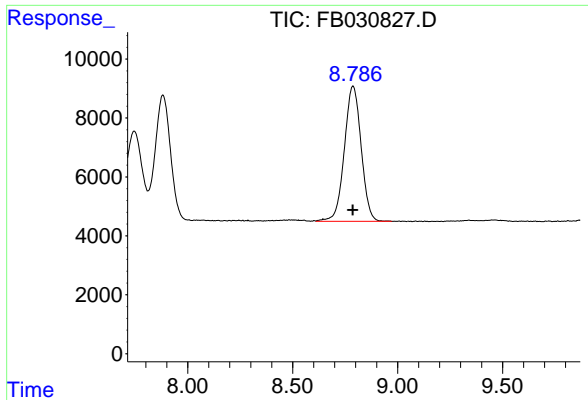

#5 AAA-TFT


R.T.: 8.788 min
 Delta R.T.: 0.001 min
 Response: 255437
 Conc: 23.93 ng/ml

Instrument : FID_B
 ClientSampleId : AU-05-072324MS

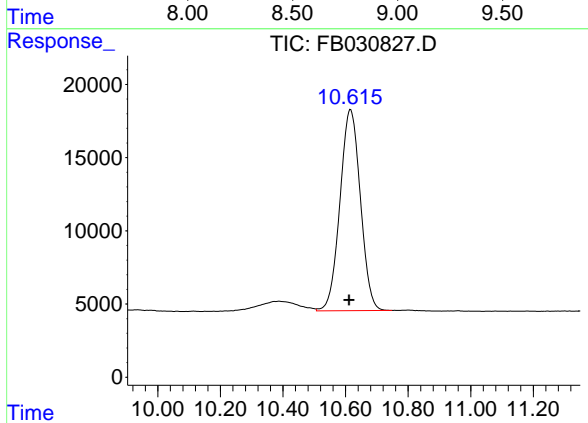


#6 Toluene

R.T.: 10.616 min
 Delta R.T.: 0.005 min
 Response: 622637
 Conc: 28.80 ng/ml

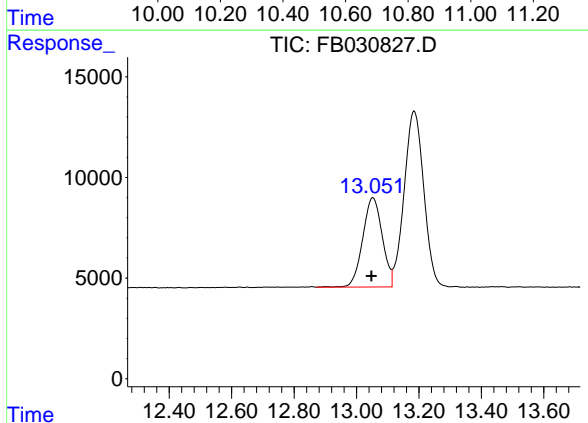


#7 Ethylbenzene

R.T.: 13.053 min
 Delta R.T.: 0.005 min
 Response: 192903
 Conc: 9.68 ng/ml

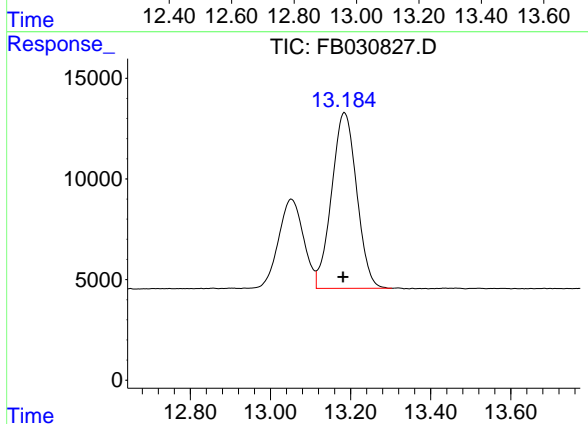


#8 m-Xylene

R.T.: 13.185 min
 Delta R.T.: 0.004 min
 Response: 380291
 Conc: 19.04 ng/ml

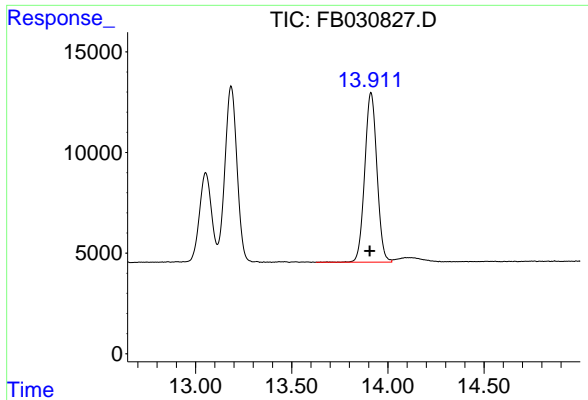

#9 O-Xylene
R.T.: 13.912 min
Delta R.T.: 0.005 min
Response: 371478
Conc: 19.43 ng/ml

Instrument : FID_B
ClientSampleId : AU-05-072324MS

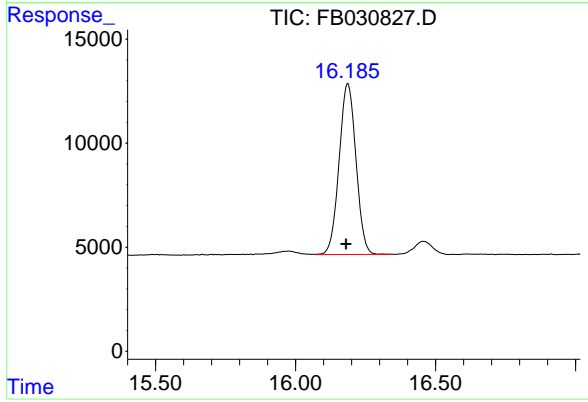

#10 1,2,4-Trimethylbenzene
R.T.: 16.187 min
Delta R.T.: 0.006 min
Response: 343479
Conc: 17.52 ng/ml