

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072424\
 Data File : FB030829.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jul 2024 16:00
 Operator : YP/AJ
 Sample : BSF0724S2
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0724S2

Integration File: Calibration.e
 Quant Time: Jul 25 03:16:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070324.M
 Quant Title :
 QLast Update : Wed Jul 03 12:25:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	221297	20.731 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	489468	28.313 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	521206	30.044 ng/ml
3) t n-Heptane	7.749	181656	9.480 ng/ml
4) t Benzene	7.885	223418	10.016 ng/ml
6) t Toluene	10.618	644016	29.791 ng/ml
7) t Ethylbenzene	13.054	201276	10.101 ng/ml
8) t m-Xylene	13.187	401957	20.122 ng/ml
9) t O-Xylene	13.913	391684	20.488 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	376142	19.191 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072424\
Data File : FB030829.D
Signal(s) : FID2B.CH
Acq On : 24 Jul 2024 16:00
Operator : YP/AJ
Sample : BSF0724S2
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0724S2

Integration File: Calibration.e
Quant Time: Jul 25 03:16:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070324.M
Quant Title :
QLast Update : Wed Jul 03 12:25:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

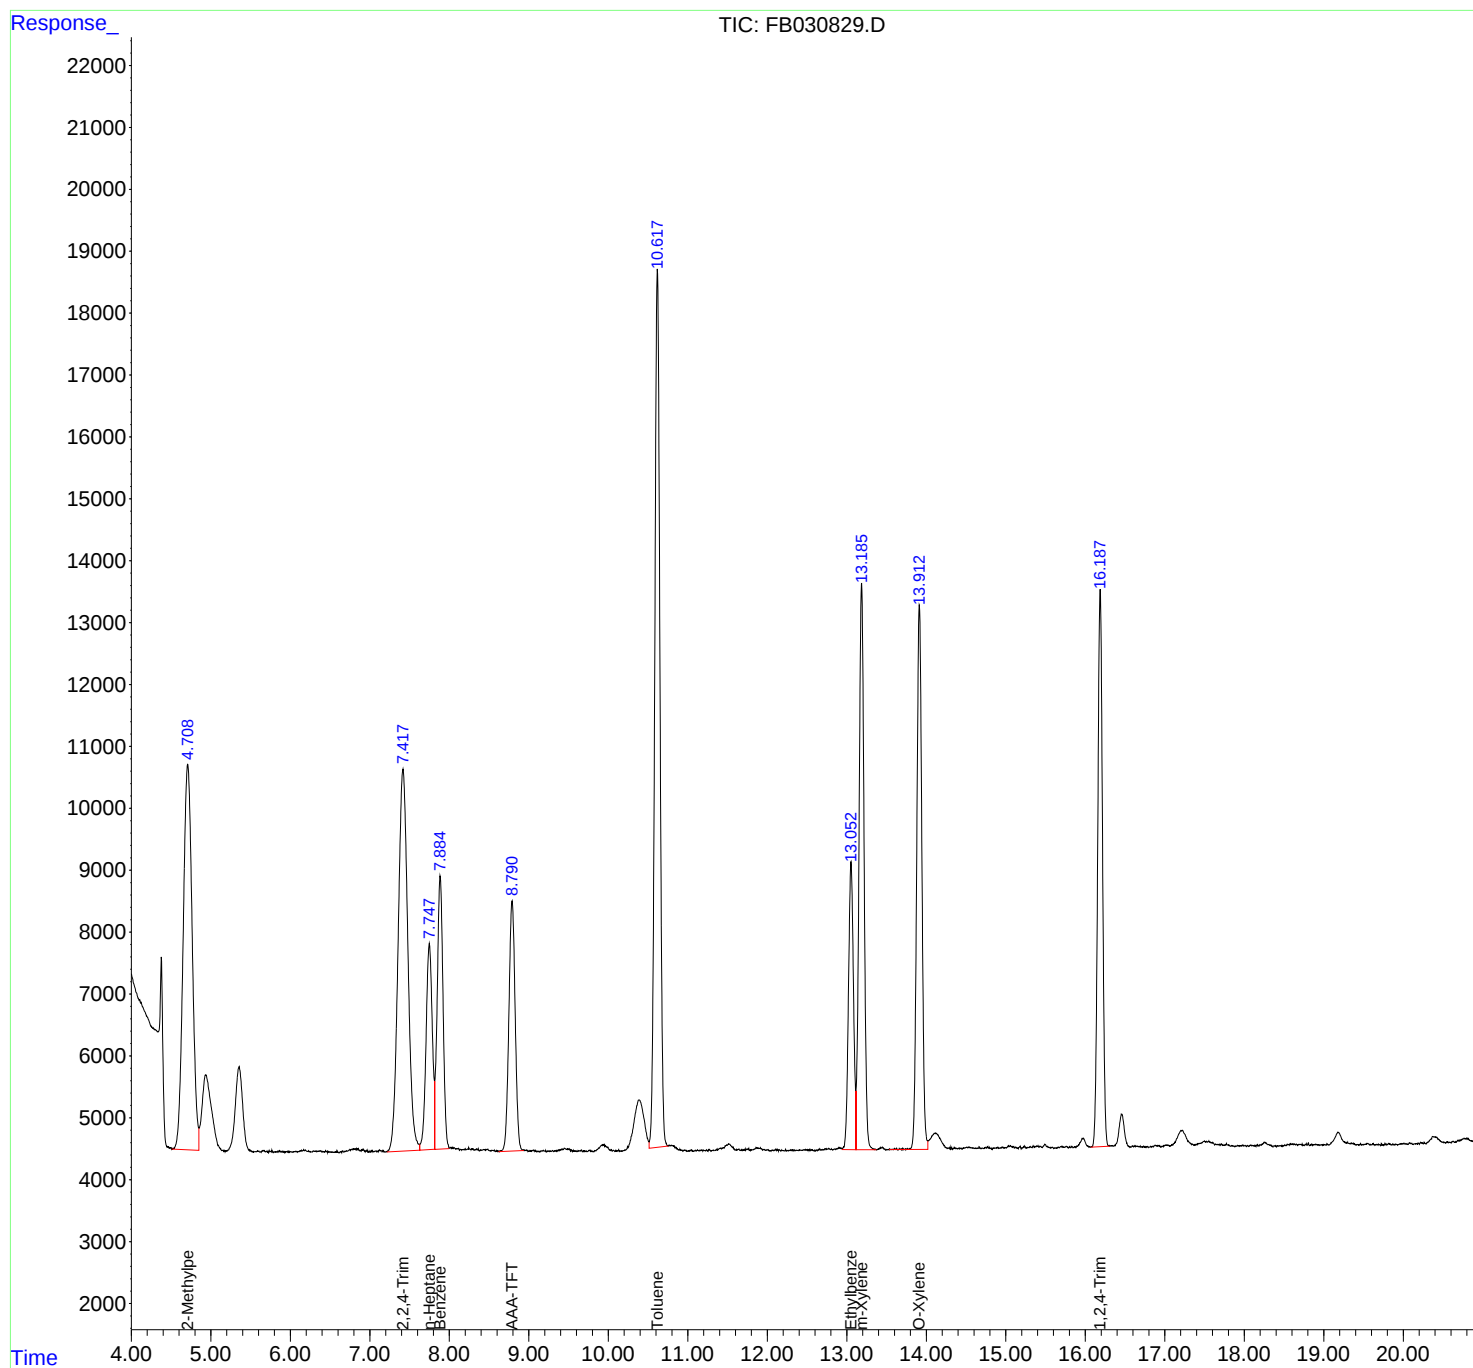


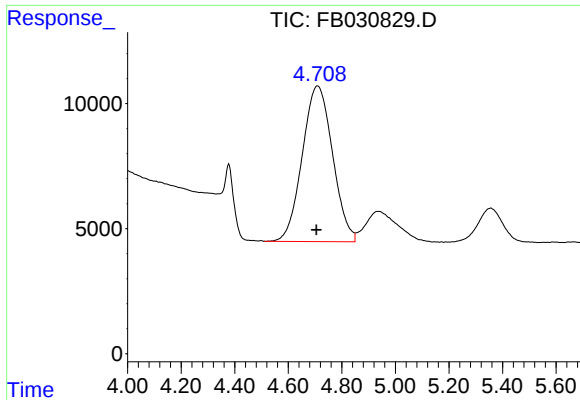

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.005 min
Response: 489468
Conc: 28.31 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0724S2

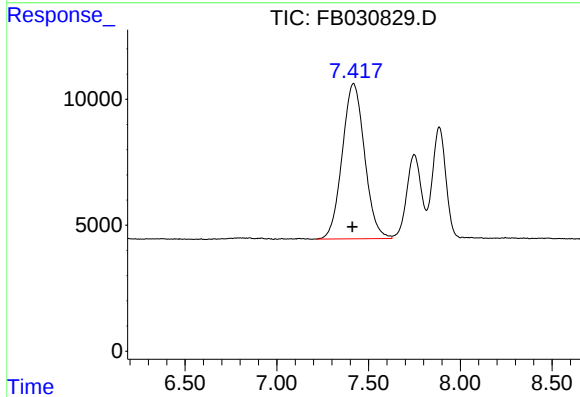


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.007 min
Response: 521206
Conc: 30.04 ng/ml

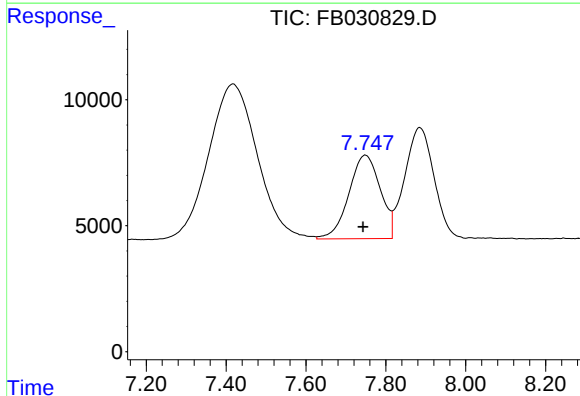


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.006 min
Response: 181656
Conc: 9.48 ng/ml

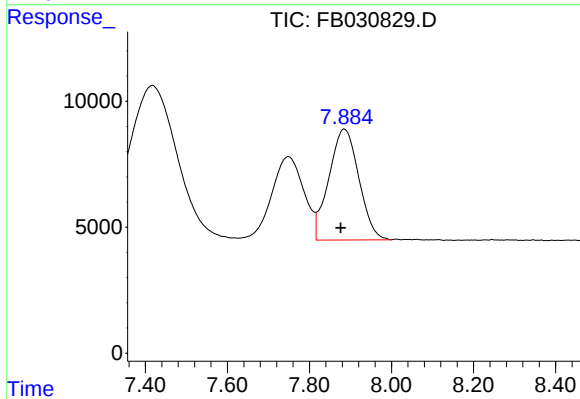

#4 Benzene


R.T.: 7.885 min
Delta R.T.: 0.009 min
Response: 223418
Conc: 10.02 ng/ml

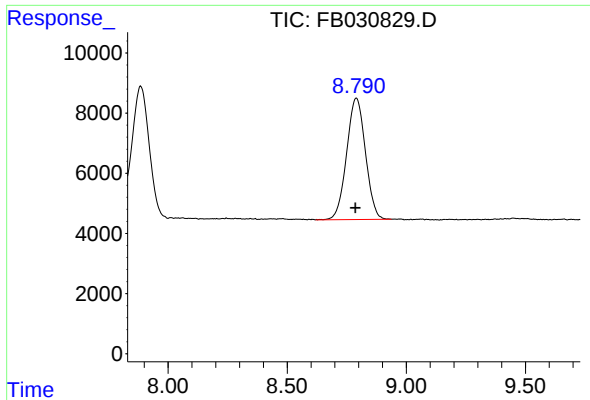

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.004 min
Response: 221297
Conc: 20.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0724S2

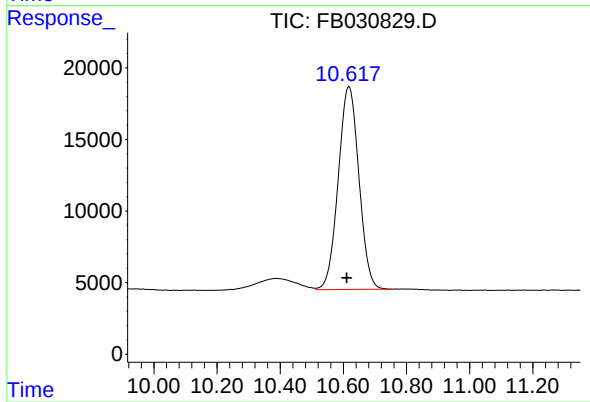


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.007 min
Response: 644016
Conc: 29.79 ng/ml

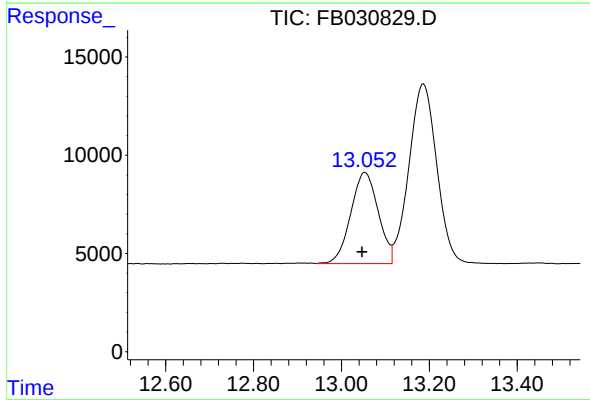


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.006 min
Response: 201276
Conc: 10.10 ng/ml

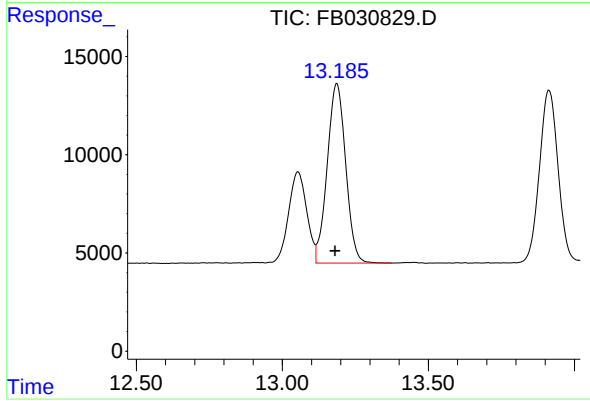

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: 0.006 min
Response: 401957
Conc: 20.12 ng/ml

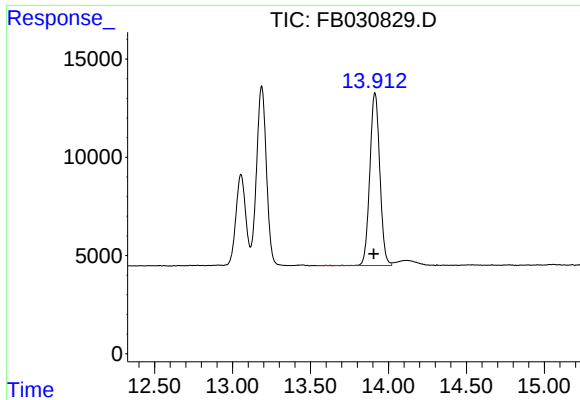

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: 0.006 min
Response: 391684
Conc: 20.49 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0724S2

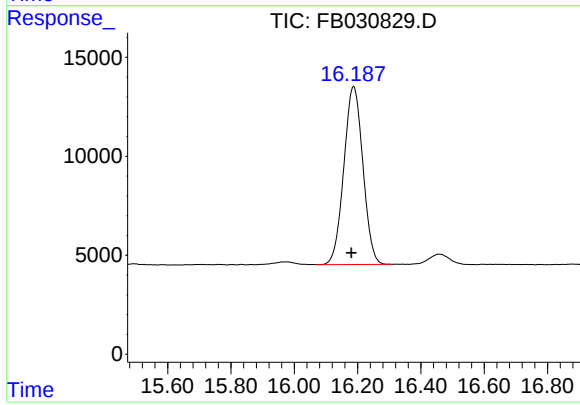

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.008 min
Response: 376142
Conc: 19.19 ng/ml