

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB072522\  
 Data File : FB027750.D  
 Signal(s) : FID2B.CH  
 Acq On : 26 Jul 2022 17:00  
 Operator : AJ/MA  
 Sample : N3839-02 50X  
 Misc : 5.00G/5.00 ML MEOH  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Jul 27 03:44:31 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB071122.M  
 Quant Title :  
 QLast Update : Mon Jul 11 14:59:12 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.  | Response | Conc Units   |
|-----------------------------|-------|----------|--------------|
| -----                       |       |          |              |
| System Monitoring Compounds |       |          |              |
| 5) s AAA-TFT                | 8.797 | 219343   | 18.847 ng/ml |
| Target Compounds            |       |          |              |
| 1) t 2-Methylpentane        | 4.693 | 57       | 0.003 ng/ml  |
| 4) t Benzene                | 7.940 | 6598     | 0.281 ng/ml  |
| -----                       |       |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB072522\  
Data File : FB027750.D  
Signal(s) : FID2B.CH  
Acq On : 26 Jul 2022 17:00  
Operator : AJ/MA  
Sample : N3839-02 50X  
Misc : 5.00G/5.00 ML MEOH  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Jul 27 03:44:31 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB071122.M  
Quant Title :  
QLast Update : Mon Jul 11 14:59:12 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

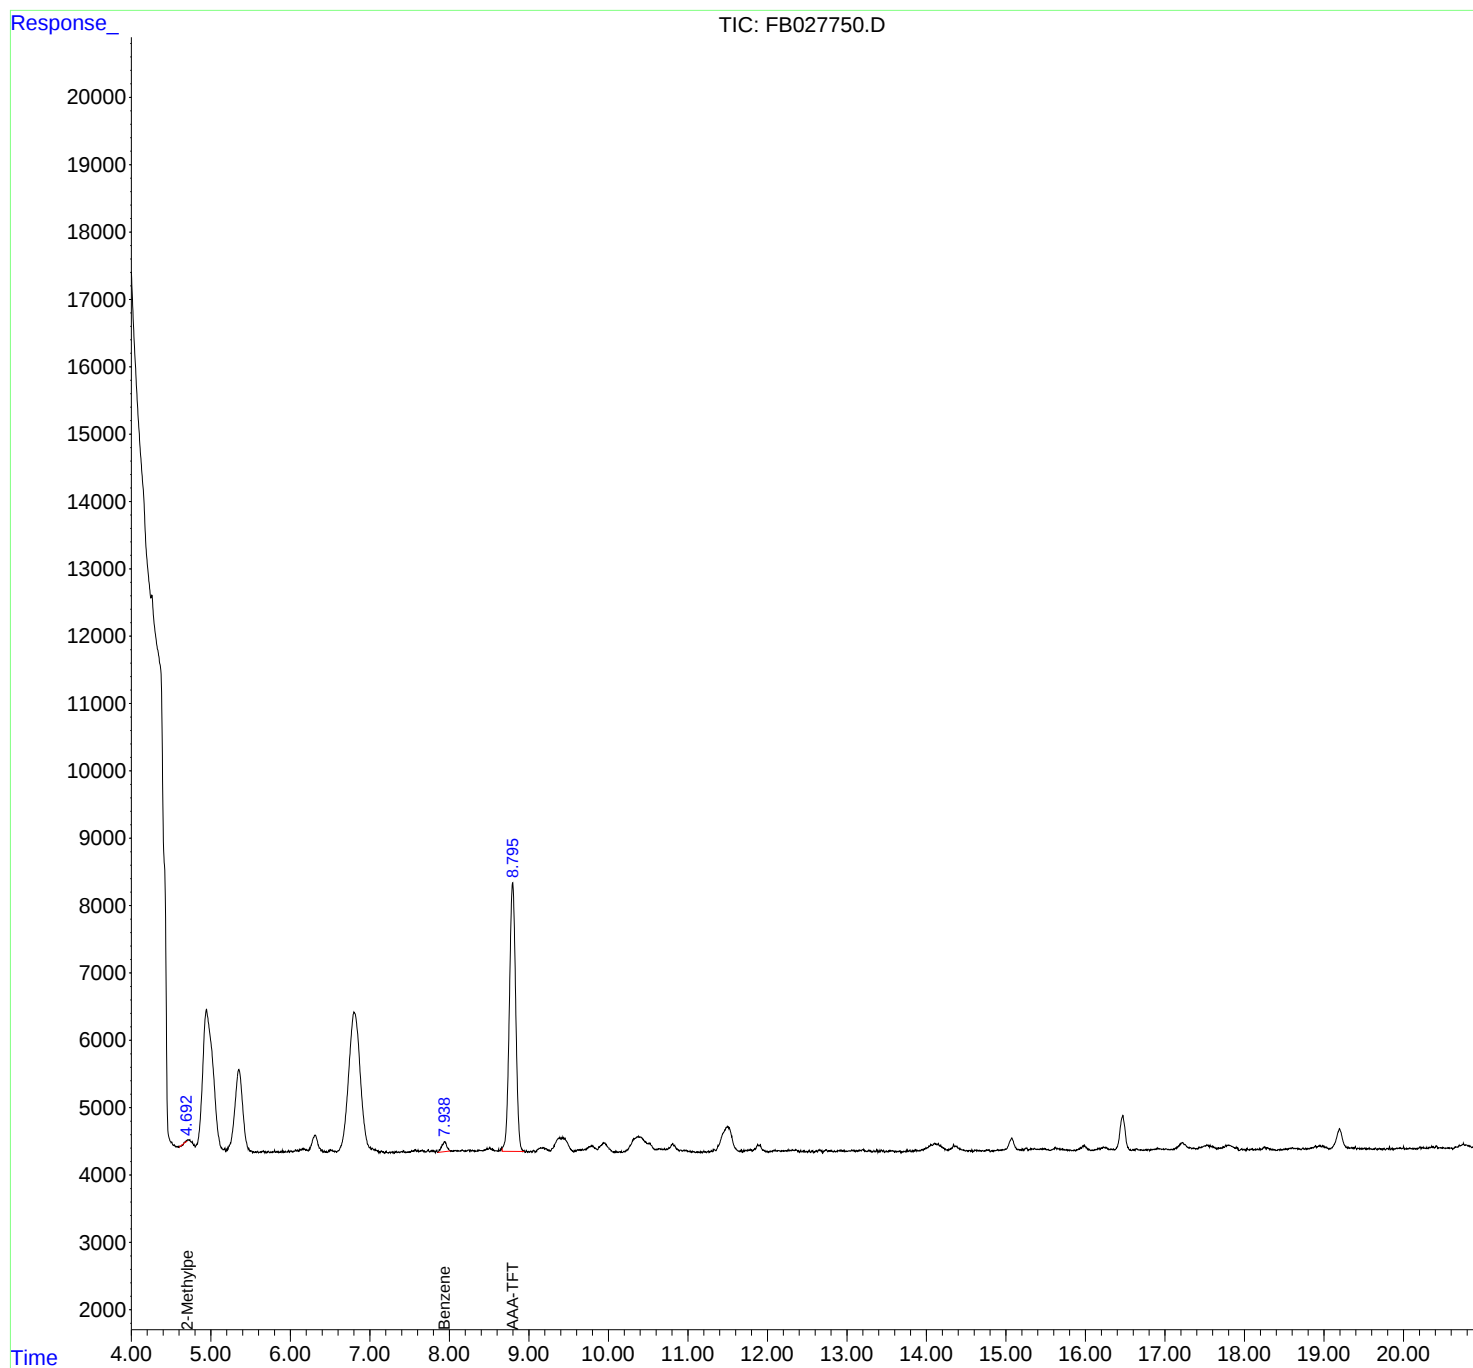


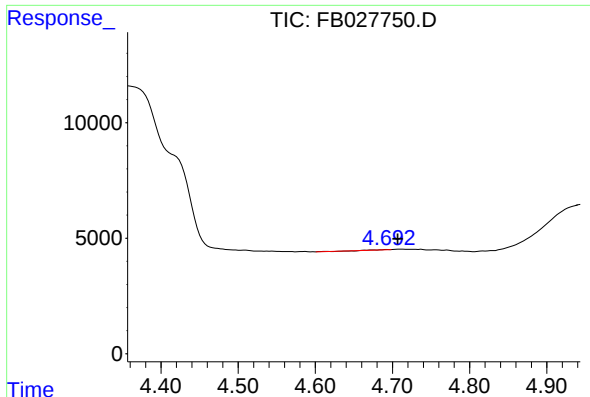

#1 2-Methylpentane


R.T.: 4.693 min  
Delta R.T.: -0.014 min  
Response: 57  
Conc: 0.00 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

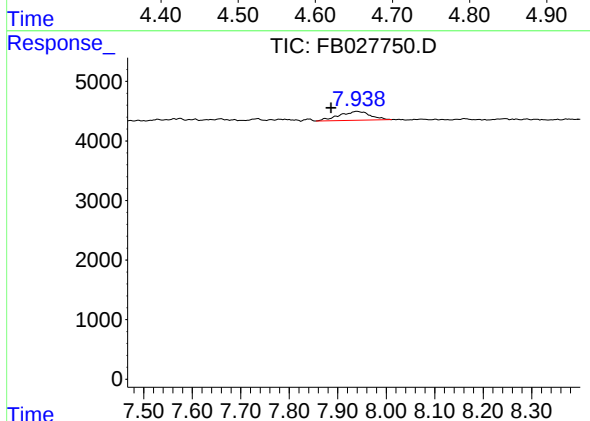

#4 Benzene

R.T.: 7.940 min  
Delta R.T.: 0.054 min  
Response: 6598  
Conc: 0.28 ng/ml

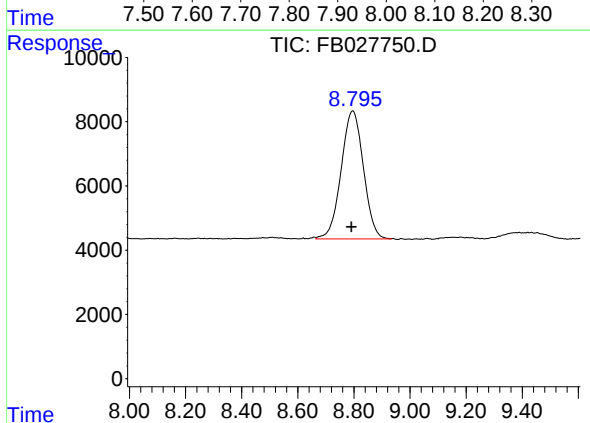

#5 AAA-TFT

R.T.: 8.797 min  
Delta R.T.: 0.006 min  
Response: 219343  
Conc: 18.85 ng/ml