

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
 Data File : FB027708.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jul 2022 12:22
 Operator : AJ/MA
 Sample : BSF0725S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0725S1

Integration File: Calibration.e
 Quant Time: Jul 26 04:48:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	220982	18.987 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	440324	20.908 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	536184	25.838 ng/ml
3) t n-Heptane	7.756	143064	6.959 ng/ml
4) t Benzene	7.893	221442	9.436 ng/ml
6) t Toluene	10.627	646005	28.930 ng/ml
7) t Ethylbenzene	13.064	211525	10.095 ng/ml
8) t m-Xylene	13.196	414638	19.803 ng/ml
9) t O-Xylene	13.923	404524	19.769 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	398047	19.154 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
Data File : FB027708.D
Signal(s) : FID2B.CH
Acq On : 25 Jul 2022 12:22
Operator : AJ/MA
Sample : BSF0725S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0725S1

Integration File: Calibration.e
Quant Time: Jul 26 04:48:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

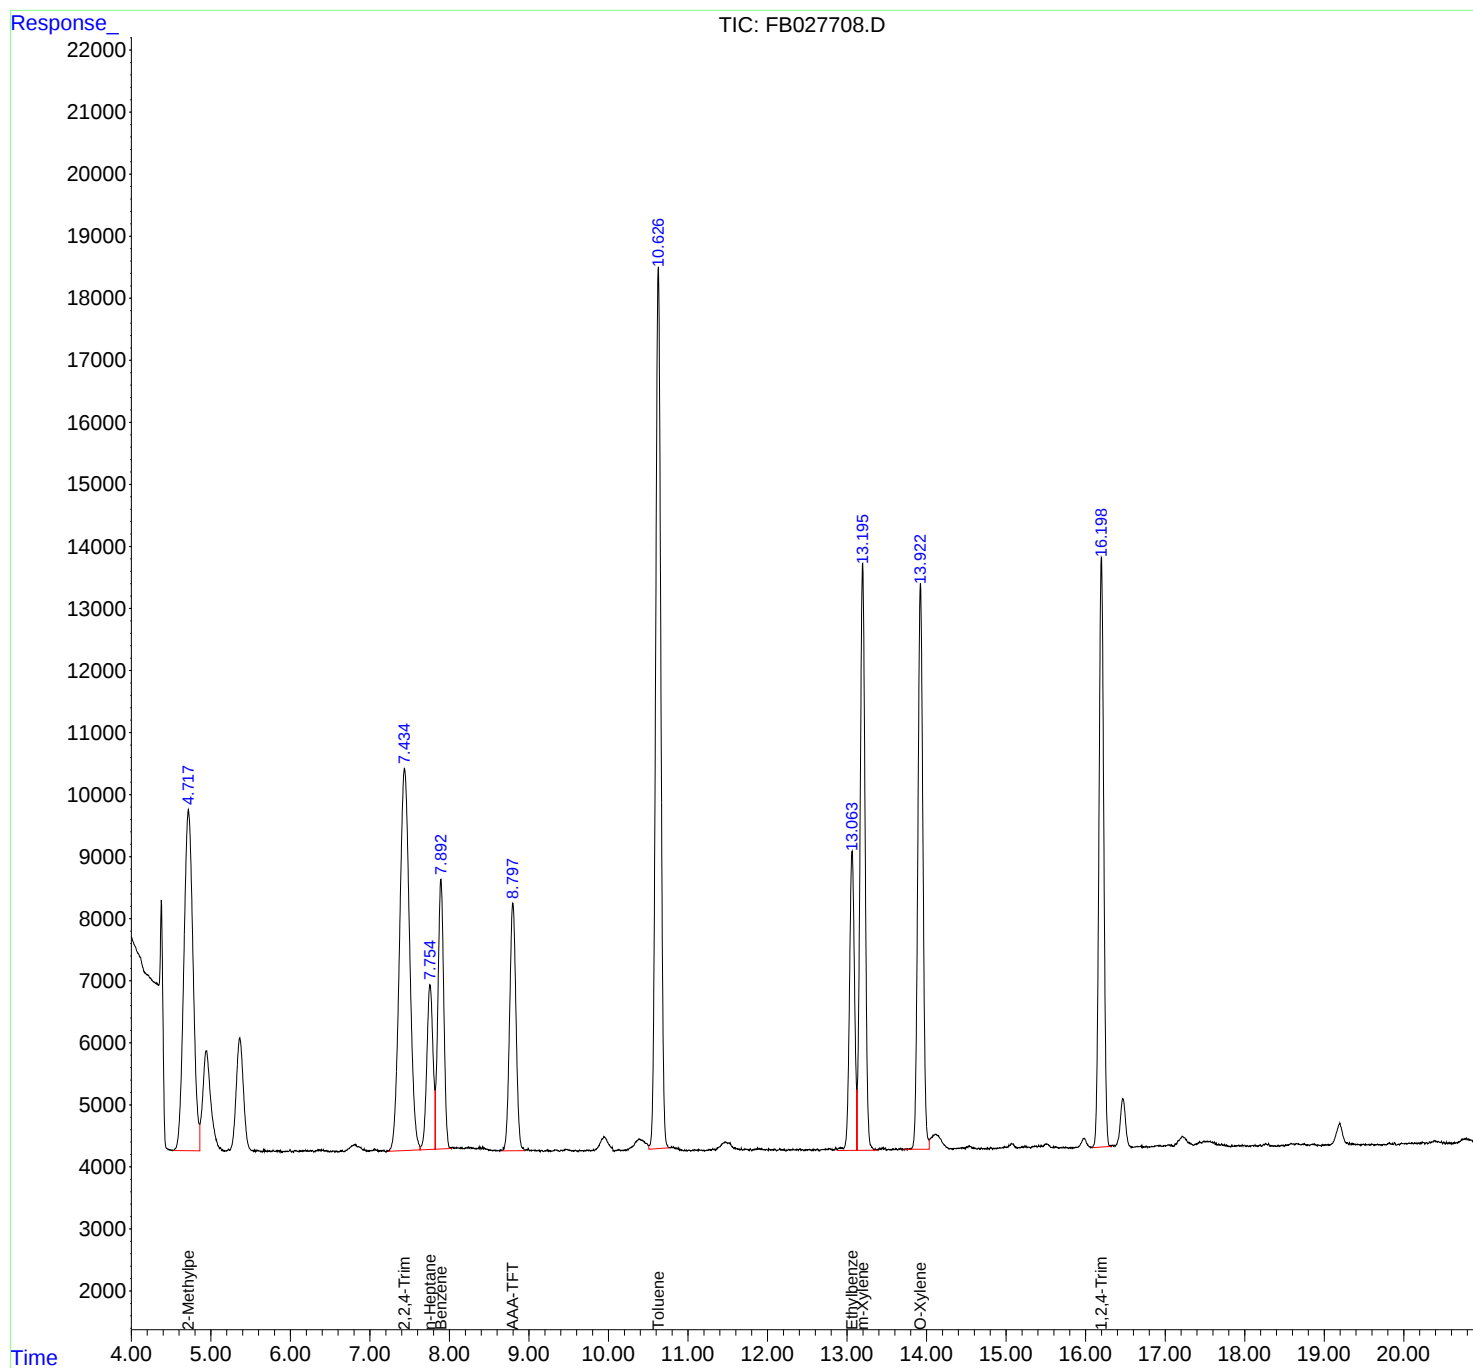


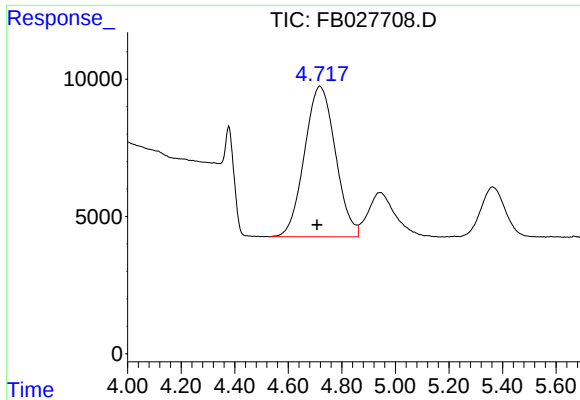

#1 2-Methylpentane


R.T.: 4.718 min
Delta R.T.: 0.011 min
Response: 440324
Conc: 20.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S1

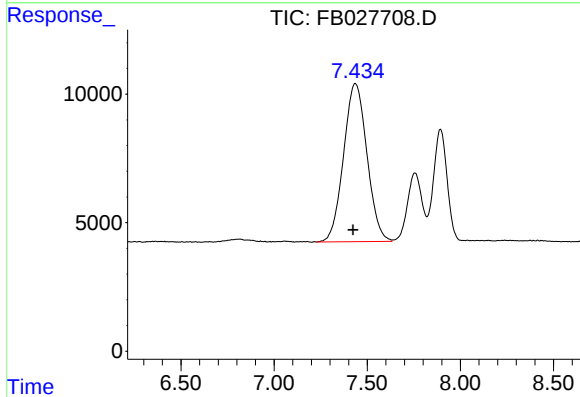


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.011 min
Response: 536184
Conc: 25.84 ng/ml

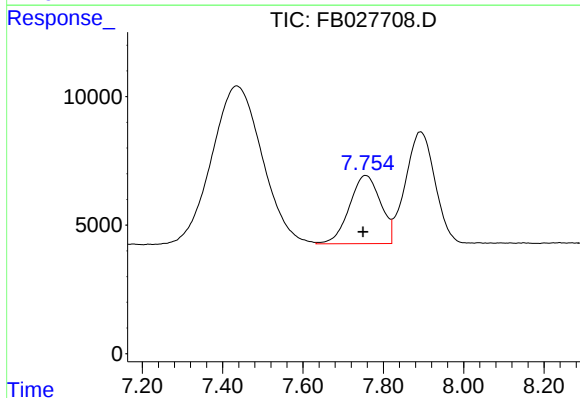


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.006 min
Response: 143064
Conc: 6.96 ng/ml

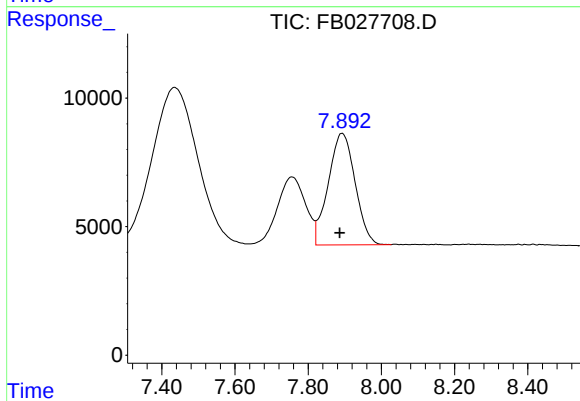

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.007 min
Response: 221442
Conc: 9.44 ng/ml

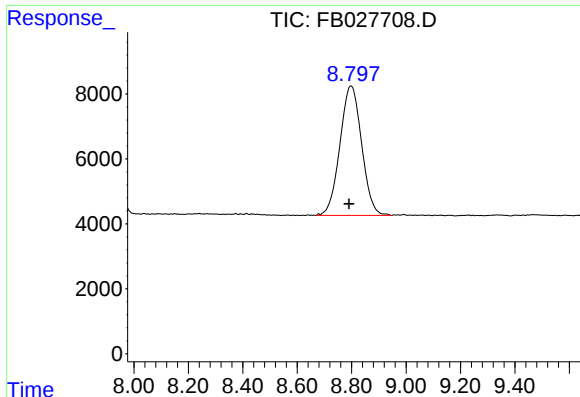

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.007 min
Response: 220982
Conc: 18.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S1

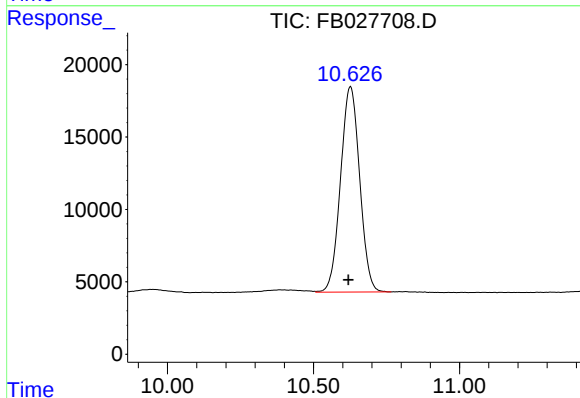


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.008 min
Response: 646005
Conc: 28.93 ng/ml

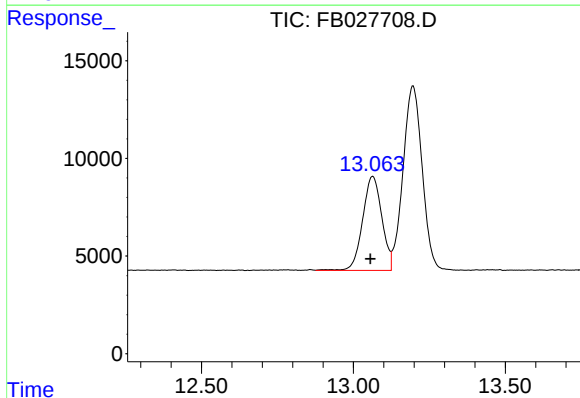


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.008 min
Response: 211525
Conc: 10.09 ng/ml

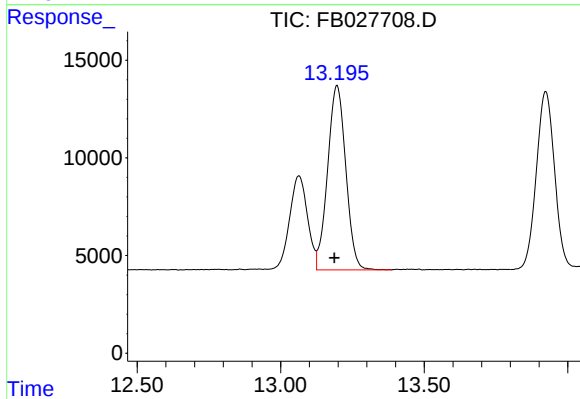

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: 0.009 min
Response: 414638
Conc: 19.80 ng/ml

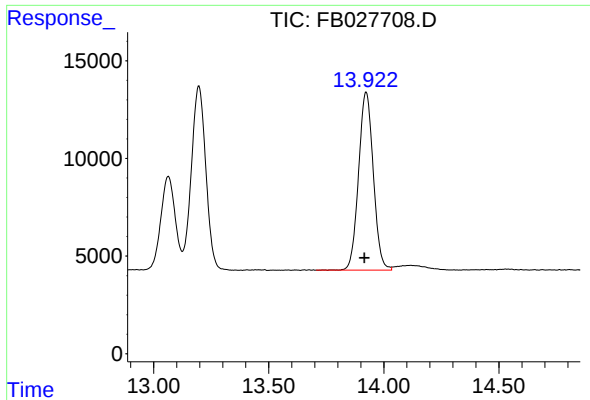

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.008 min
Response: 404524
Conc: 19.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S1

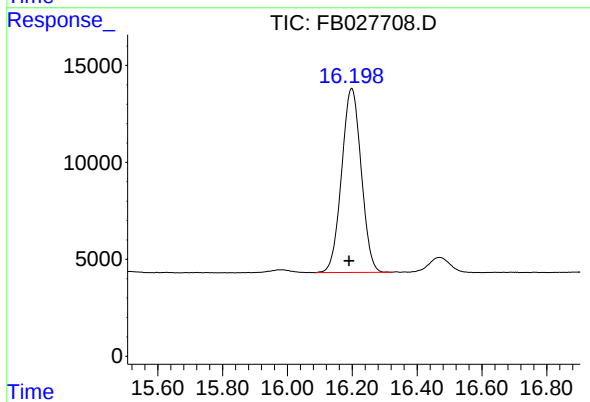

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.009 min
Response: 398047
Conc: 19.15 ng/ml