

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
 Data File : FB027716.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jul 2022 17:25
 Operator : AJ/MA
 Sample : BSF0725S2
 Misc : 5.08G/5.00 ML DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0725S2

Integration File: Calibration.e
 Quant Time: Jul 26 04:49:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	256010	21.997 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.723	392206	18.624 ng/ml
2) t 2,2,4-Trimethylpentane	7.438	501152	24.150 ng/ml
3) t n-Heptane	7.760	133234	6.481 ng/ml
4) t Benzene	7.896	214908	9.158 ng/ml
6) t Toluene	10.630	624265	27.956 ng/ml
7) t Ethylbenzene	13.066	204403	9.755 ng/ml
8) t m-Xylene	13.199	401652	19.183 ng/ml
9) t O-Xylene	13.926	390916	19.104 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	384674	18.510 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
Data File : FB072716.D
Signal(s) : FID2B.CH
Acq On : 25 Jul 2022 17:25
Operator : AJ/MA
Sample : BSF0725S2
Misc : 5.08G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0725S2

Integration File: Calibration.e
Quant Time: Jul 26 04:49:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

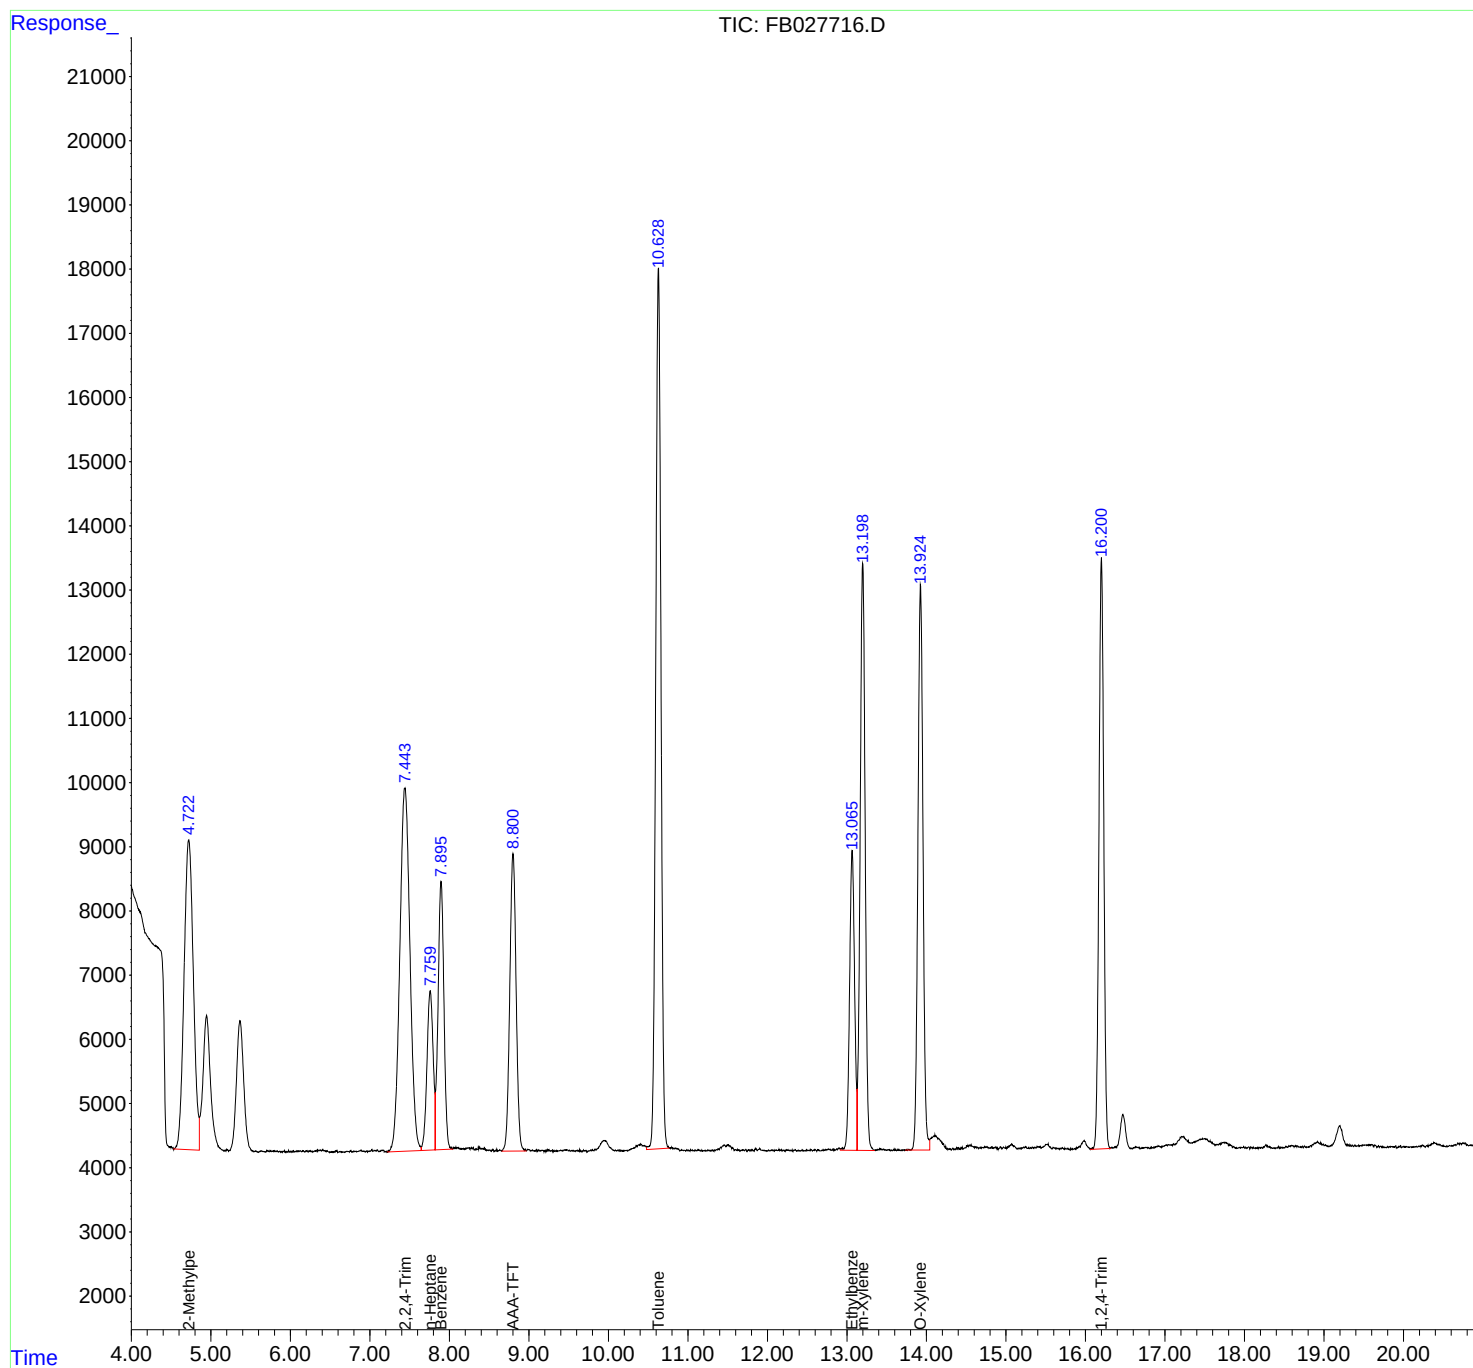


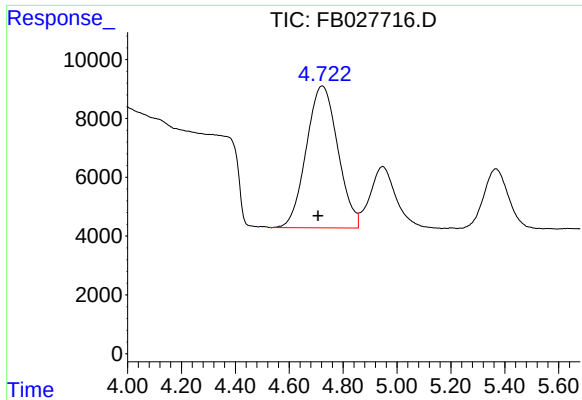

#1 2-Methylpentane


R.T.: 4.723 min
Delta R.T.: 0.016 min
Response: 392206
Conc: 18.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S2

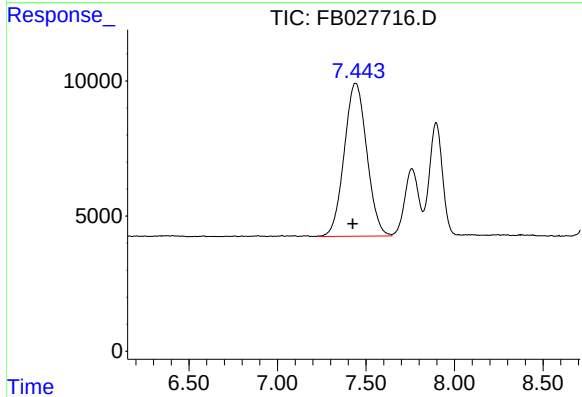


#2 2,2,4-Trimethylpentane

R.T.: 7.438 min
Delta R.T.: 0.014 min
Response: 501152
Conc: 24.15 ng/ml

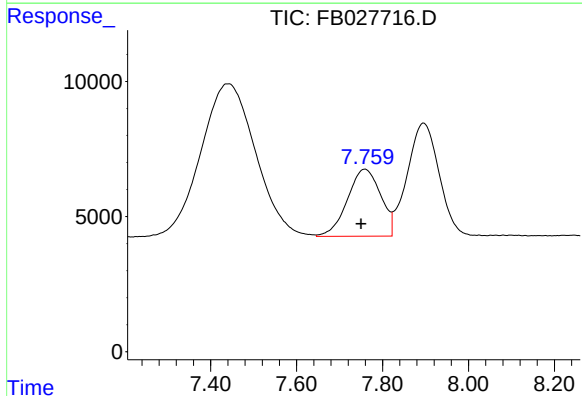


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.010 min
Response: 133234
Conc: 6.48 ng/ml

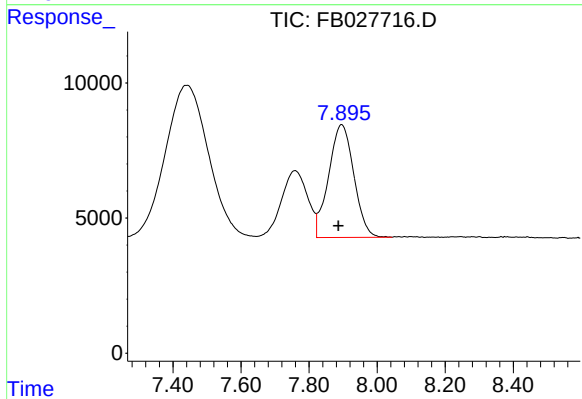

#4 Benzene


R.T.: 7.896 min
Delta R.T.: 0.010 min
Response: 214908
Conc: 9.16 ng/ml

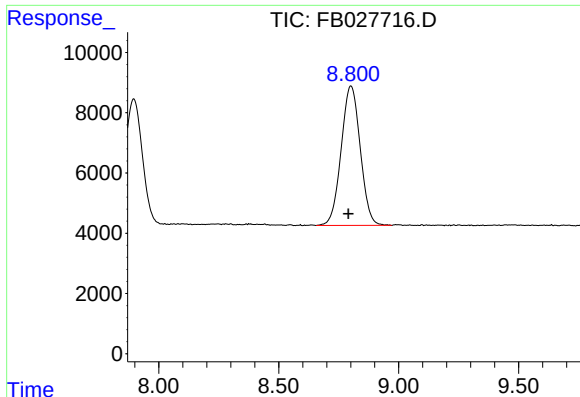

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.010 min
Response: 256010
Conc: 22.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S2

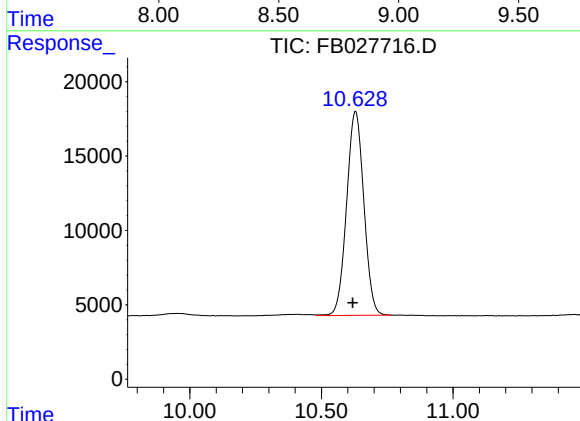


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.011 min
Response: 624265
Conc: 27.96 ng/ml

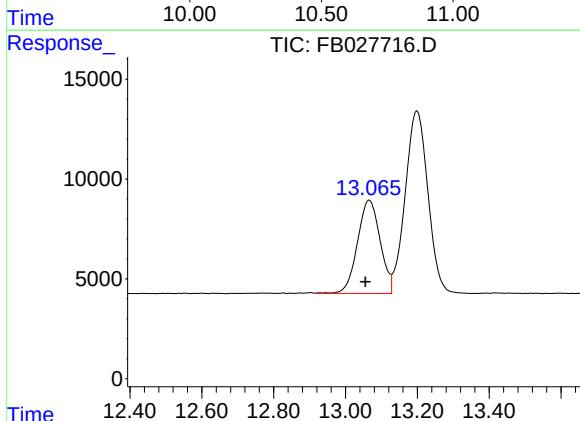


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: 0.011 min
Response: 204403
Conc: 9.75 ng/ml

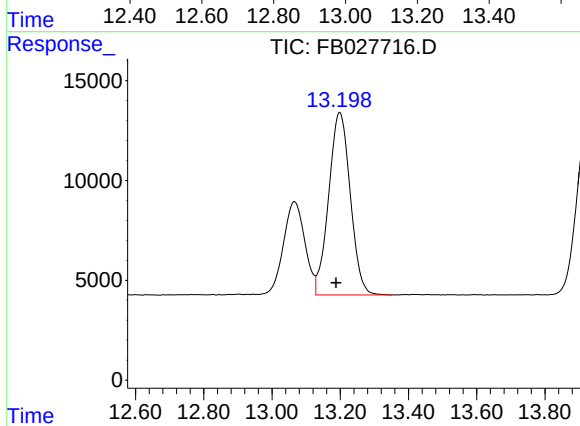

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: 0.011 min
Response: 401652
Conc: 19.18 ng/ml

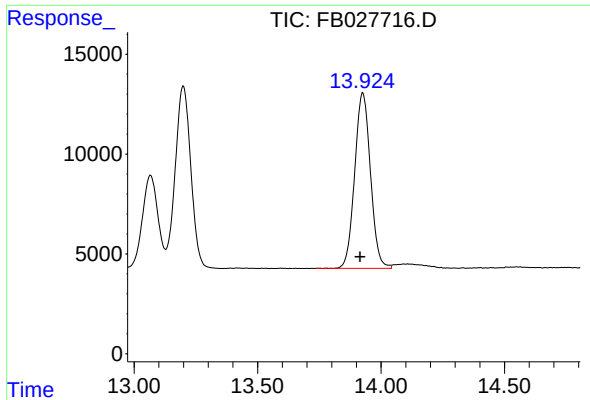

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.011 min
Response: 390916
Conc: 19.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S2

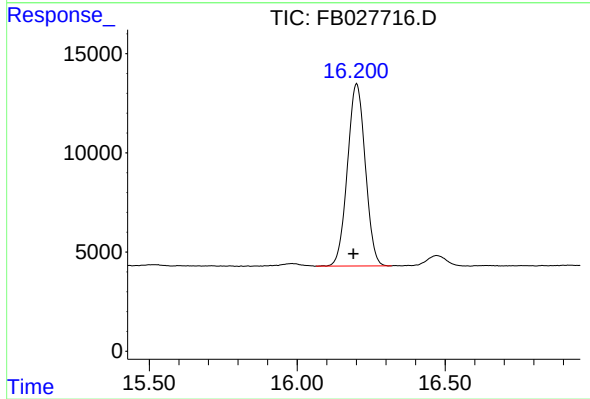

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.011 min
Response: 384674
Conc: 18.51 ng/ml