

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
 Data File : FB027731.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jul 2022 3:59
 Operator : AJ/MA
 Sample : N3857-02MS
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-4MS

Integration File: Calibration.e
 Quant Time: Jul 26 06:25:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	163877	14.081 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	265755	12.619 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	258760	12.469 ng/ml
3) t n-Heptane	7.754	61753	3.004 ng/ml
4) t Benzene	7.892	155422	6.623 ng/ml
6) t Toluene	10.626	429342	19.227 ng/ml
7) t Ethylbenzene	13.063	130304	6.219 ng/ml
8) t m-Xylene	13.195	256542	12.252 ng/ml
9) t O-Xylene	13.923	262475	12.827 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	228516	10.996 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
Data File : FB027731.D
Signal(s) : FID2B.CH
Acq On : 26 Jul 2022 3:59
Operator : AJ/MA
Sample : N3857-02MS
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-4MS

Integration File: Calibration.e
Quant Time: Jul 26 06:25:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

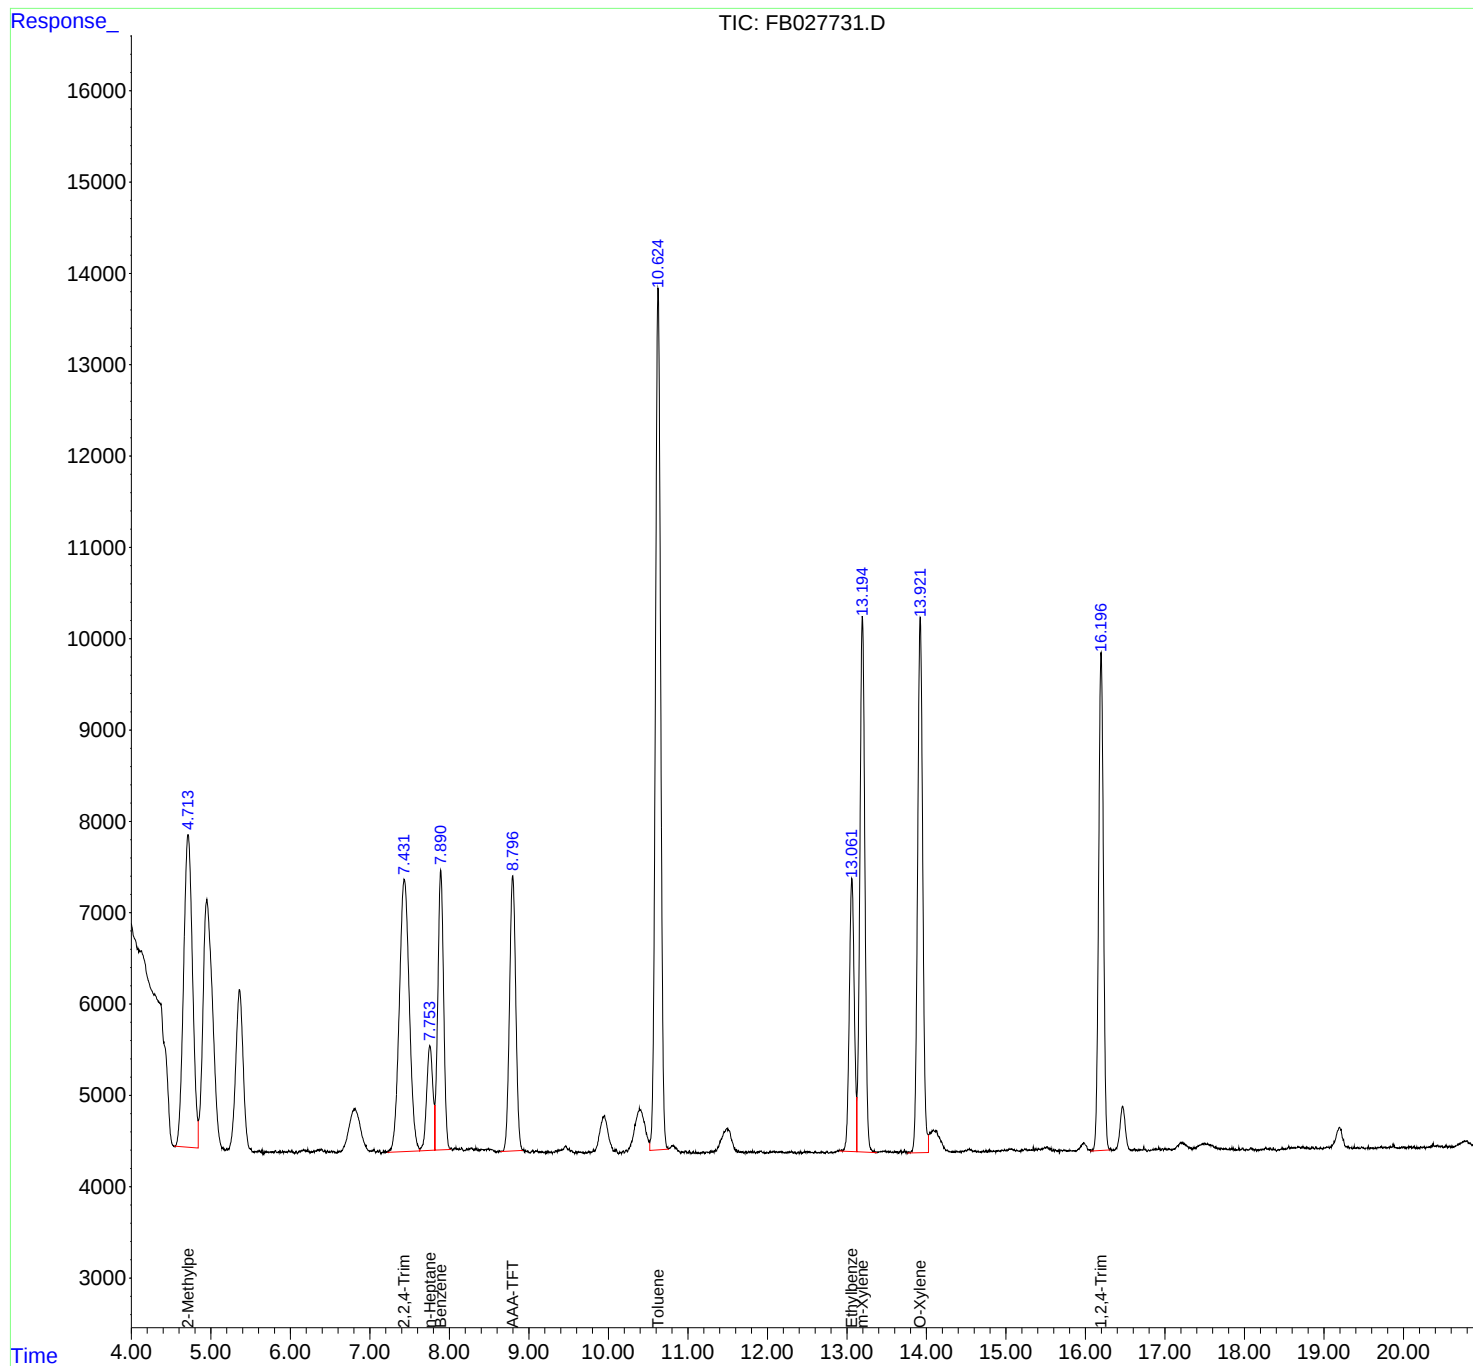


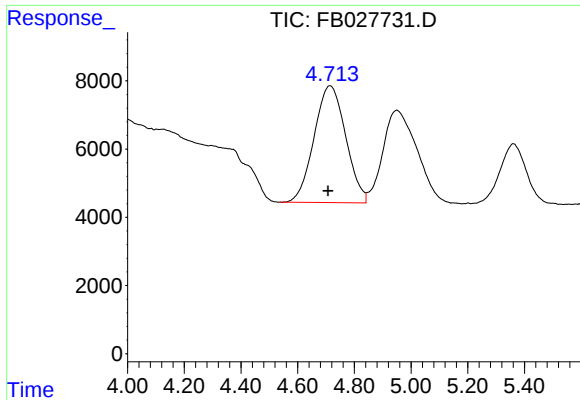

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: 0.008 min
Response: 265755
Conc: 12.62 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-4MS

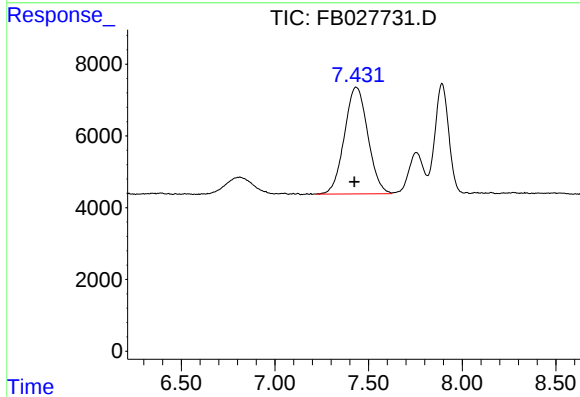


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: 0.008 min
Response: 258760
Conc: 12.47 ng/ml

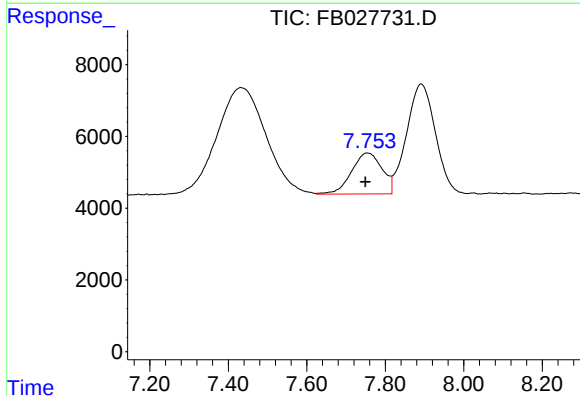


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.005 min
Response: 61753
Conc: 3.00 ng/ml

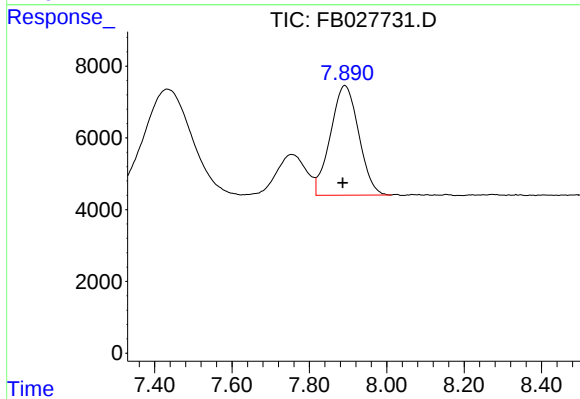

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.006 min
Response: 155422
Conc: 6.62 ng/ml

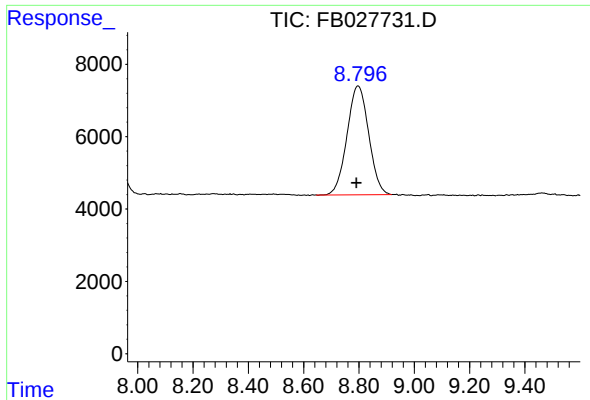

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.006 min
Response: 163877
Conc: 14.08 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-4MS

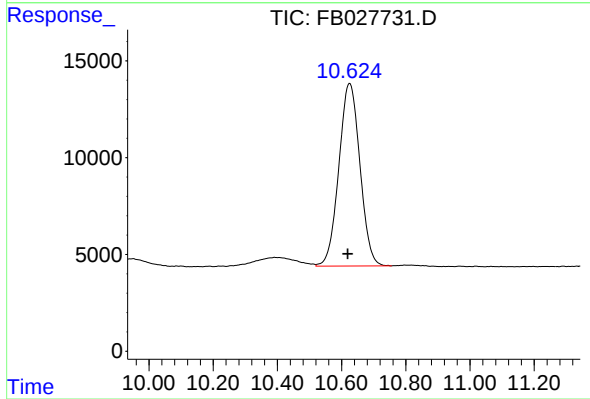


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.007 min
Response: 429342
Conc: 19.23 ng/ml

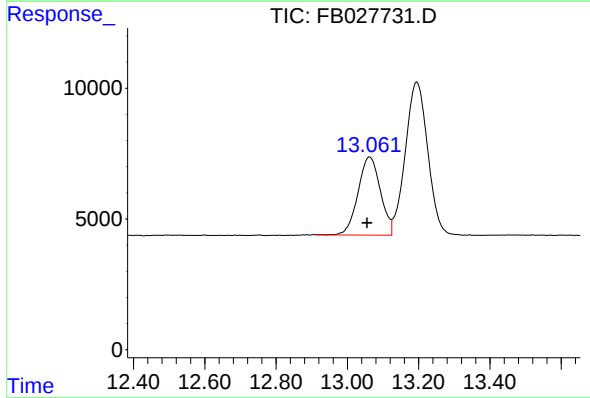


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.007 min
Response: 130304
Conc: 6.22 ng/ml

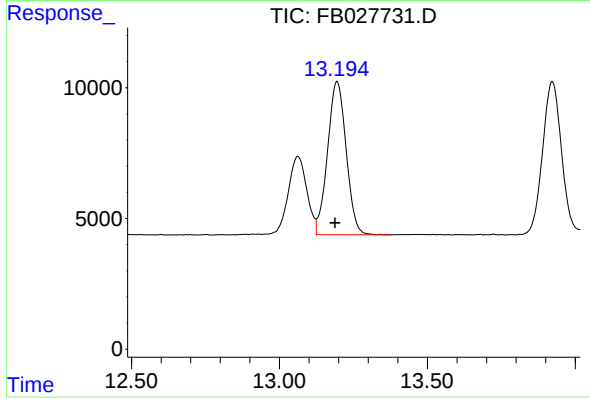

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.007 min
Response: 256542
Conc: 12.25 ng/ml

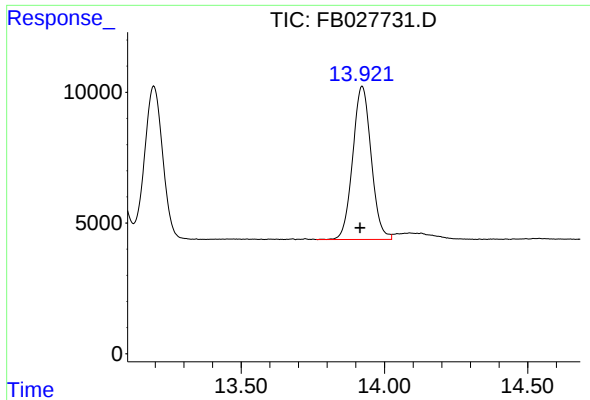

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.007 min
Response: 262475
Conc: 12.83 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-4MS

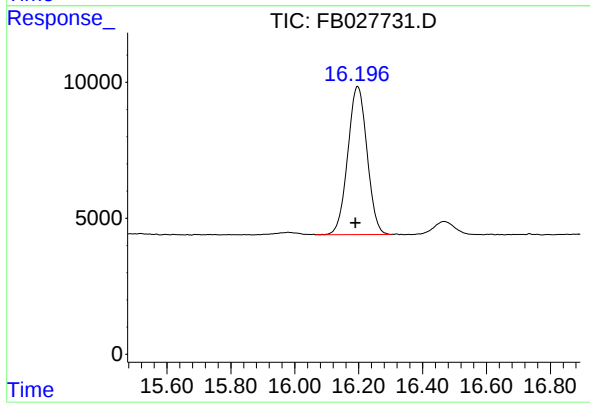

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.007 min
Response: 228516
Conc: 11.00 ng/ml