

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
 Data File : FB027734.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jul 2022 5:50
 Operator : AJ/MA
 Sample : N3857-02MS
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-4MS

Integration File: Calibration.e
 Quant Time: Jul 26 08:59:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	174657	15.007 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	264663	12.567 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	256895	12.379 ng/ml
3) t n-Heptane	7.753	58081	2.825 ng/ml
4) t Benzene	7.890	160765	6.851 ng/ml
6) t Toluene	10.624	429169	19.219 ng/ml
7) t Ethylbenzene	13.061	131923	6.296 ng/ml
8) t m-Xylene	13.193	259373	12.388 ng/ml
9) t O-Xylene	13.920	265460	12.973 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	234481	11.283 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
Data File : FB027734.D
Signal(s) : FID2B.CH
Acq On : 26 Jul 2022 5:50
Operator : AJ/MA
Sample : N3857-02MS
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-4MS

Integration File: Calibration.e
Quant Time: Jul 26 08:59:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

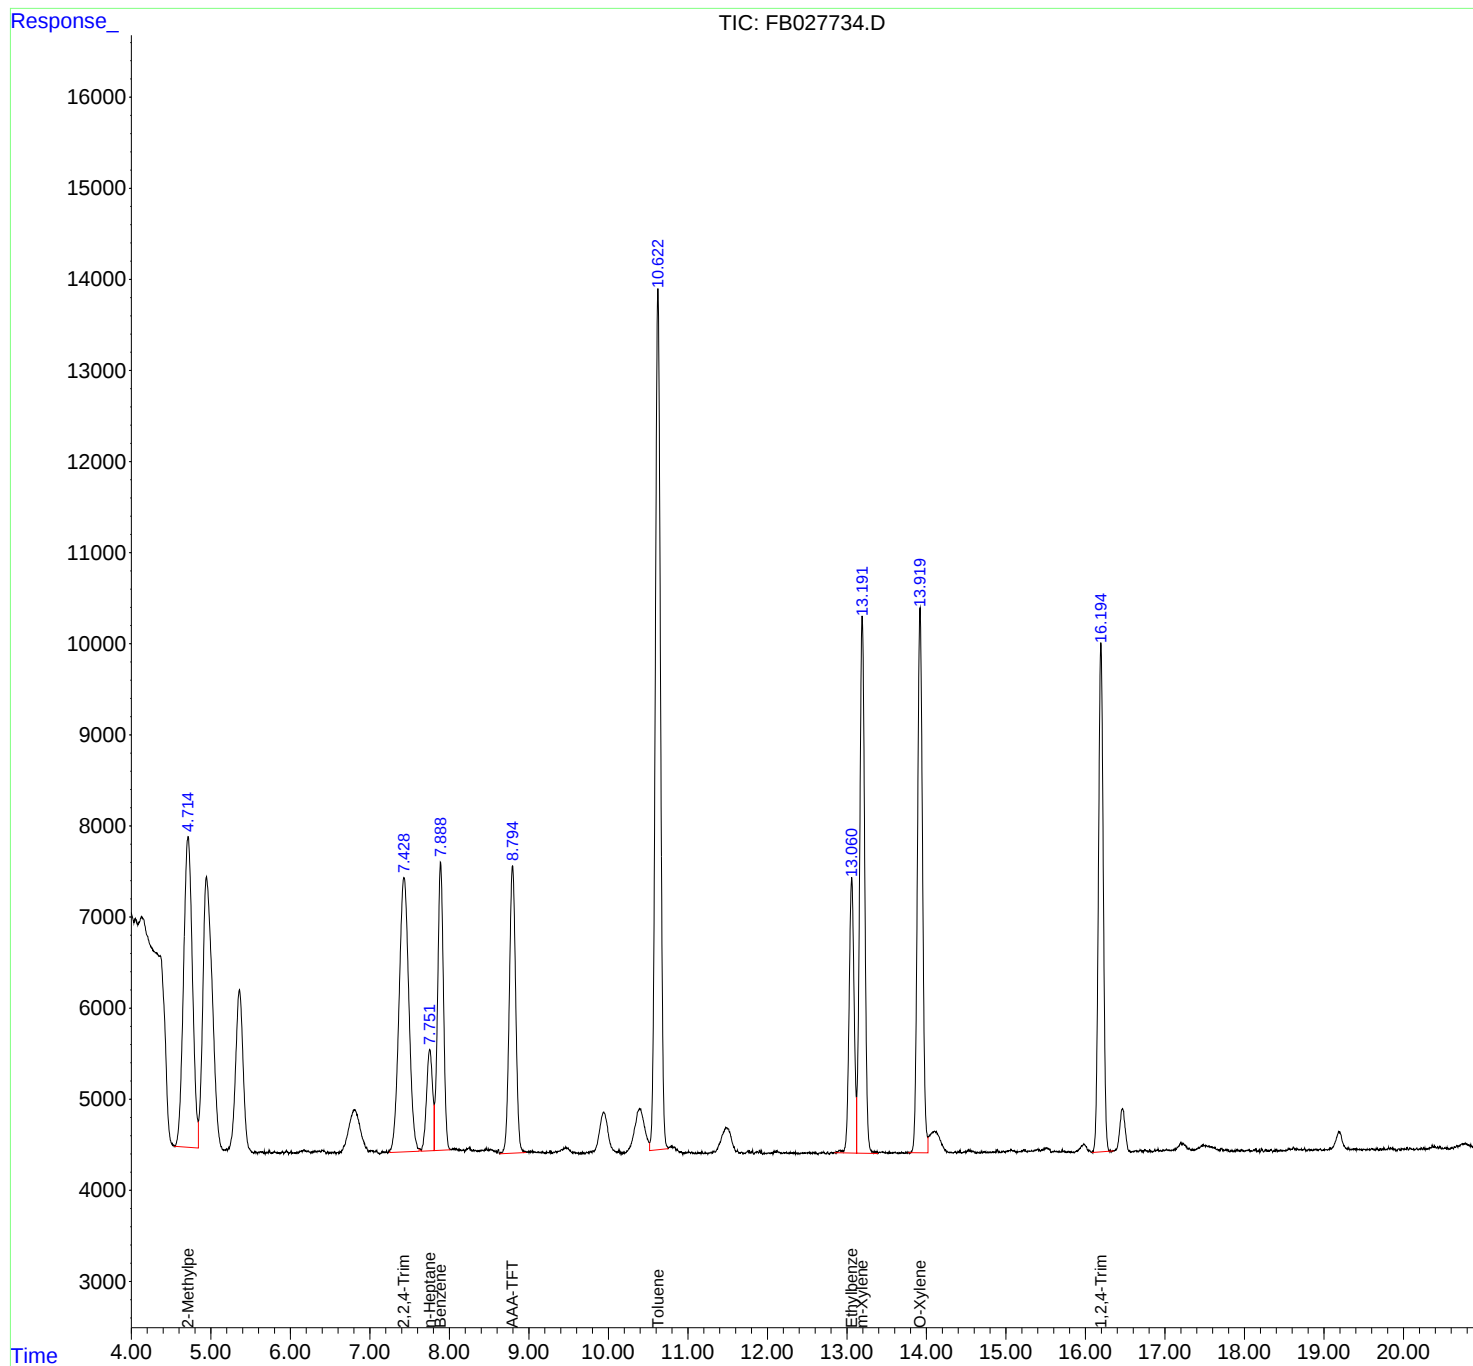


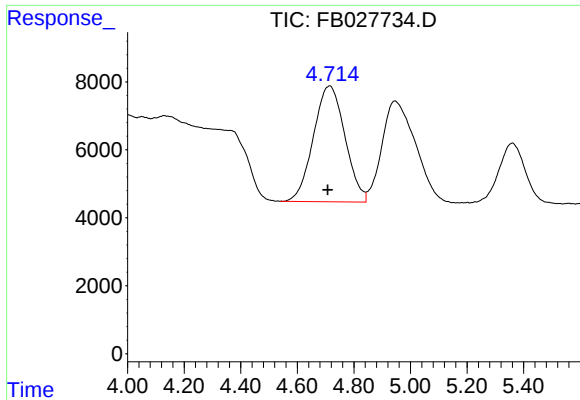

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.009 min
Response: 264663
Conc: 12.57 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-4MS

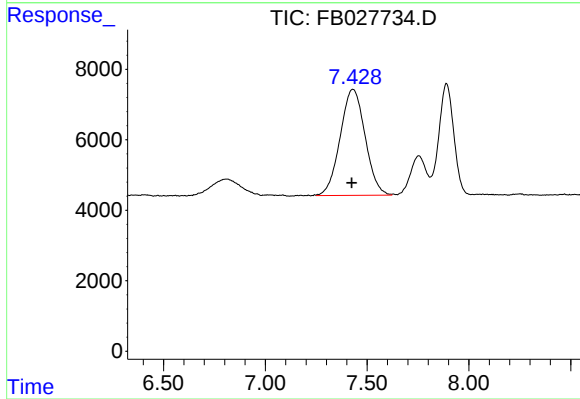


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.006 min
Response: 256895
Conc: 12.38 ng/ml

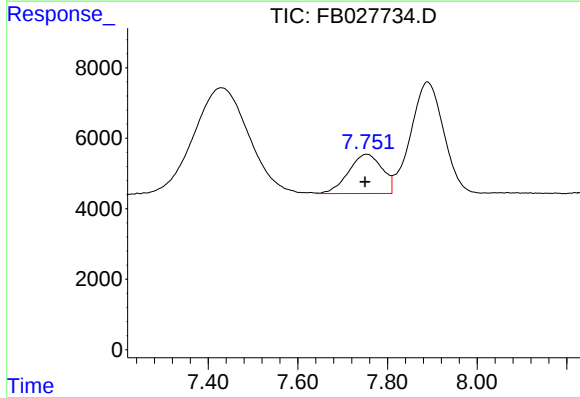


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.003 min
Response: 58081
Conc: 2.83 ng/ml

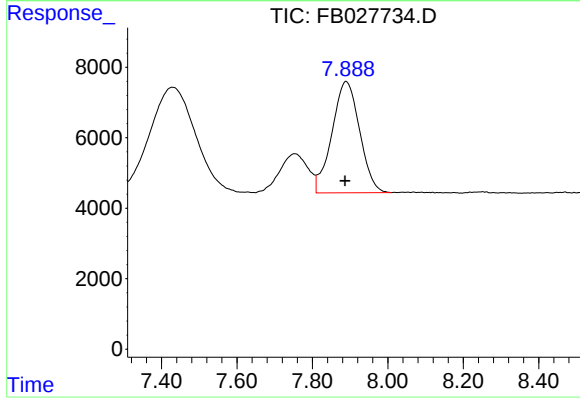

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.003 min
Response: 160765
Conc: 6.85 ng/ml

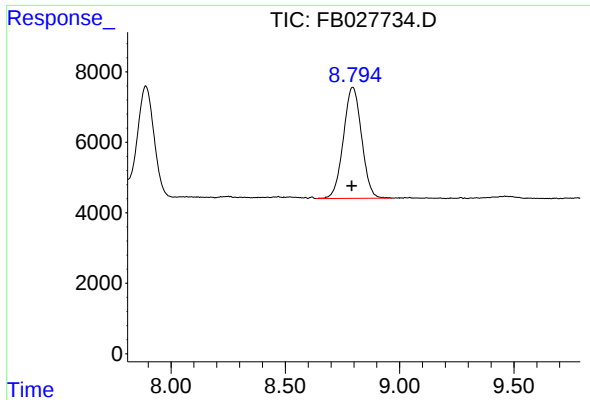

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 174657
Conc: 15.01 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-4MS

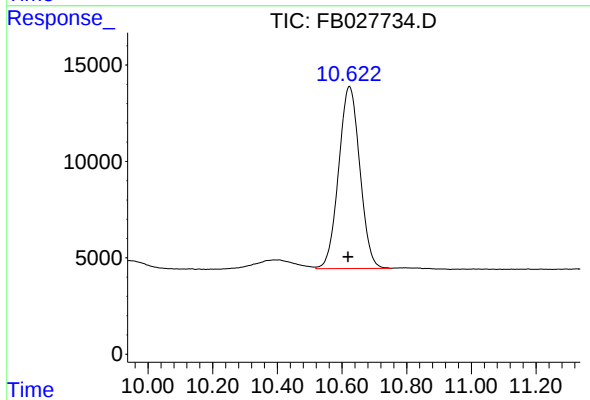


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.005 min
Response: 429169
Conc: 19.22 ng/ml

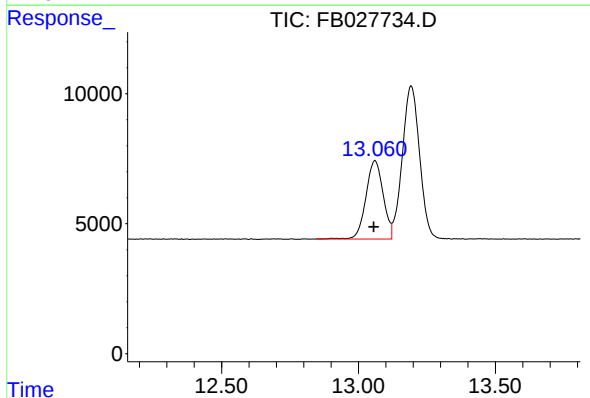


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.005 min
Response: 131923
Conc: 6.30 ng/ml

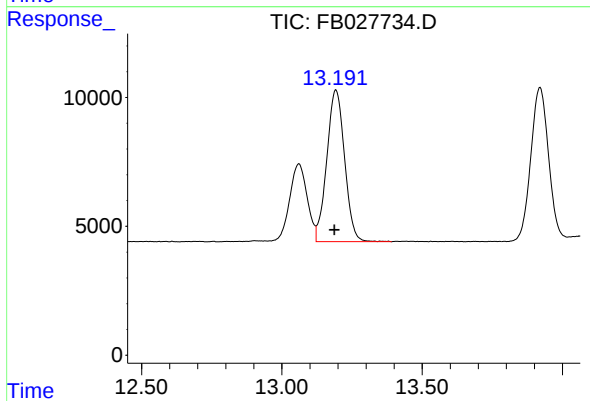

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.005 min
Response: 259373
Conc: 12.39 ng/ml

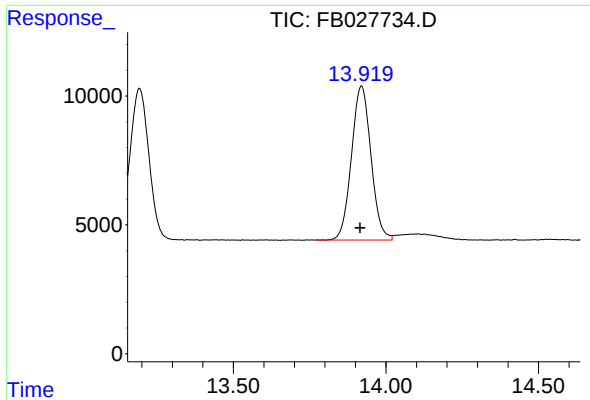

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.005 min
Response: 265460
Conc: 12.97 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-4MS

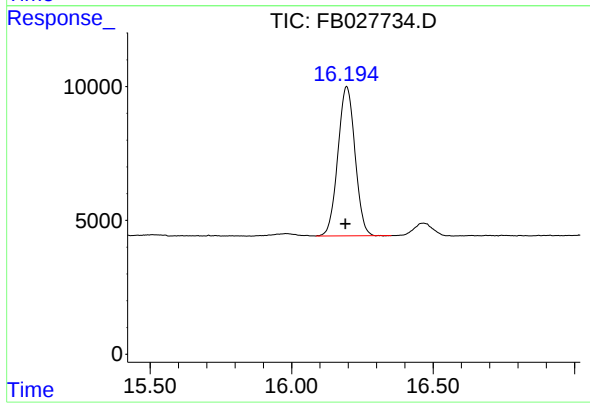

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.005 min
Response: 234481
Conc: 11.28 ng/ml