

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
 Data File : FB027746.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jul 2022 14:32
 Operator : AJ/MA
 Sample : BSF0725S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0725S3

Integration File: Calibration.e
 Quant Time: Jul 27 03:44:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	267028	22.944 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	411244	19.528 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	523713	25.237 ng/ml
3) t n-Heptane	7.754	136577	6.643 ng/ml
4) t Benzene	7.891	221761	9.450 ng/ml
6) t Toluene	10.625	640967	28.704 ng/ml
7) t Ethylbenzene	13.063	210434	10.043 ng/ml
8) t m-Xylene	13.195	414338	19.789 ng/ml
9) t O-Xylene	13.922	398138	19.457 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	390670	18.799 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
Data File : FB027746.D
Signal(s) : FID2B.CH
Acq On : 26 Jul 2022 14:32
Operator : AJ/MA
Sample : BSF0725S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0725S3

Integration File: Calibration.e
Quant Time: Jul 27 03:44:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

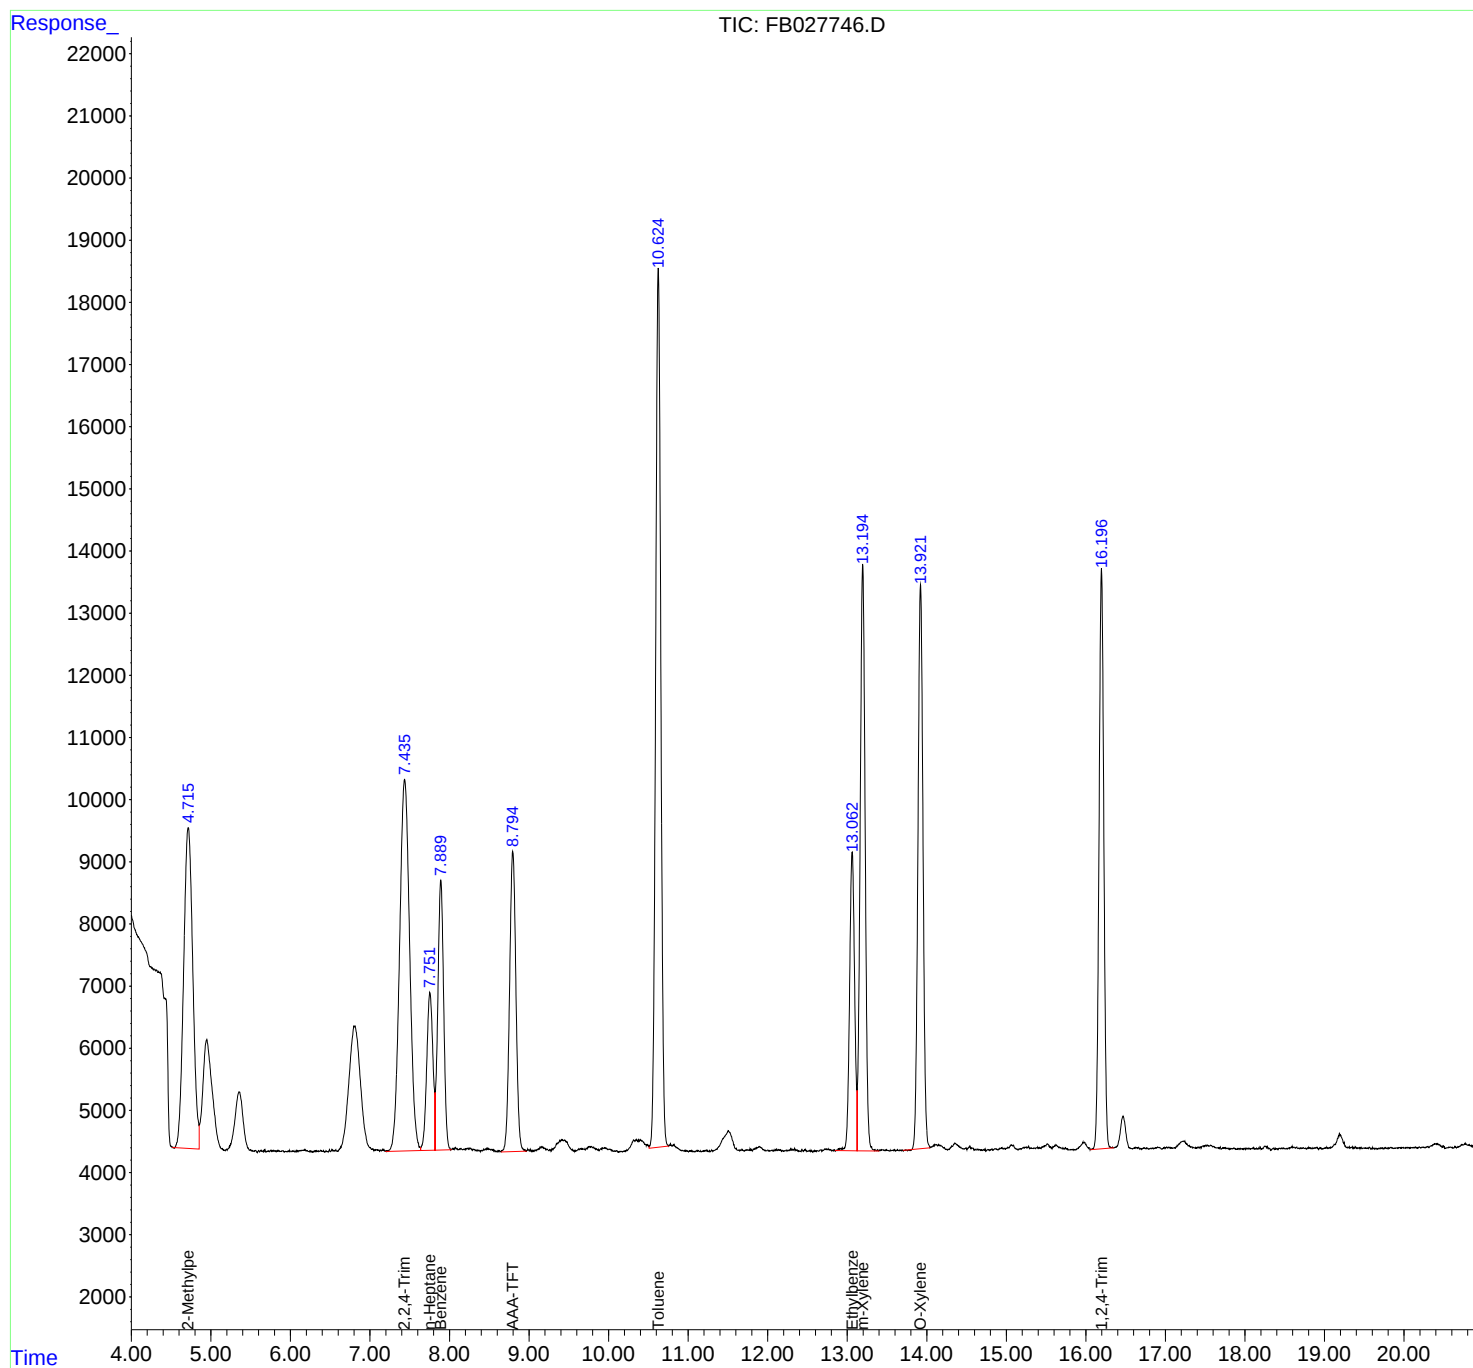


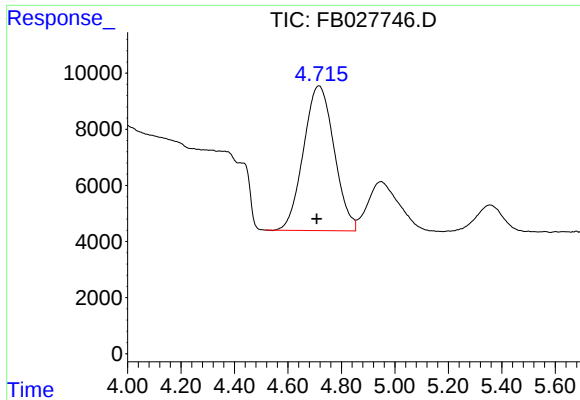

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.010 min
Response: 411244
Conc: 19.53 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S3

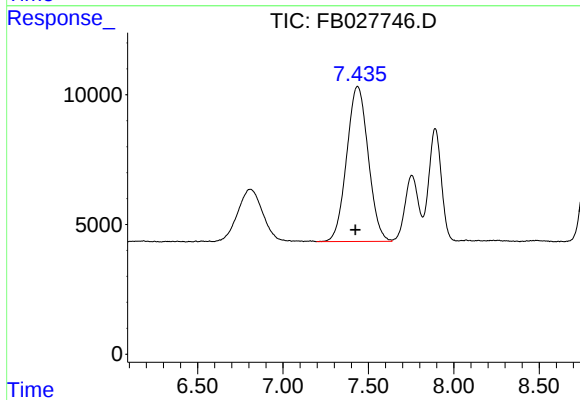


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
Delta R.T.: 0.012 min
Response: 523713
Conc: 25.24 ng/ml

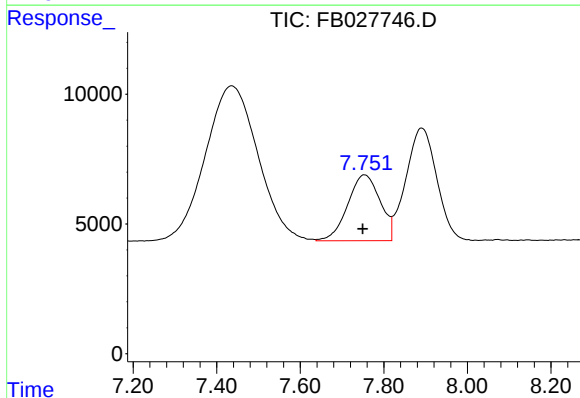


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.004 min
Response: 136577
Conc: 6.64 ng/ml

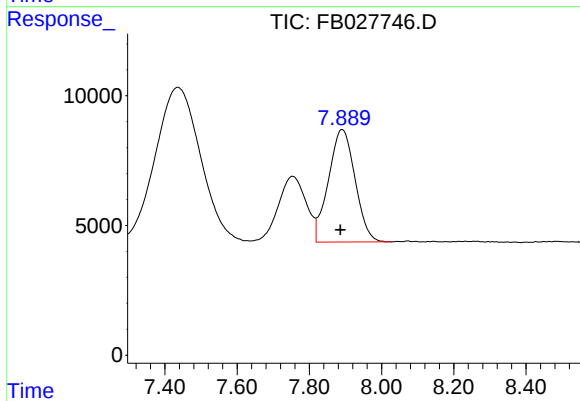

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.005 min
Response: 221761
Conc: 9.45 ng/ml

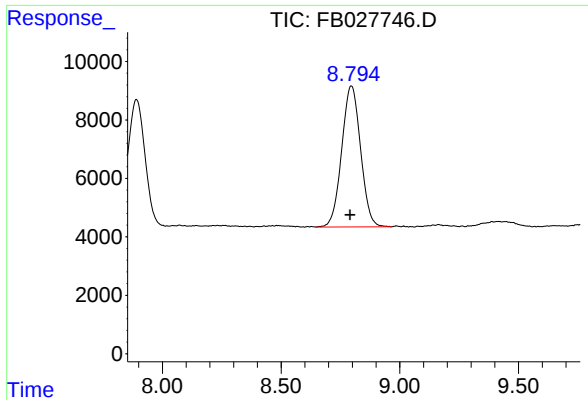

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 267028
Conc: 22.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S3

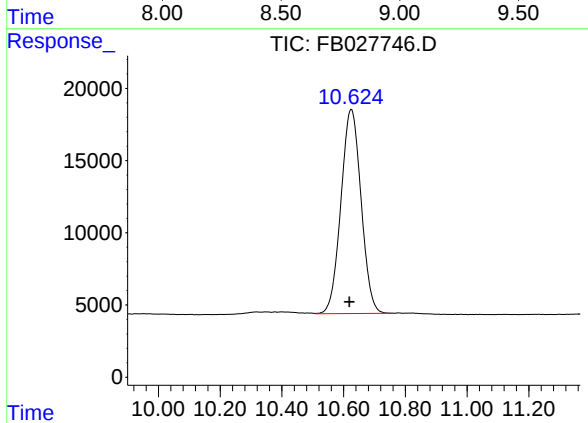


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.006 min
Response: 640967
Conc: 28.70 ng/ml

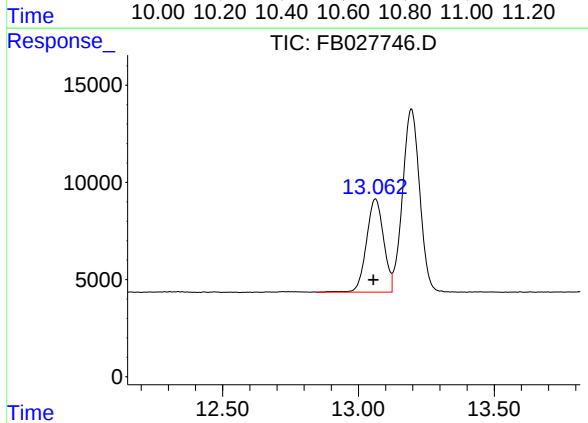


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.007 min
Response: 210434
Conc: 10.04 ng/ml

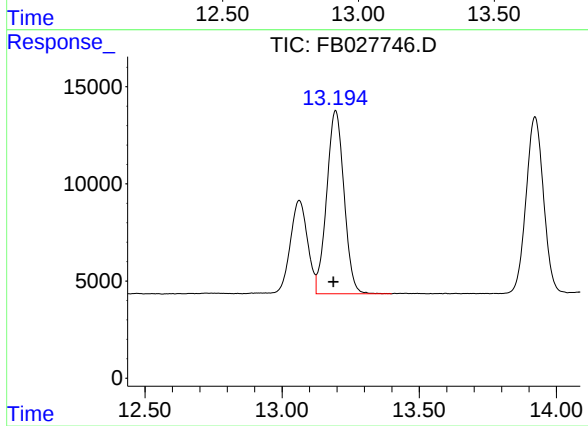

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.007 min
Response: 414338
Conc: 19.79 ng/ml

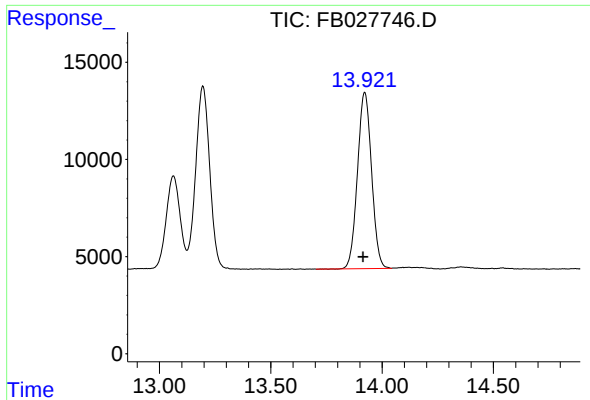

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.007 min
Response: 398138
Conc: 19.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S3

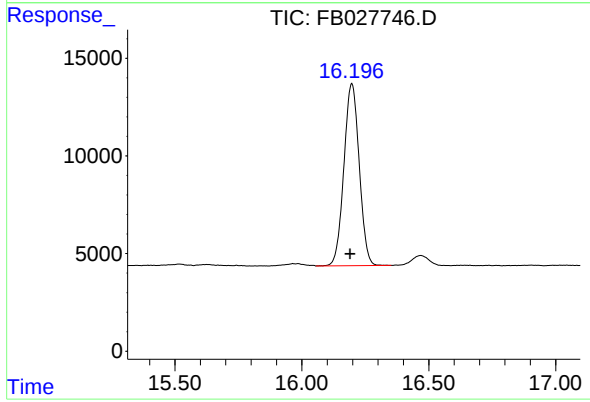

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.007 min
Response: 390670
Conc: 18.80 ng/ml