

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
 Data File : FB027747.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jul 2022 15:09
 Operator : AJ/MA
 Sample : BSF0725S4
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0725S4

Integration File: Calibration.e
 Quant Time: Jul 27 03:44:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	225529	19.378 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.720	428455	20.345 ng/ml
2) t 2,2,4-Trimethylpentane	7.438	504621	24.317 ng/ml
3) t n-Heptane	7.754	127482	6.201 ng/ml
4) t Benzene	7.893	208831	8.899 ng/ml
6) t Toluene	10.625	605818	27.130 ng/ml
7) t Ethylbenzene	13.062	194418	9.278 ng/ml
8) t m-Xylene	13.195	381468	18.219 ng/ml
9) t O-Xylene	13.922	377568	18.452 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	355901	17.126 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072522\
Data File : FB027747.D
Signal(s) : FID2B.CH
Acq On : 26 Jul 2022 15:09
Operator : AJ/MA
Sample : BSF0725S4
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0725S4

Integration File: Calibration.e
Quant Time: Jul 27 03:44:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

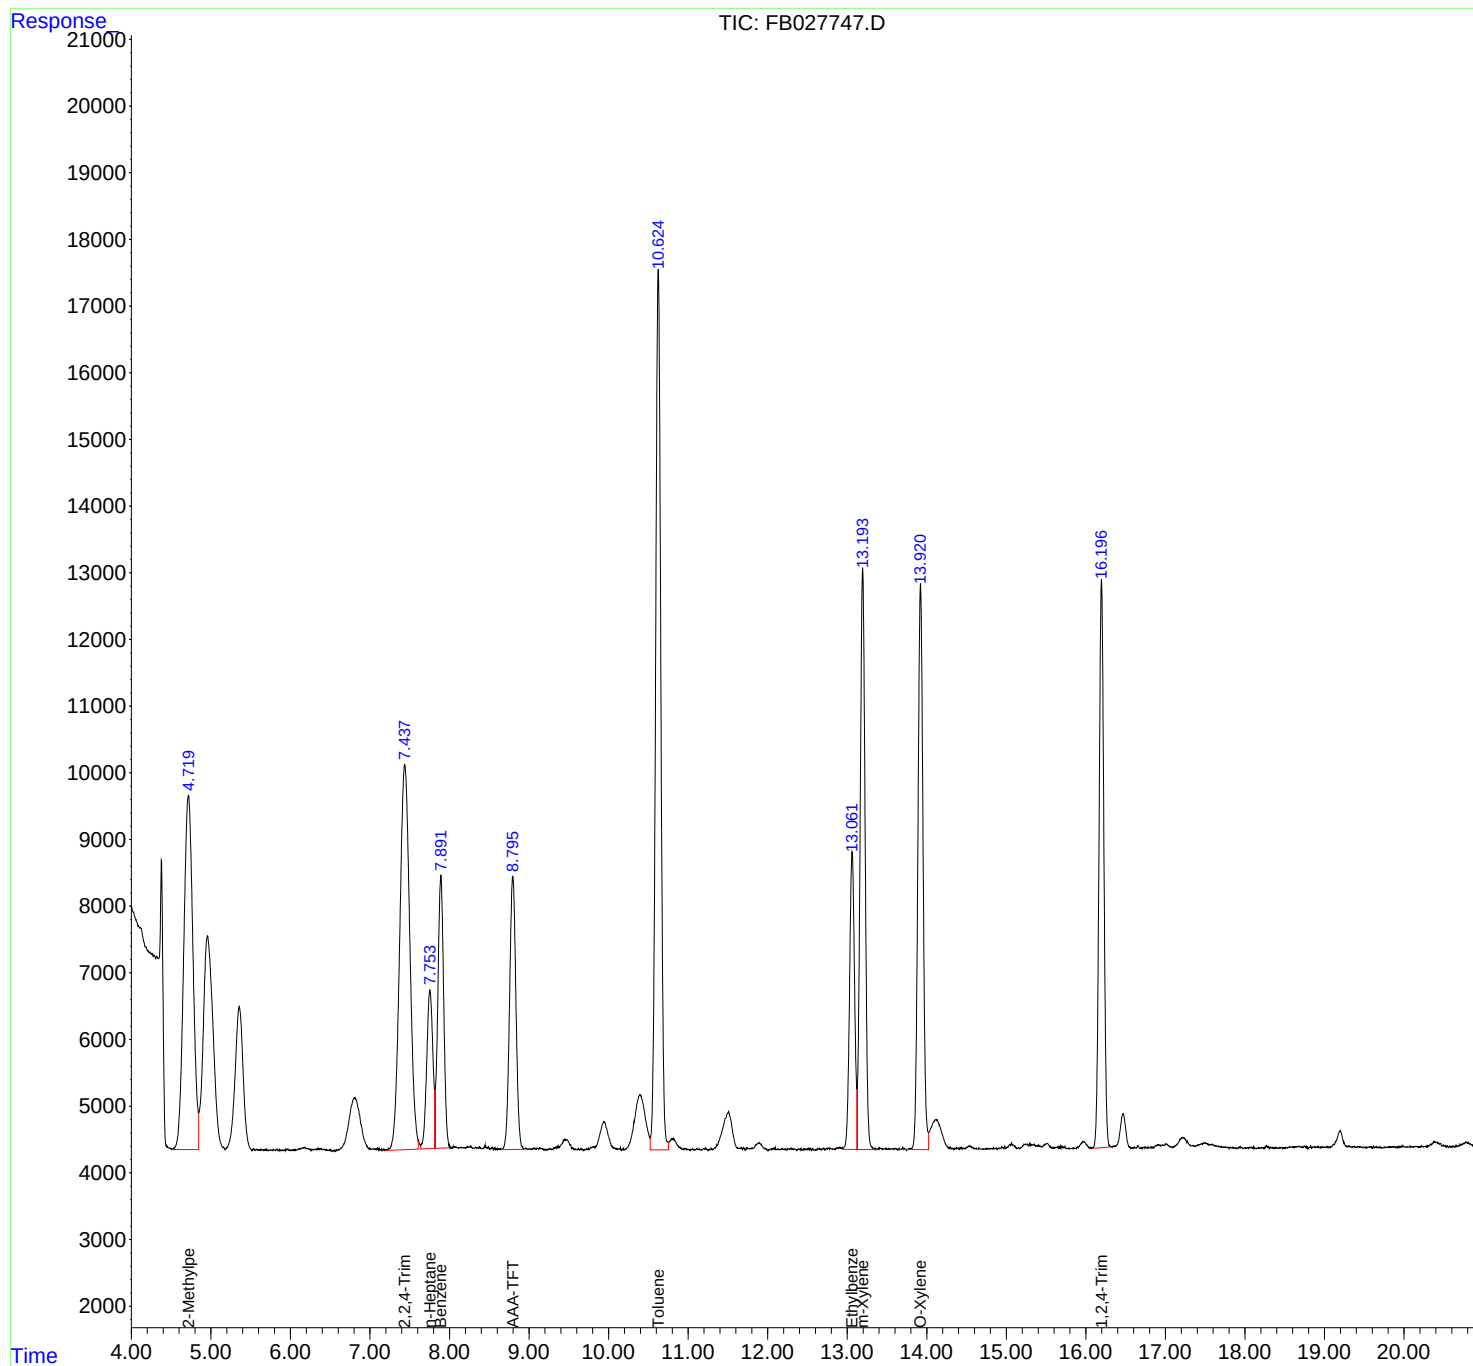


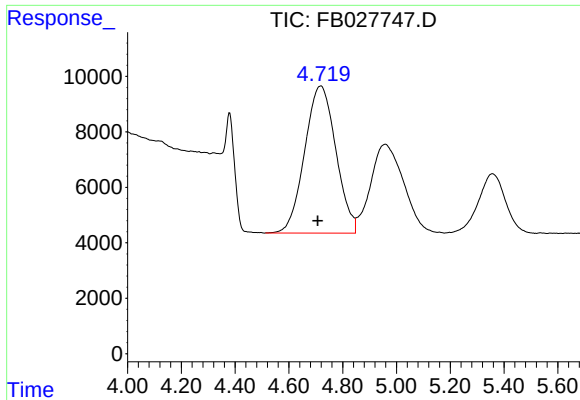

#1 2-Methylpentane


R.T.: 4.720 min
Delta R.T.: 0.013 min
Response: 428455
Conc: 20.34 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S4

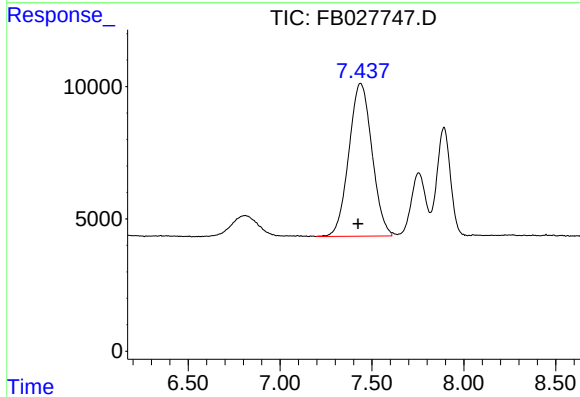


#2 2,2,4-Trimethylpentane

R.T.: 7.438 min
Delta R.T.: 0.014 min
Response: 504621
Conc: 24.32 ng/ml

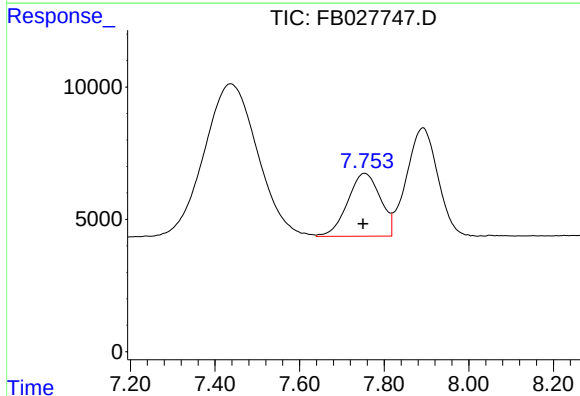


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.005 min
Response: 127482
Conc: 6.20 ng/ml

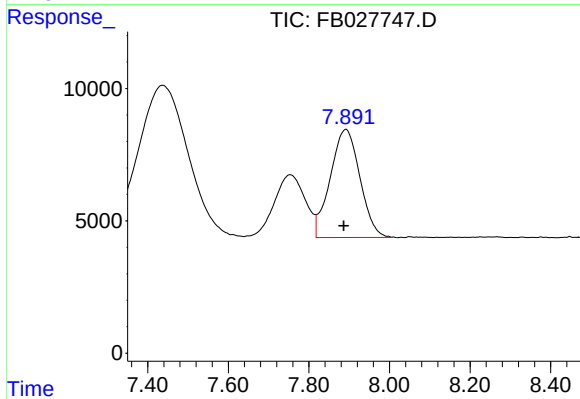

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.007 min
Response: 208831
Conc: 8.90 ng/ml

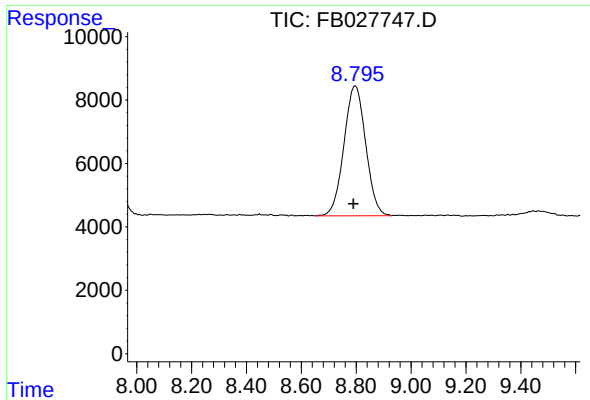

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.006 min
Response: 225529
Conc: 19.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S4

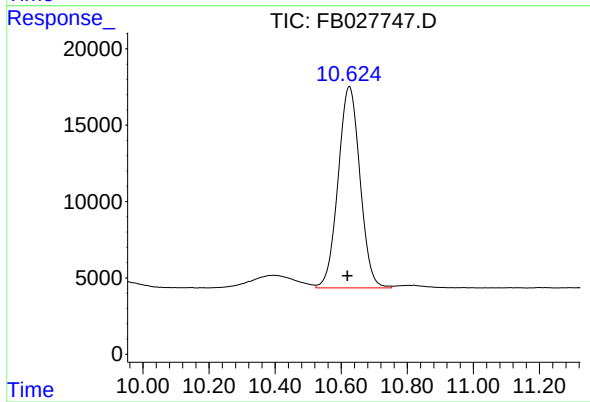


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.006 min
Response: 605818
Conc: 27.13 ng/ml

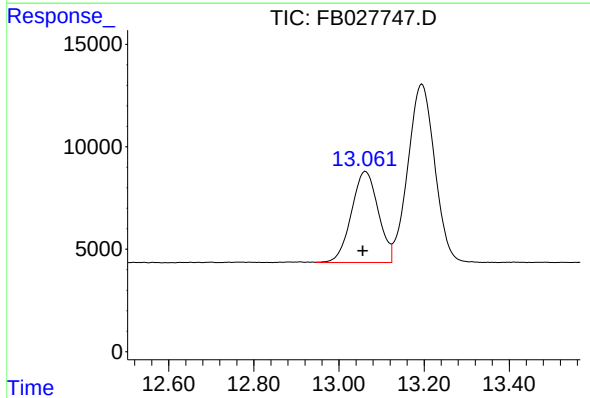


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.007 min
Response: 194418
Conc: 9.28 ng/ml

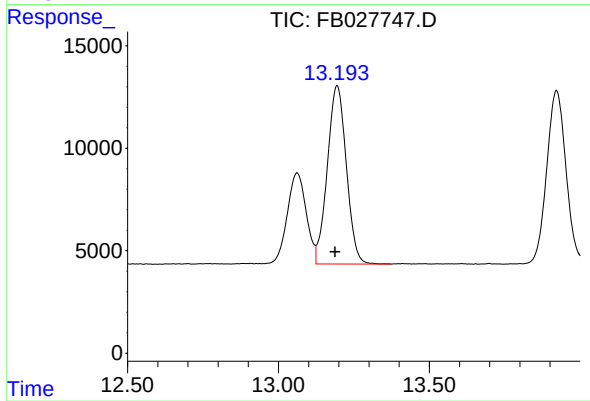

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.007 min
Response: 381468
Conc: 18.22 ng/ml

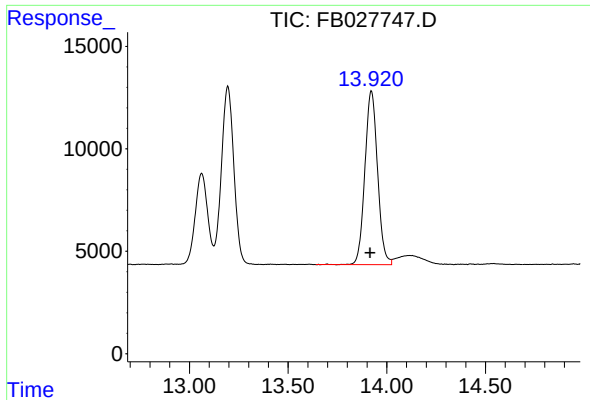

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.007 min
Response: 377568
Conc: 18.45 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S4

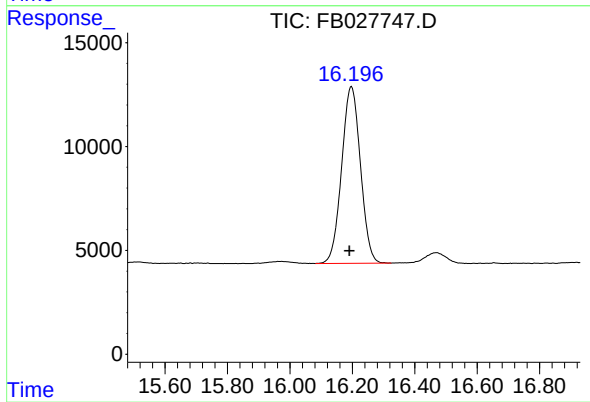

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.007 min
Response: 355901
Conc: 17.13 ng/ml