

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072523\
 Data File : FB030196.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jul 2023 13:19
 Operator : YP/AJ
 Sample : 20 PPB GRO CCC
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 26 01:15:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.789	272002	22.130 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.706	426307	25.806 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	516557	27.837 ng/ml
3) t	n-Heptane	7.748	176154	9.157 ng/ml
4) t	Benzene	7.884	216839	9.218 ng/ml
6) t	Toluene	10.616	647246	28.243 ng/ml
7) t	Ethylbenzene	13.053	200216	9.329 ng/ml
8) t	m-Xylene	13.185	392028	18.641 ng/ml
9) t	O-Xylene	13.912	381477	18.587 ng/ml
10) t	1,2,4-Trimethylbenzene	16.187	366694	18.734 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072523\
Data File : FB030196.D
Signal(s) : FID2B.CH
Acq On : 25 Jul 2023 13:19
Operator : YP/AJ
Sample : 20 PPB GRO CCC
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 26 01:15:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

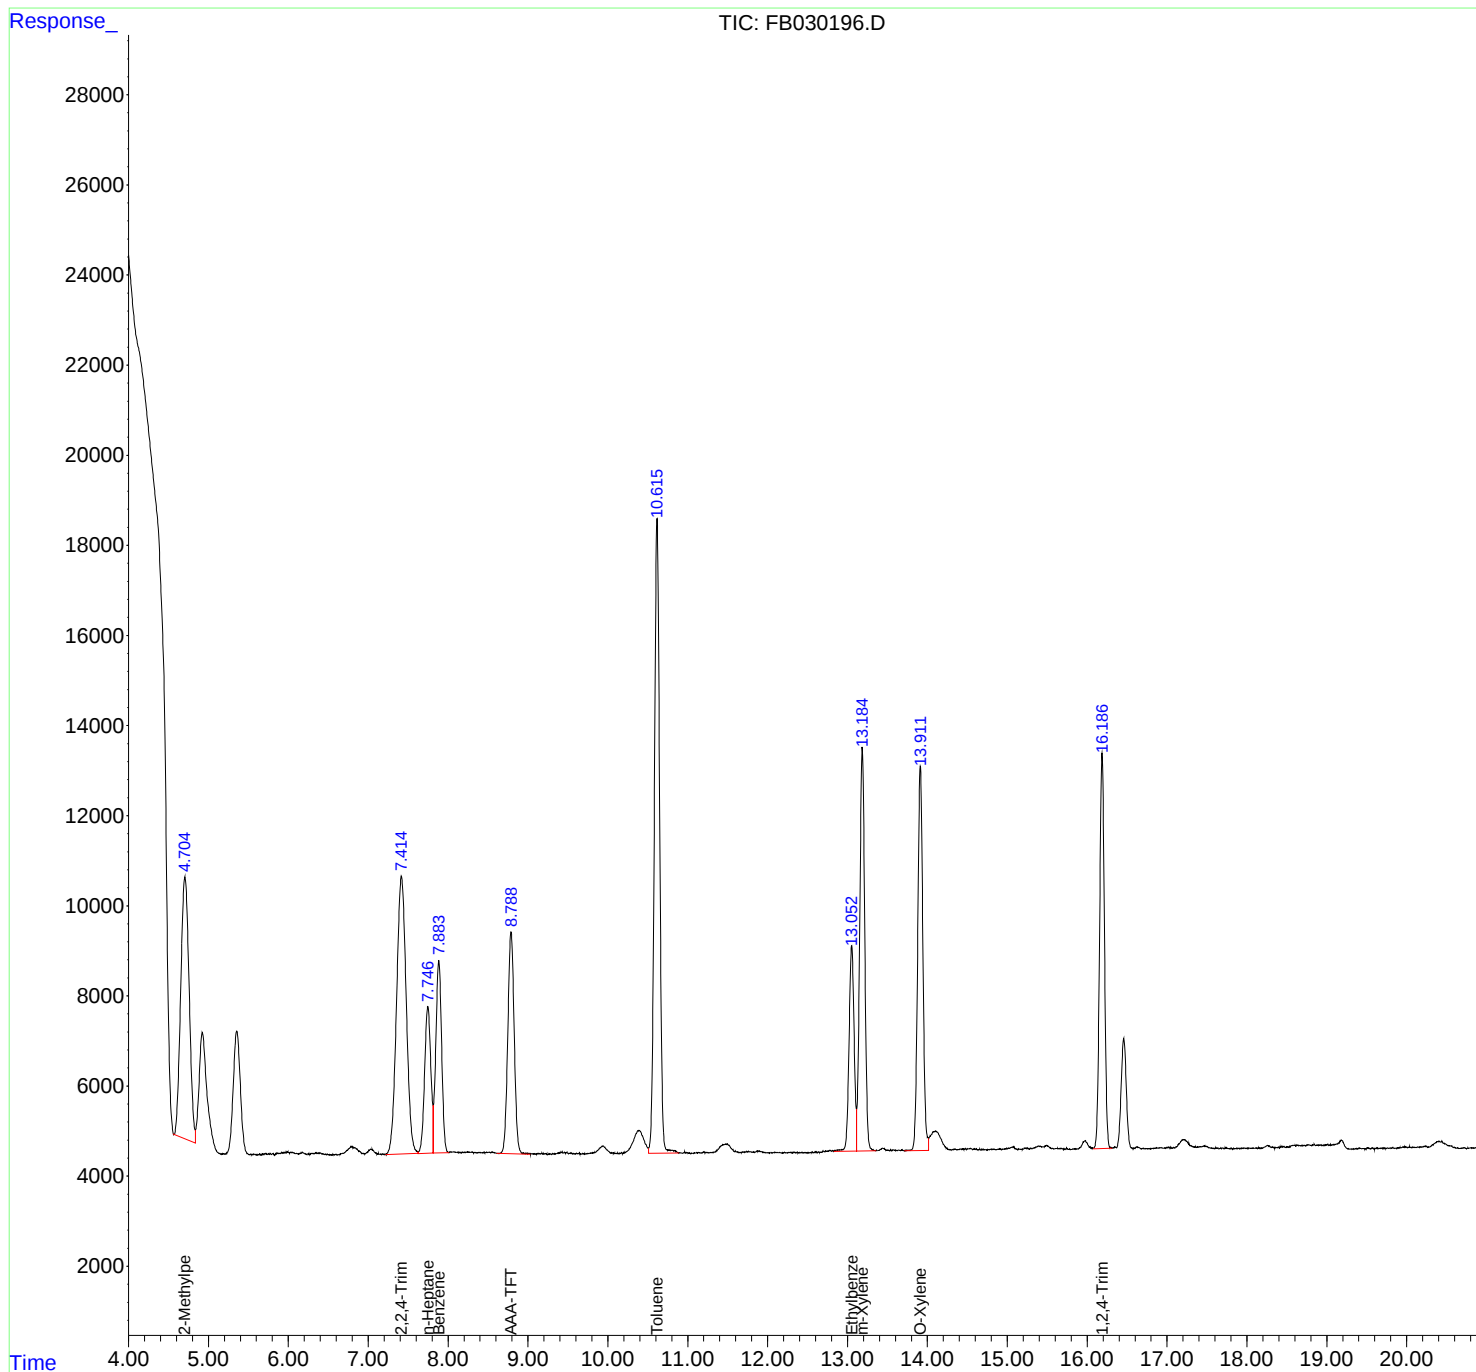

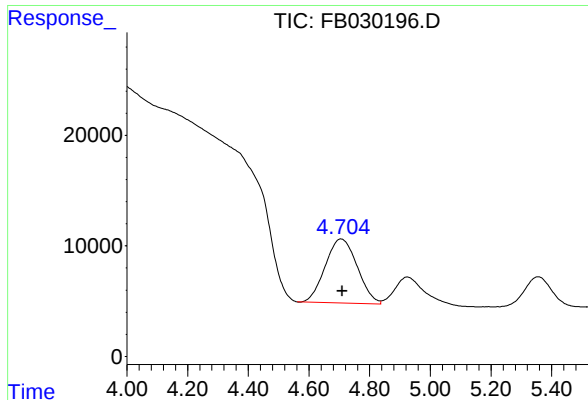


#1 2-Methylpentane

R.T.: 4.706 min
Delta R.T.: -0.004 min
Response: 426307
Conc: 25.81 ng/ml


Instrument : FID_B

ClientSampleId :

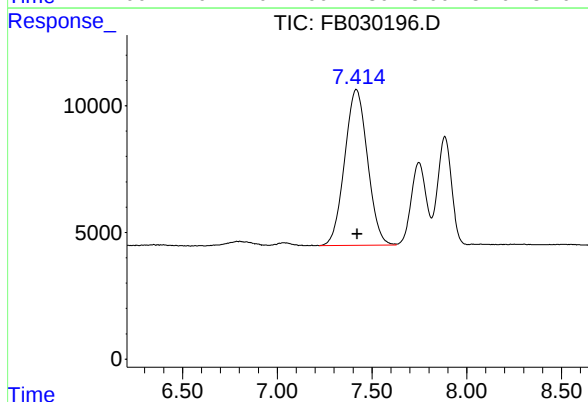


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.005 min
Response: 516557
Conc: 27.84 ng/ml

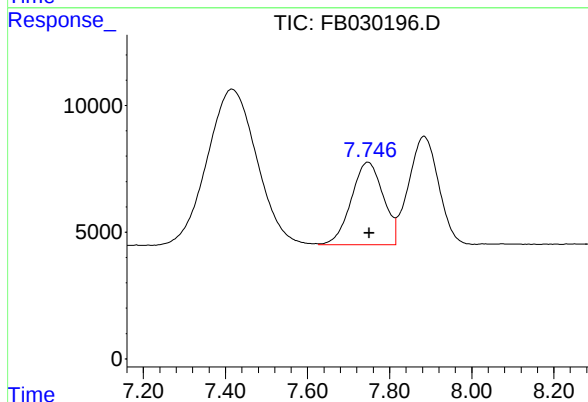


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.003 min
Response: 176154
Conc: 9.16 ng/ml

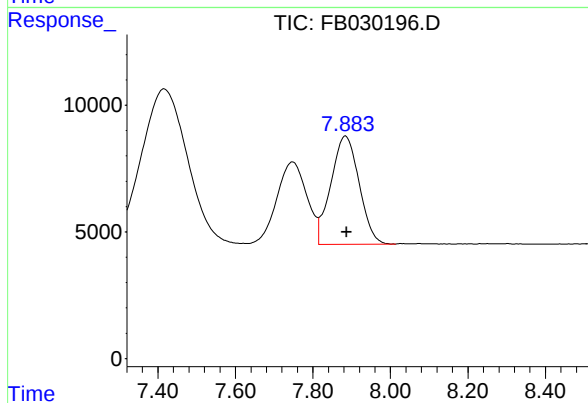

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.003 min
Response: 216839
Conc: 9.22 ng/ml

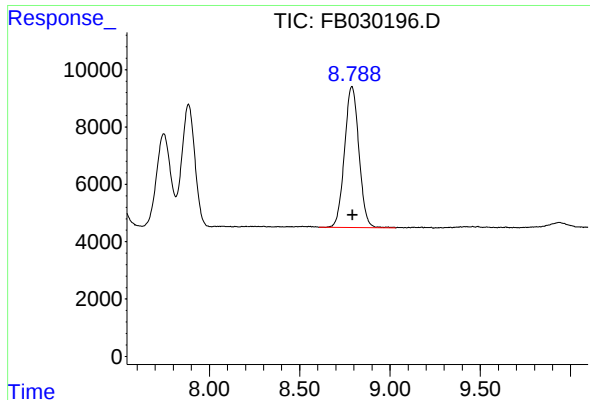

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.004 min
Response: 272002
Conc: 22.13 ng/ml

Instrument :
FID_B
ClientSampleId :

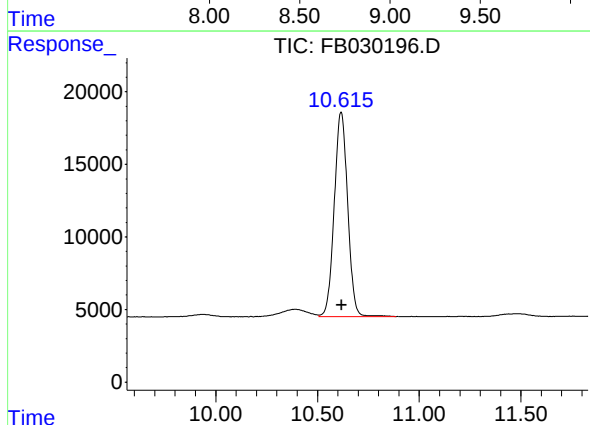


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.004 min
Response: 647246
Conc: 28.24 ng/ml

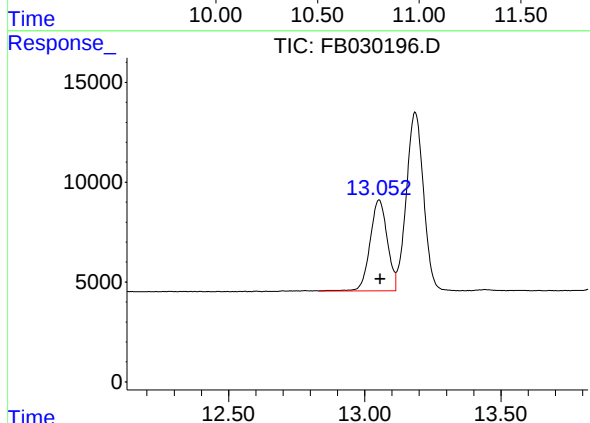


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.004 min
Response: 200216
Conc: 9.33 ng/ml

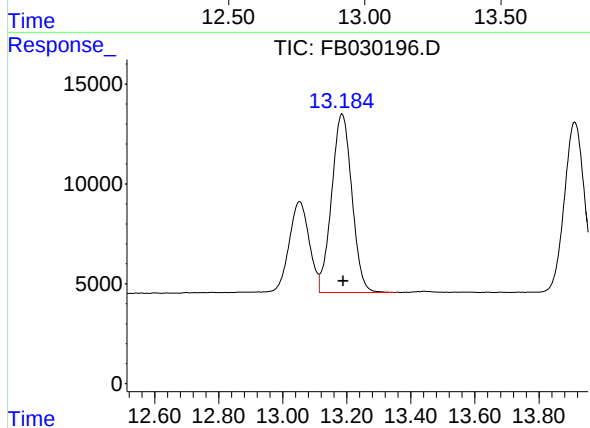

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.003 min
Response: 392028
Conc: 18.64 ng/ml

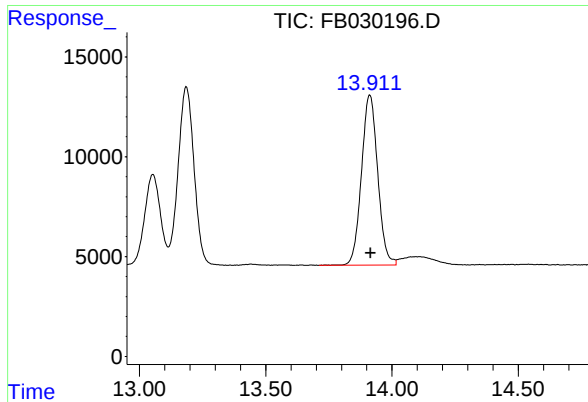

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.003 min
Response: 381477
Conc: 18.59 ng/ml

Instrument :
FID_B
ClientSampleId :

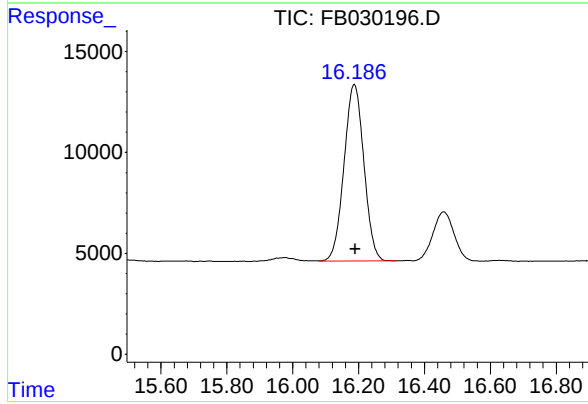

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.003 min
Response: 366694
Conc: 18.73 ng/ml