

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072523\
 Data File : FB030203.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jul 2023 18:13
 Operator : YP/AJ
 Sample : 03742-01MS 50X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-27MS

Integration File: Calibration.e
 Quant Time: Jul 26 01:16:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	247007	20.097 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	379275	22.959 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	493261	26.582 ng/ml
3) t n-Heptane	7.751	168787	8.774 ng/ml
4) t Benzene	7.888	220210	9.361 ng/ml
6) t Toluene	10.621	643755	28.091 ng/ml
7) t Ethylbenzene	13.058	198976	9.271 ng/ml
8) t m-Xylene	13.191	392121	18.646 ng/ml
9) t O-Xylene	13.917	378393	18.437 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	338425	17.290 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072523\
Data File : FB030203.D
Signal(s) : FID2B.CH
Acq On : 25 Jul 2023 18:13
Operator : YP/AJ
Sample : 03742-01MS 50X
Misc : 5.07G/5.00 ML MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WC-27MS

Integration File: Calibration.e
Quant Time: Jul 26 01:16:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

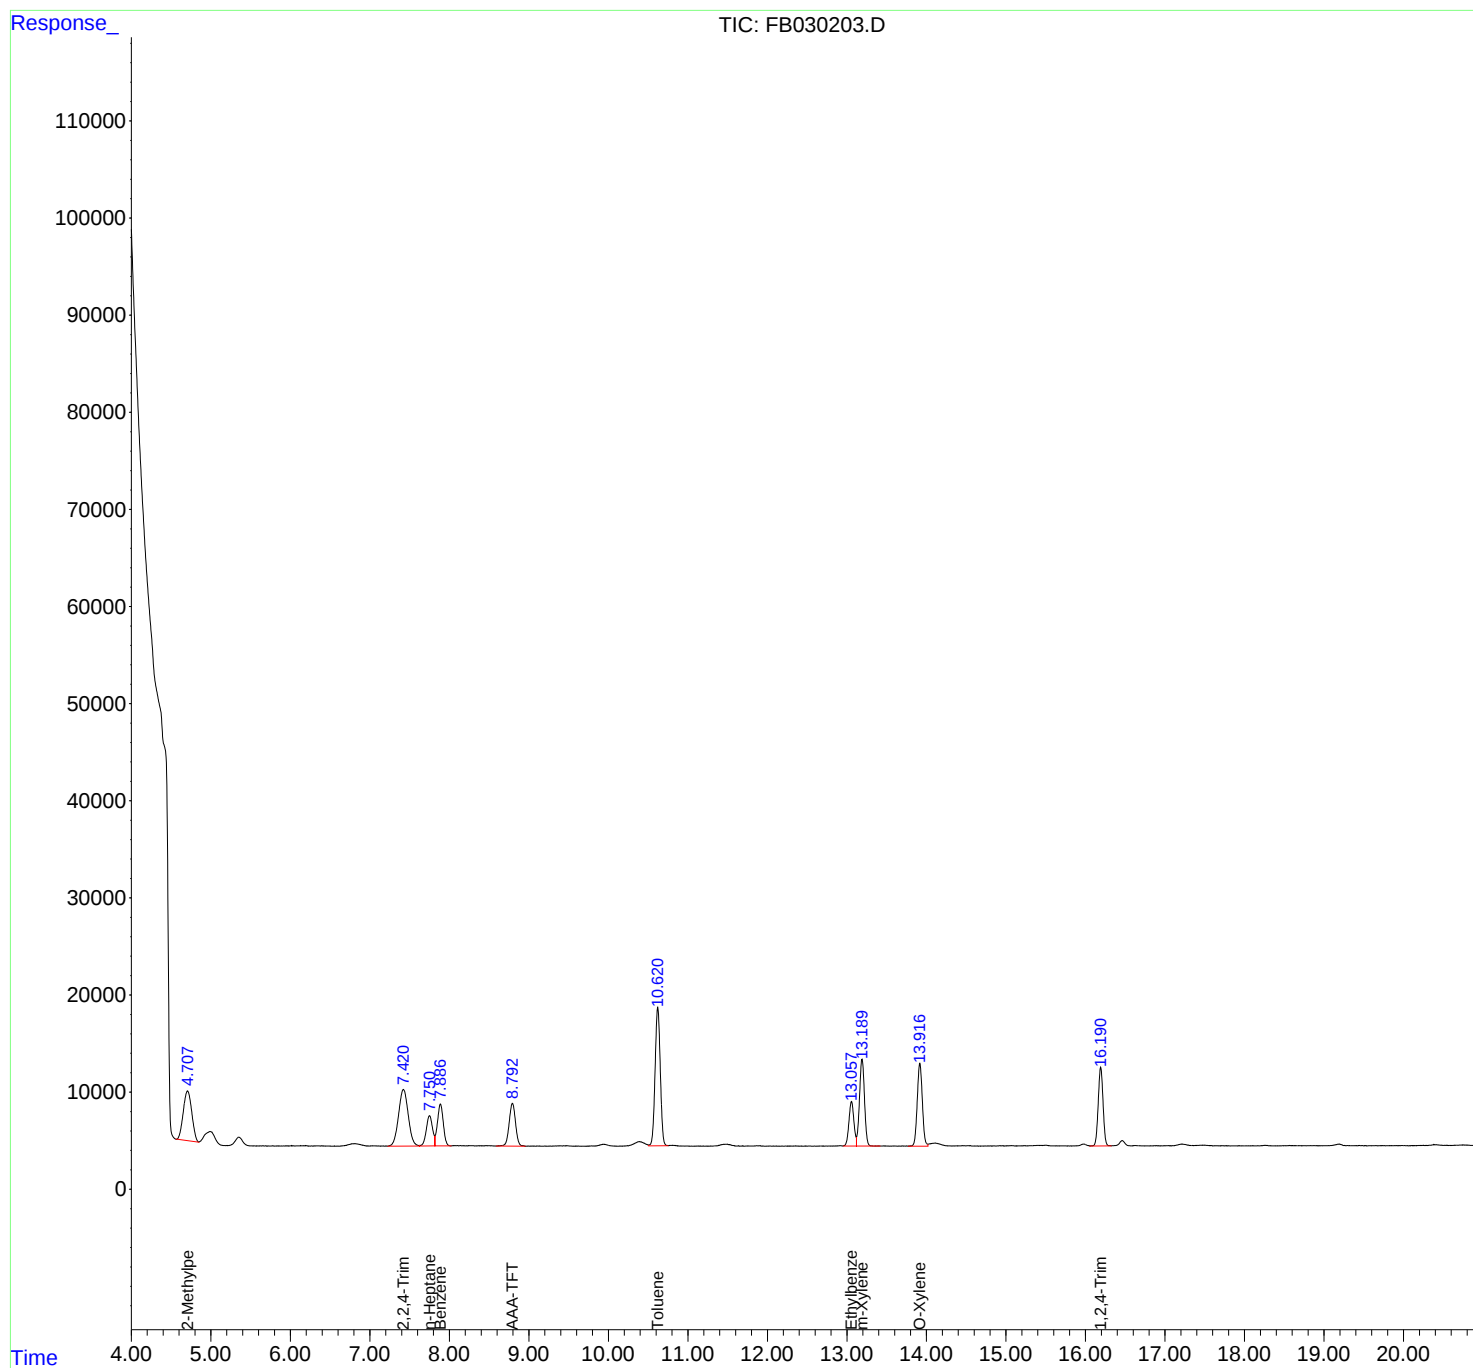


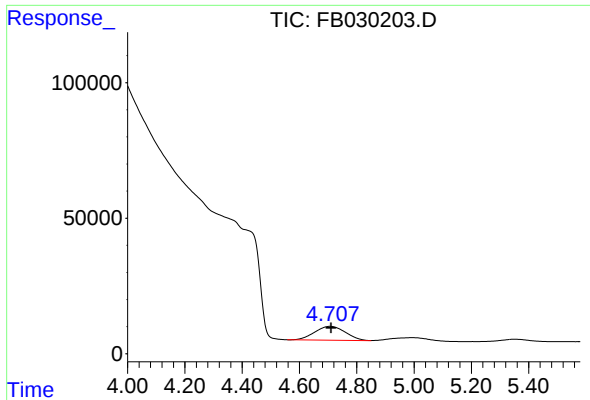

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.002 min
Response: 379275
Conc: 22.96 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-27MS

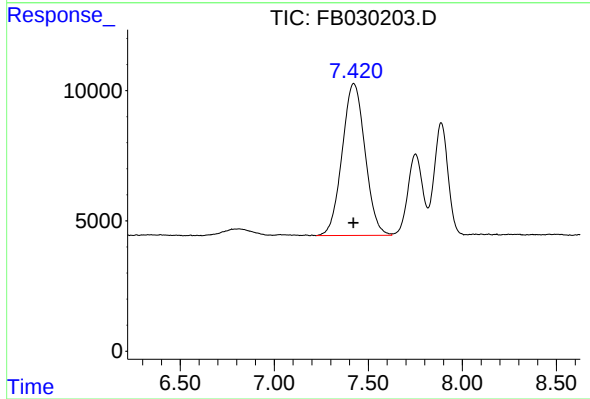


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 493261
Conc: 26.58 ng/ml

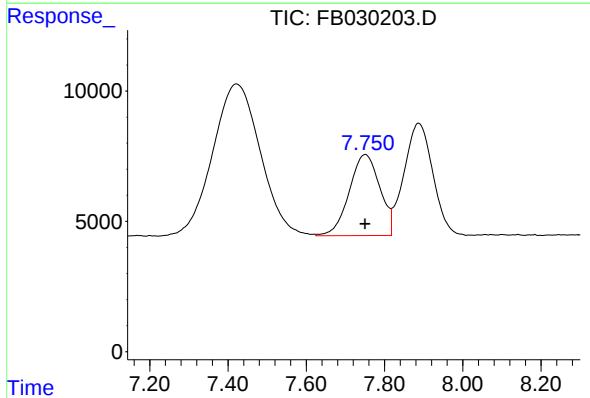


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.001 min
Response: 168787
Conc: 8.77 ng/ml

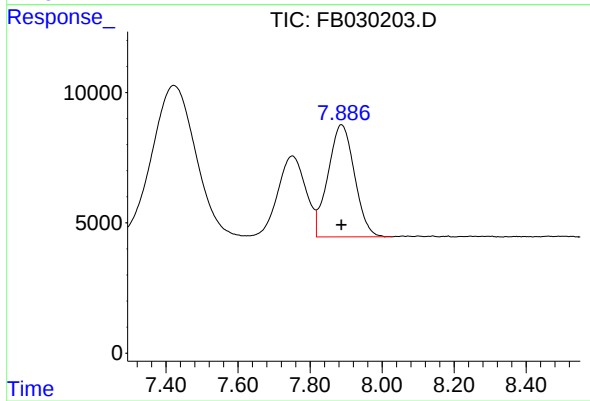

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 220210
Conc: 9.36 ng/ml

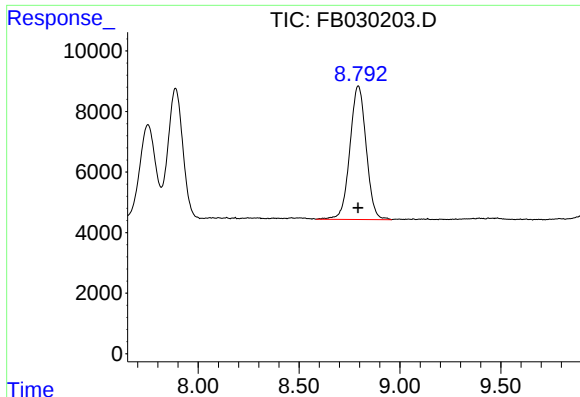

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 247007
Conc: 20.10 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-27MS

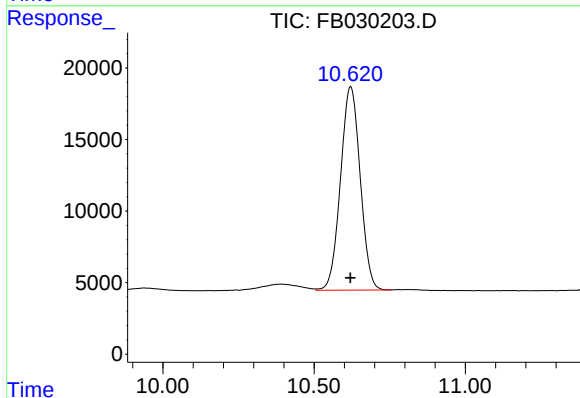


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 643755
Conc: 28.09 ng/ml

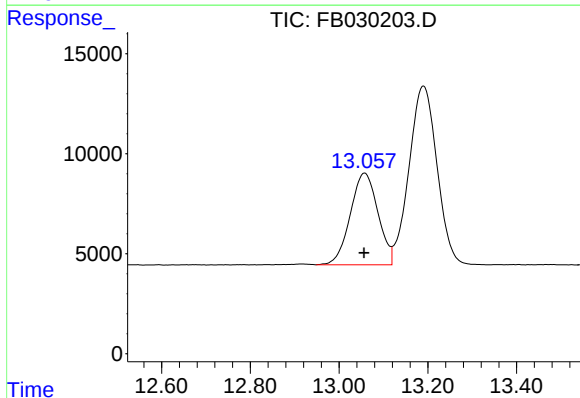


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.001 min
Response: 198976
Conc: 9.27 ng/ml

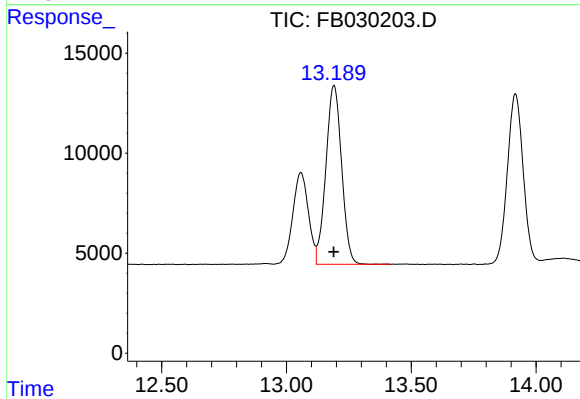

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 392121
Conc: 18.65 ng/ml

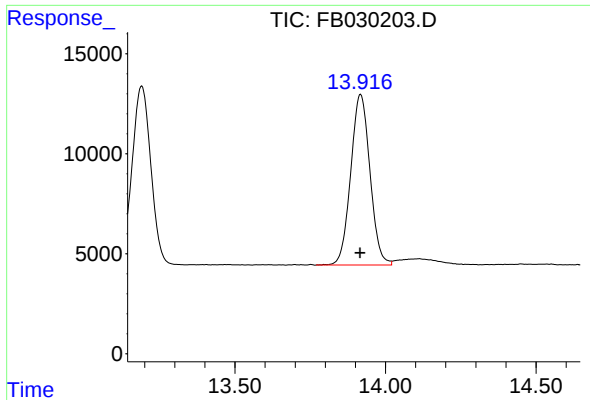

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.002 min
Response: 378393
Conc: 18.44 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-27MS

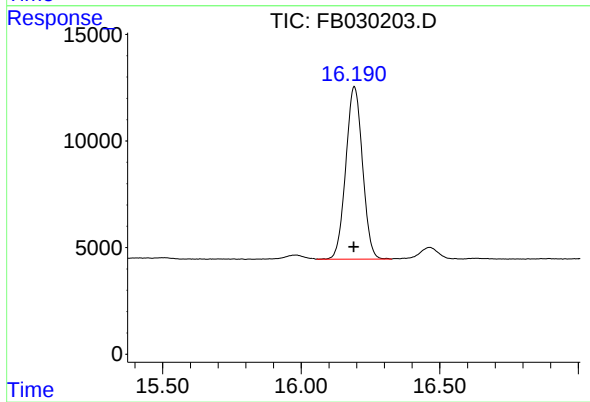

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.002 min
Response: 338425
Conc: 17.29 ng/ml