

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072523\
 Data File : FB030204.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jul 2023 18:52
 Operator : YP/AJ
 Sample : 03742-01MSD 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-27MSD

Integration File: Calibration.e
 Quant Time: Jul 26 01:16:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	216214	17.591 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	405868	24.569 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	521142	28.084 ng/ml
3) t n-Heptane	7.750	173721	9.030 ng/ml
4) t Benzene	7.887	230752	9.809 ng/ml
6) t Toluene	10.621	661940	28.884 ng/ml
7) t Ethylbenzene	13.057	205575	9.578 ng/ml
8) t m-Xylene	13.190	406298	19.320 ng/ml
9) t O-Xylene	13.917	392212	19.110 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	356658	18.222 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072523\
 Data File : FB030204.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jul 2023 18:52
 Operator : YP/AJ
 Sample : 03742-01MSD 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-27MSD

Integration File: Calibration.e
 Quant Time: Jul 26 01:16:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

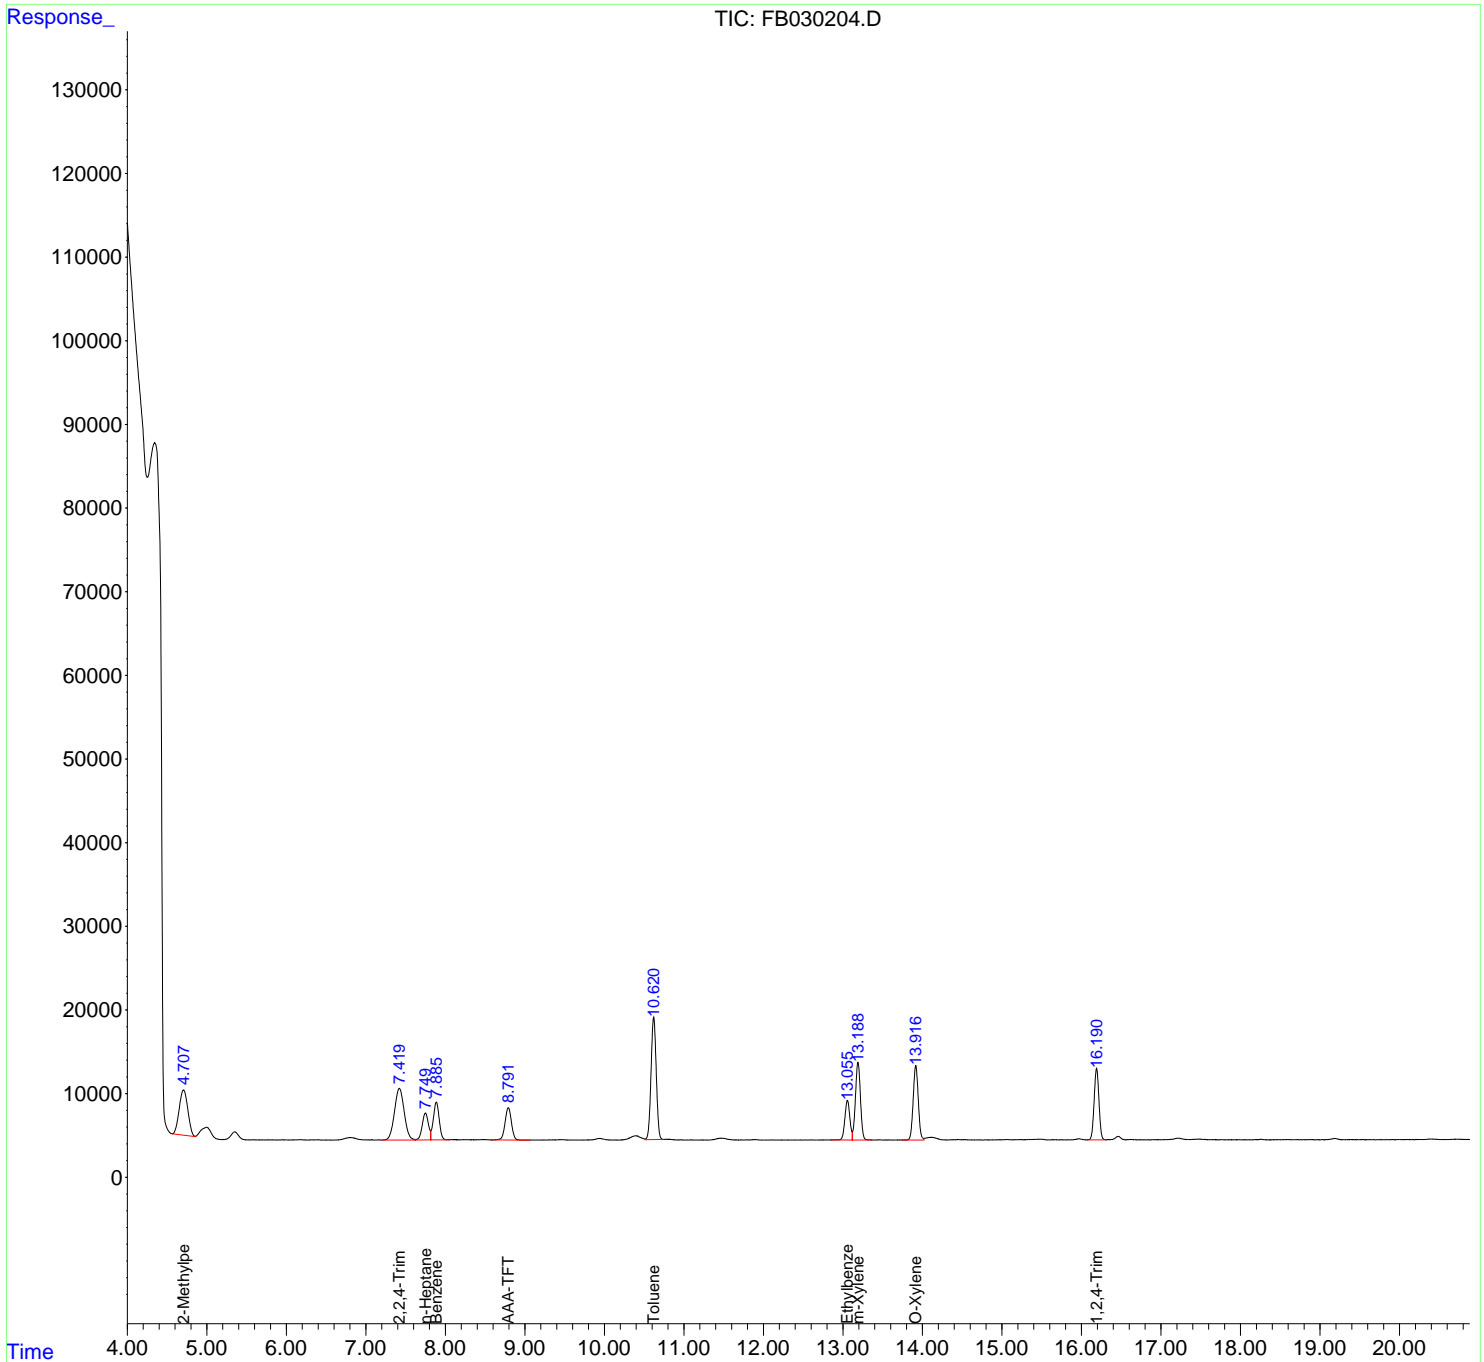


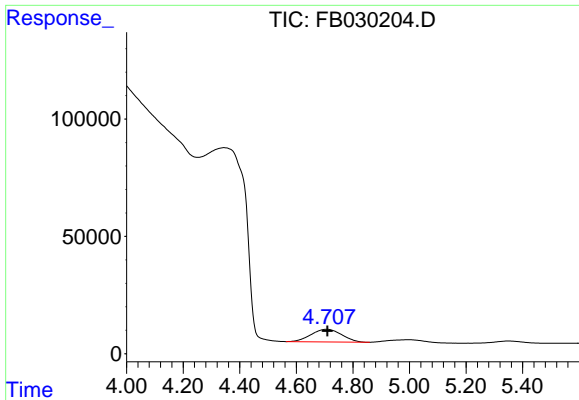

#1 2-Methylpentane


R.T.: 4.708 min
 Delta R.T.: -0.002 min
 Response: 405868
 Conc: 24.57 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 WC-27MSD

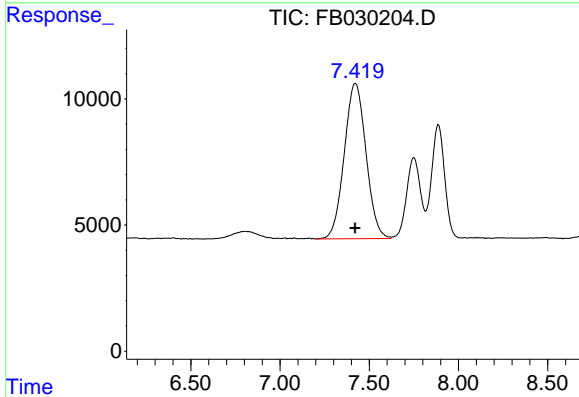


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
 Delta R.T.: 0.000 min
 Response: 521142
 Conc: 28.08 ng/ml

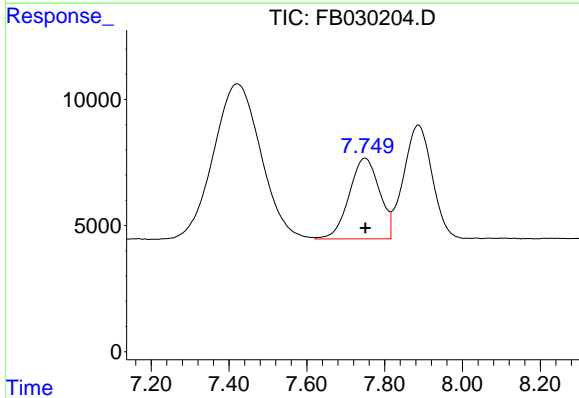


#3 n-Heptane

R.T.: 7.750 min
 Delta R.T.: 0.000 min
 Response: 173721
 Conc: 9.03 ng/ml

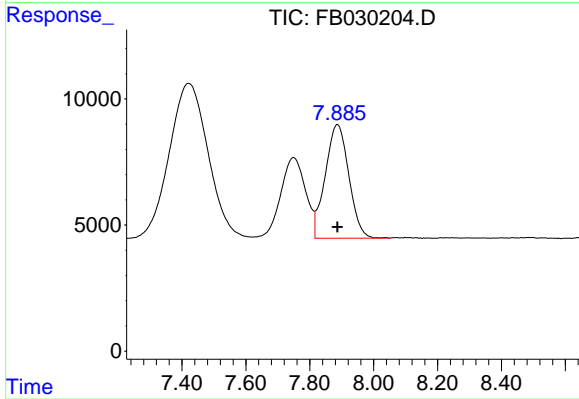

#4 Benzene


R.T.: 7.887 min
 Delta R.T.: 0.000 min
 Response: 230752
 Conc: 9.81 ng/ml

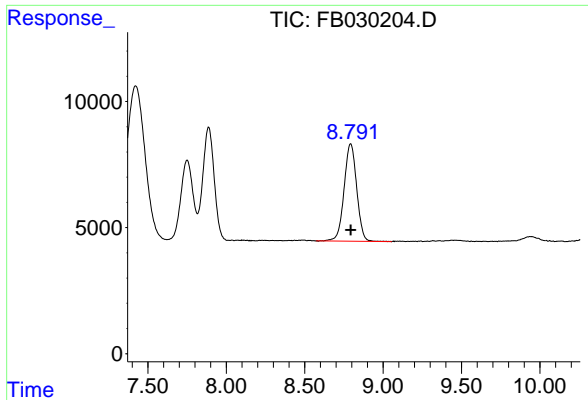

#5 AAA-TFT


R.T.: 8.793 min
 Delta R.T.: 0.000 min
 Response: 216214
 Conc: 17.59 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 WC-27MSD

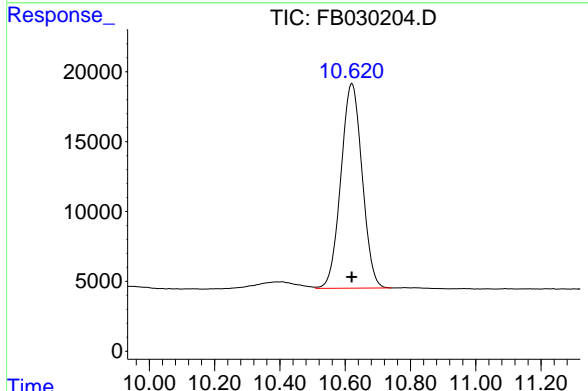


#6 Toluene

R.T.: 10.621 min
 Delta R.T.: 0.000 min
 Response: 661940
 Conc: 28.88 ng/ml

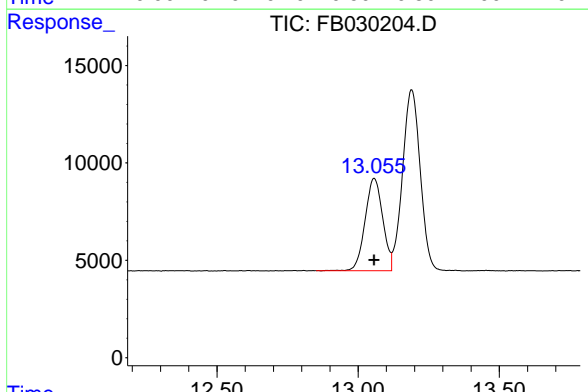


#7 Ethylbenzene

R.T.: 13.057 min
 Delta R.T.: 0.000 min
 Response: 205575
 Conc: 9.58 ng/ml

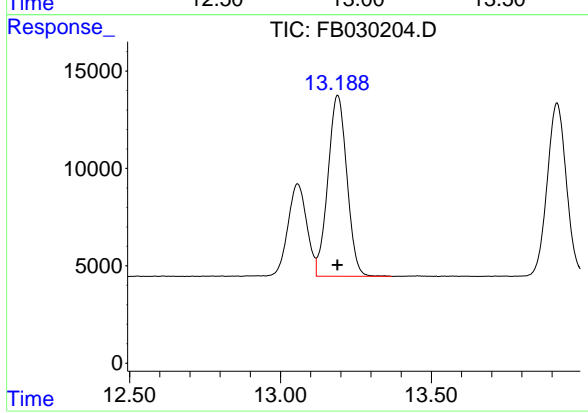

#8 m-Xylene


R.T.: 13.190 min
 Delta R.T.: 0.001 min
 Response: 406298
 Conc: 19.32 ng/ml

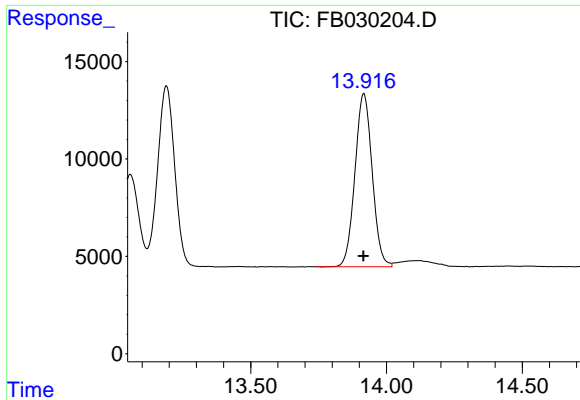

#9 O-Xylene

R.T.: 13.917 min
 Delta R.T.: 0.001 min
 Response: 392212
 Conc: 19.11 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 WC-27MSD

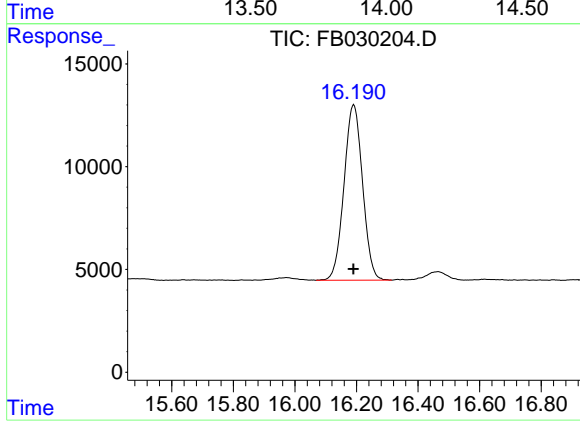

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
 Delta R.T.: 0.001 min
 Response: 356658
 Conc: 18.22 ng/ml