

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072523\
 Data File : FB030205.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jul 2023 19:32
 Operator : YP/AJ
 Sample : BSF0725S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0725S2

Integration File: Calibration.e
 Quant Time: Jul 26 01:16:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	212405	17.281 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	477066	28.879 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	549840	29.631 ng/ml
3) t n-Heptane	7.753	182055	9.463 ng/ml
4) t Benzene	7.889	225801	9.599 ng/ml
6) t Toluene	10.622	664139	28.980 ng/ml
7) t Ethylbenzene	13.058	206441	9.619 ng/ml
8) t m-Xylene	13.190	408712	19.434 ng/ml
9) t O-Xylene	13.917	396400	19.314 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	371755	18.993 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072523\
Data File : FB030205.D
Signal(s) : FID2B.CH
Acq On : 25 Jul 2023 19:32
Operator : YP/AJ
Sample : BSF0725S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0725S2

Integration File: Calibration.e
Quant Time: Jul 26 01:16:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

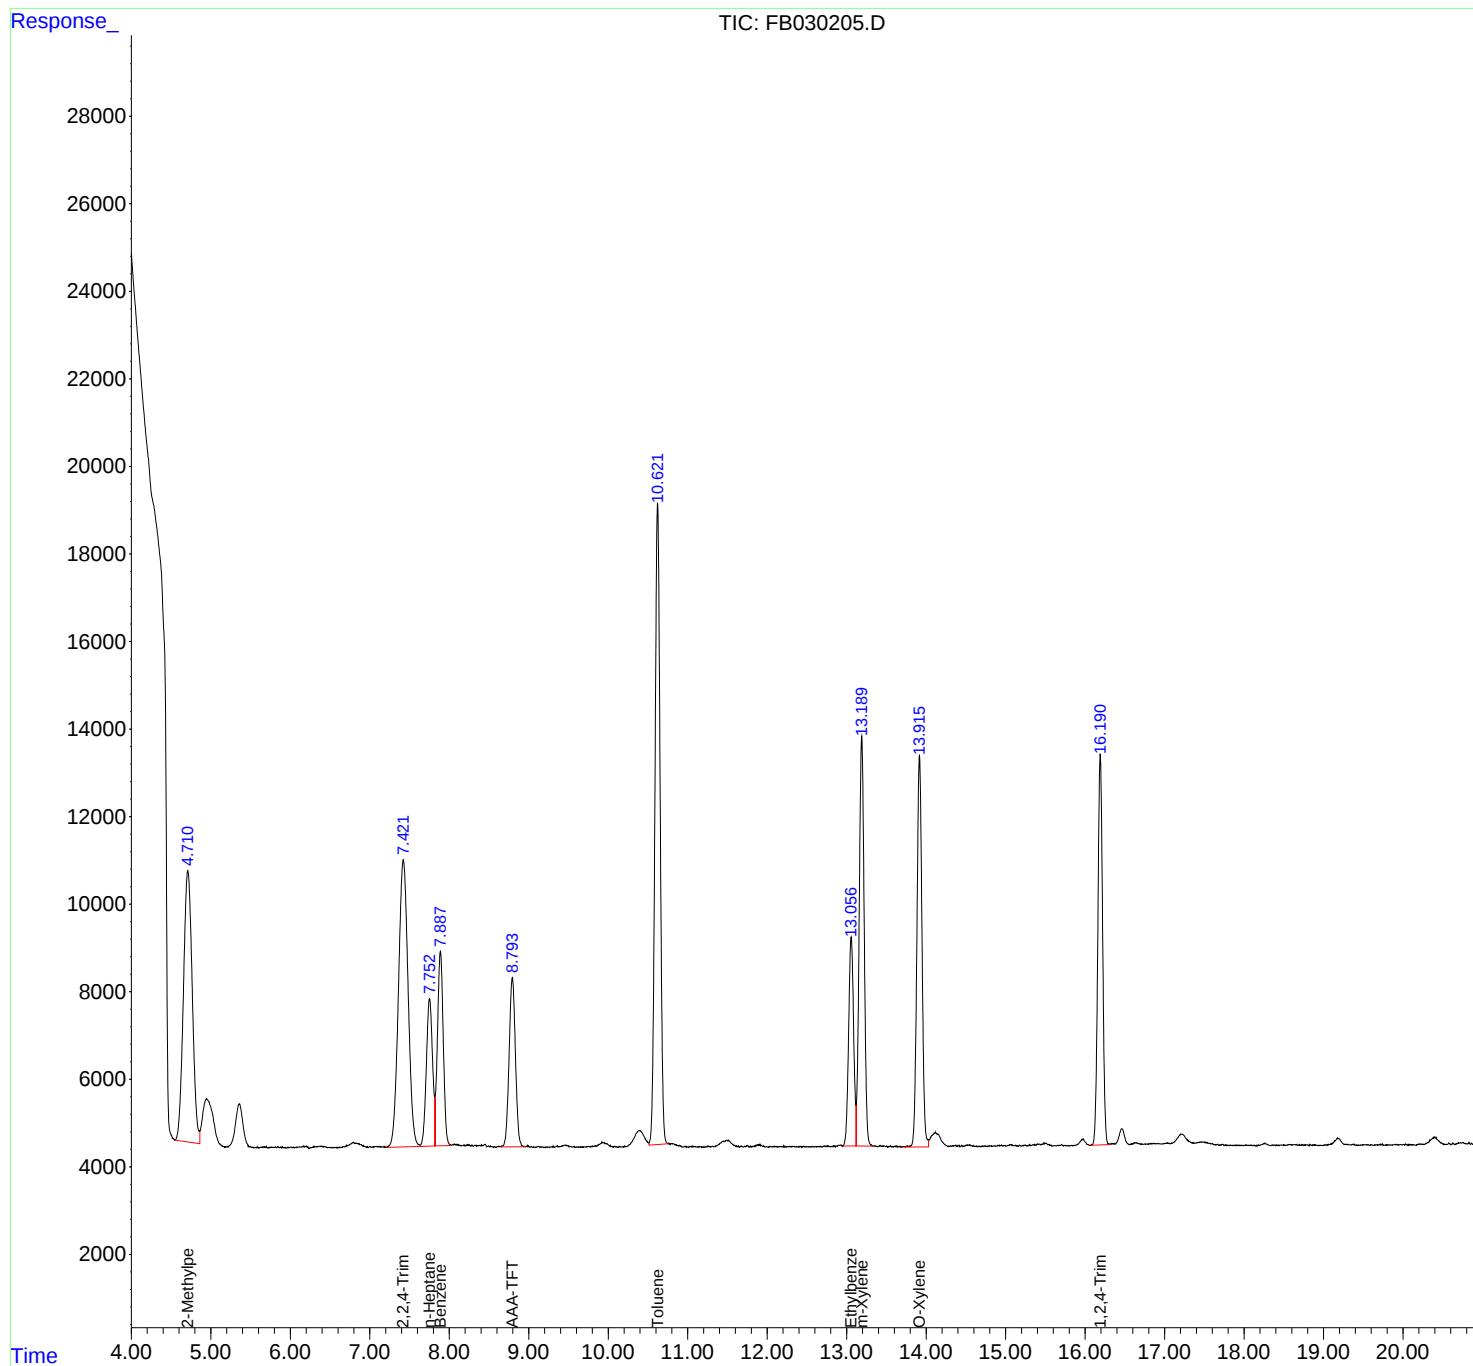


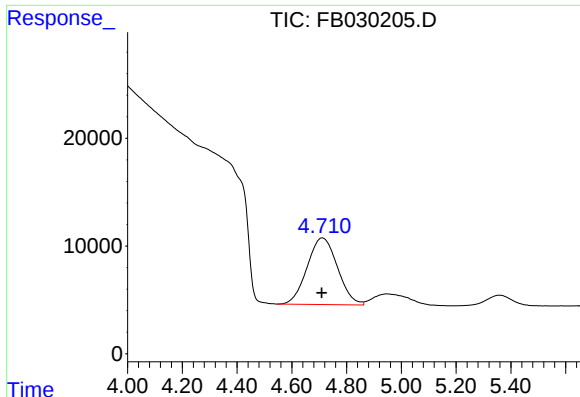

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.001 min
Response: 477066
Conc: 28.88 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S2

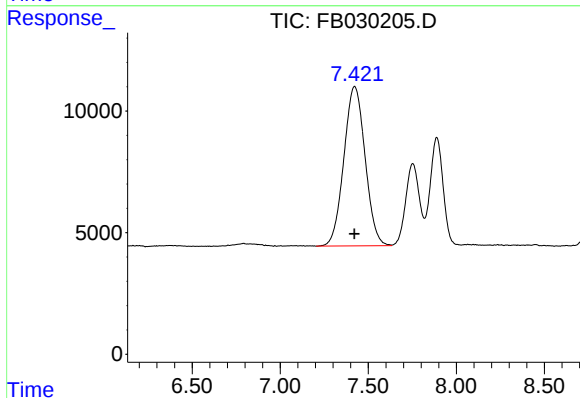


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: 0.001 min
Response: 549840
Conc: 29.63 ng/ml

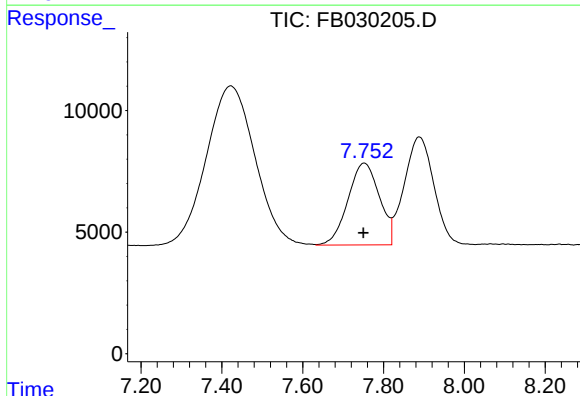


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.002 min
Response: 182055
Conc: 9.46 ng/ml

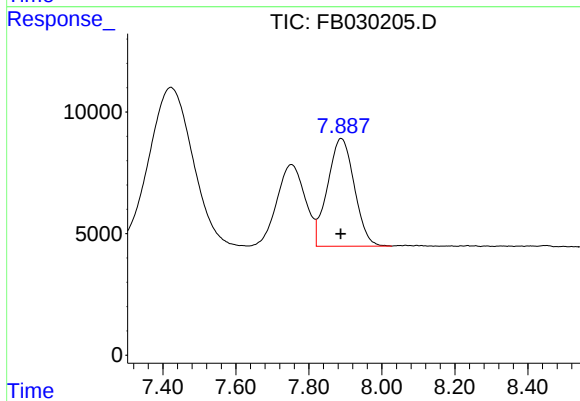

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.002 min
Response: 225801
Conc: 9.60 ng/ml

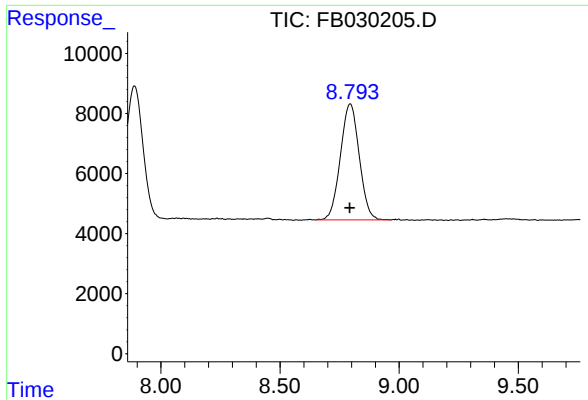

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.002 min
Response: 212405
Conc: 17.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S2

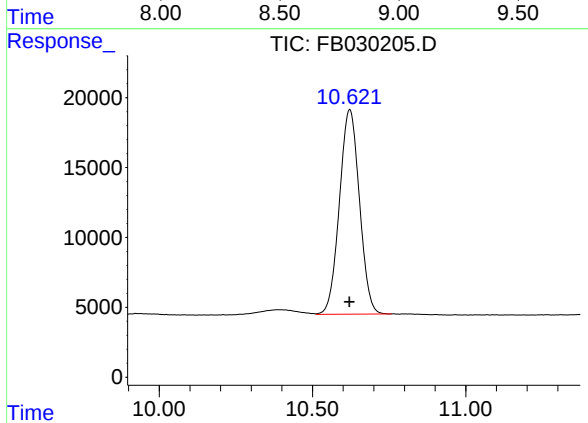


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.002 min
Response: 664139
Conc: 28.98 ng/ml

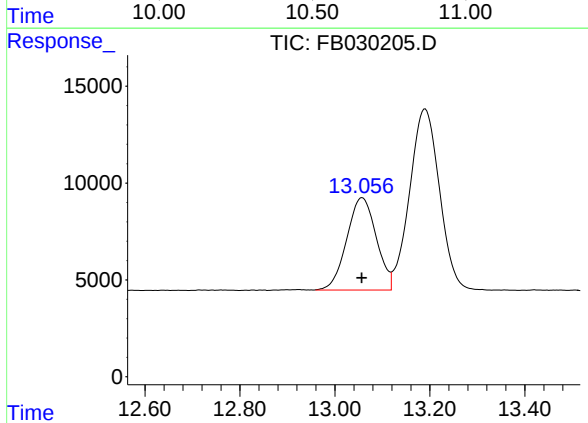


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.001 min
Response: 206441
Conc: 9.62 ng/ml

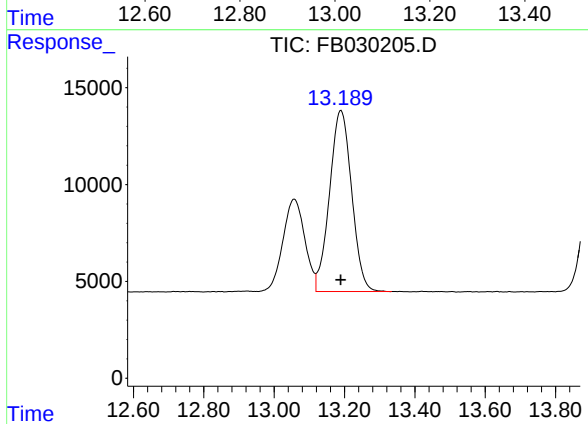

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.001 min
Response: 408712
Conc: 19.43 ng/ml

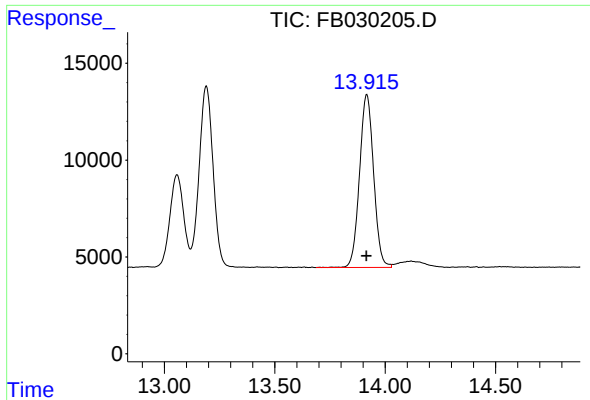

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.001 min
Response: 396400
Conc: 19.31 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S2

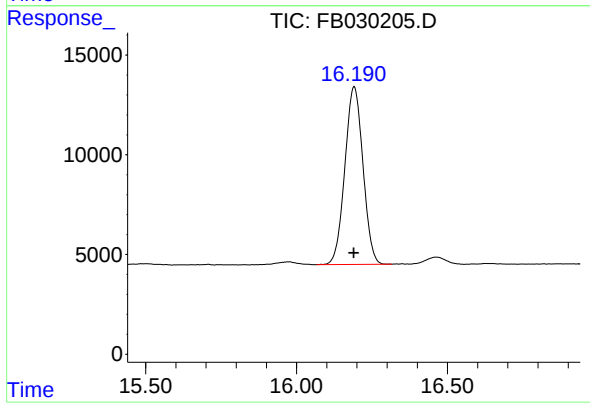

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.001 min
Response: 371755
Conc: 18.99 ng/ml