

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072523\
 Data File : FB030210.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jul 2023 23:26
 Operator : YP/AJ
 Sample : BSF0725S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0725S3

Integration File: Calibration.e
 Quant Time: Jul 26 01:16:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	249404	20.291 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	427786	25.896 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	508471	27.401 ng/ml
3) t n-Heptane	7.751	162081	8.425 ng/ml
4) t Benzene	7.887	201390	8.561 ng/ml
6) t Toluene	10.619	570329	24.887 ng/ml
7) t Ethylbenzene	13.055	181206	8.443 ng/ml
8) t m-Xylene	13.188	359402	17.090 ng/ml
9) t O-Xylene	13.915	359123	17.498 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	357361	18.258 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072523\
Data File : FB030210.D
Signal(s) : FID2B.CH
Acq On : 25 Jul 2023 23:26
Operator : YP/AJ
Sample : BSF0725S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0725S3

Integration File: Calibration.e
Quant Time: Jul 26 01:16:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

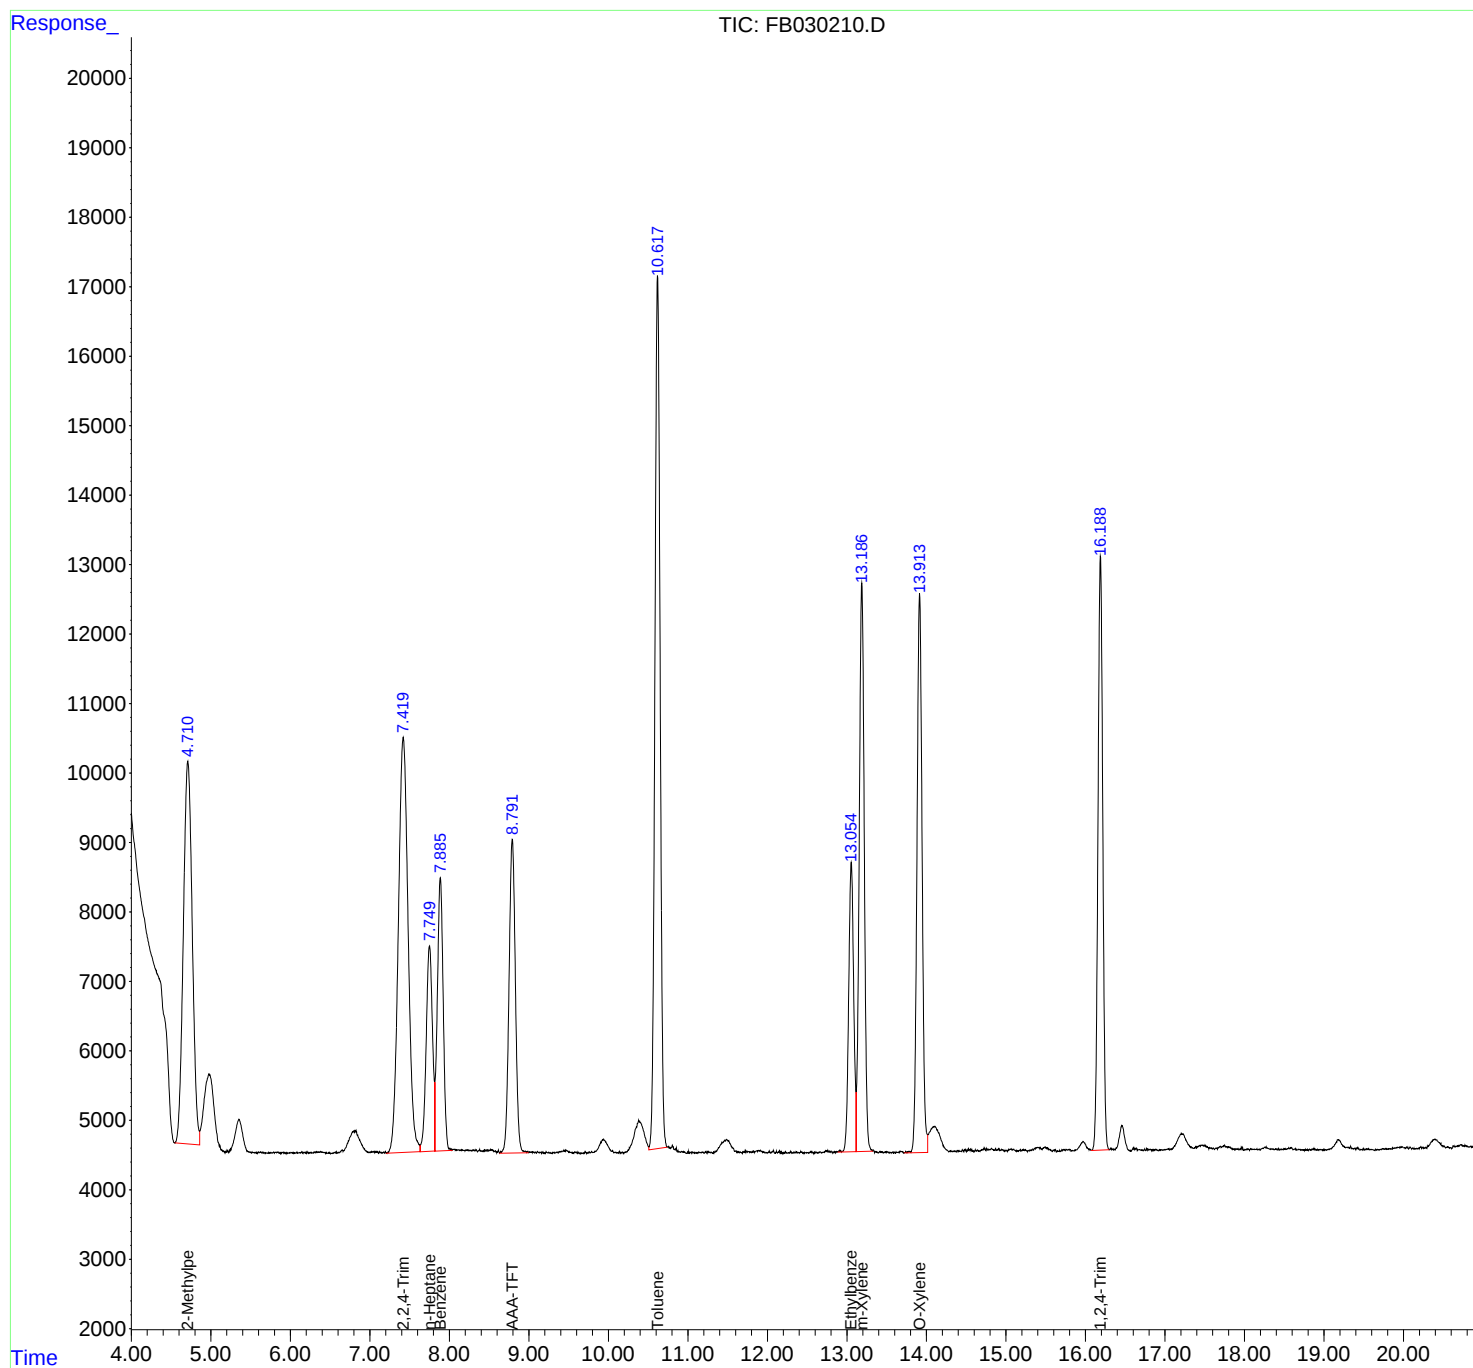


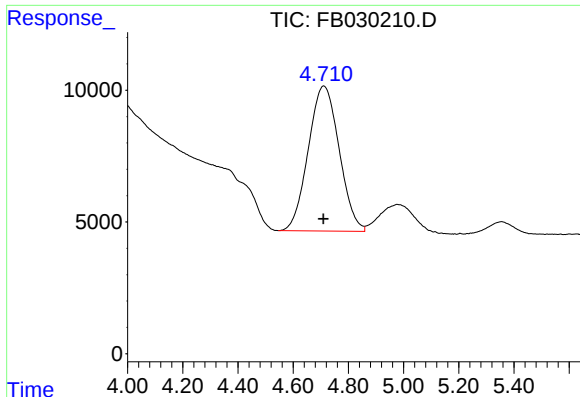

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 427786
Conc: 25.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S3

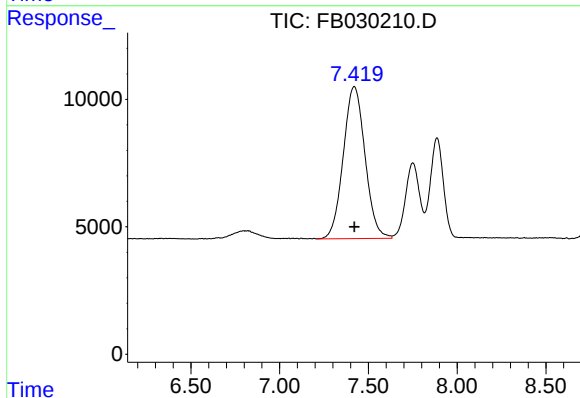


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 508471
Conc: 27.40 ng/ml

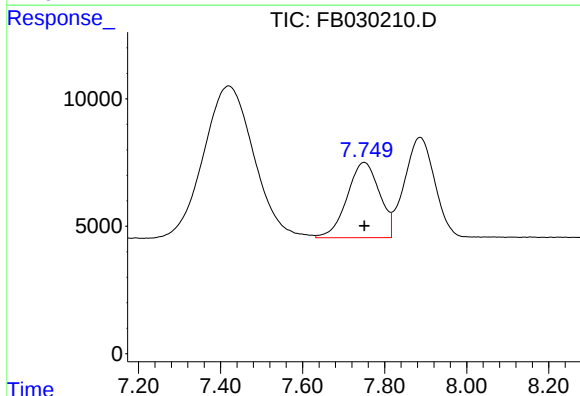


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 162081
Conc: 8.42 ng/ml

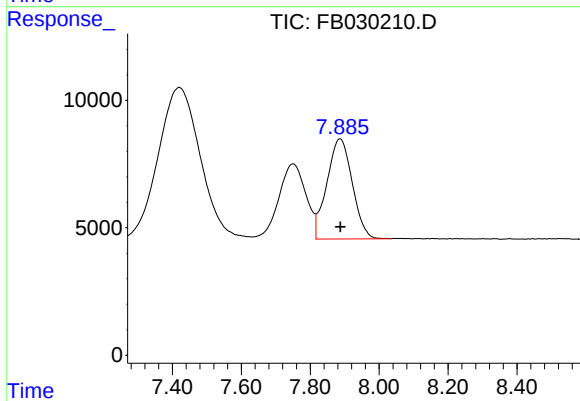

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 201390
Conc: 8.56 ng/ml

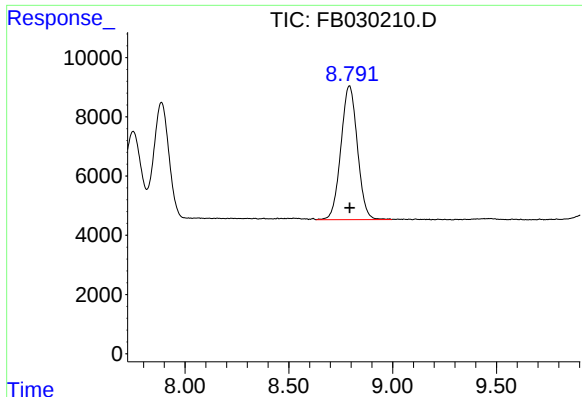

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 249404
Conc: 20.29 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S3

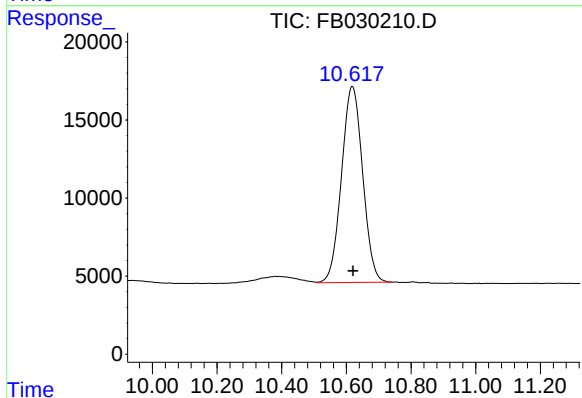


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.001 min
Response: 570329
Conc: 24.89 ng/ml

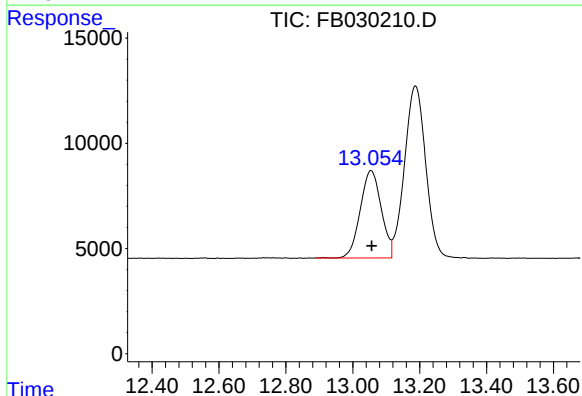


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.001 min
Response: 181206
Conc: 8.44 ng/ml

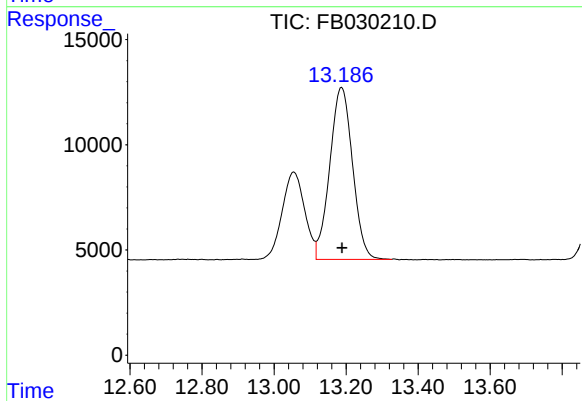

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.001 min
Response: 359402
Conc: 17.09 ng/ml

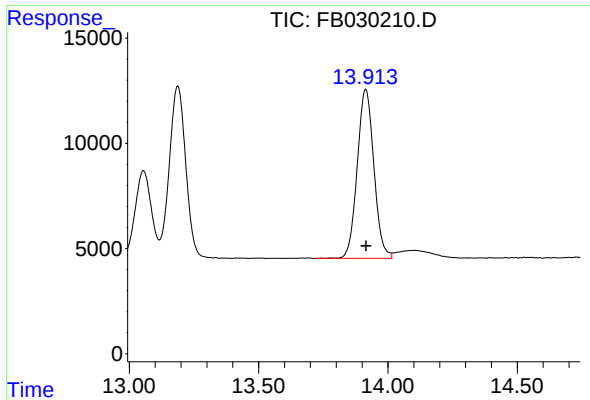

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.001 min
Response: 359123
Conc: 17.50 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0725S3

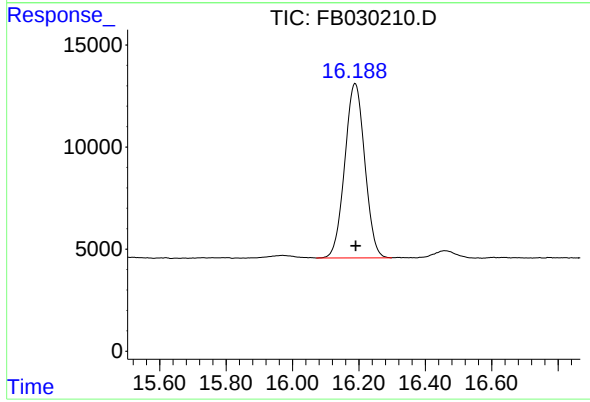

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: 0.000 min
Response: 357361
Conc: 18.26 ng/ml