

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072619\
 Data File : FB021817.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jul 2019 15:21
 Operator : DD/AJ
 Sample : K3620-11MS
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 26 23:28:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.990	312348	22.888 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.859	721479	26.163 ng/ml
2) t	2,2,4-Trimethylpentane	7.610	717502	27.143 ng/ml
3) t	n-Heptane	7.950	216603	8.736 ng/ml
4) t	Benzene	8.084	296325	10.143 ng/ml
6) t	Toluene	10.831	598587	29.091 ng/ml
7) t	Ethylbenzene	13.276	206323	9.917 ng/ml
8) t	m-Xylene	13.409	437952	19.714 ng/ml
9) t	O-Xylene	14.138	454308	19.750 ng/ml
10) t	1,2,4-Trimethylbenzene	16.418	451403	19.146 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072619\
Data File : FB021817.D
Signal(s) : FID2B.CH
Acq On : 26 Jul 2019 15:21
Operator : DD/AJ
Sample : K3620-11MS
Misc : 5.02/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 26 23:28:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

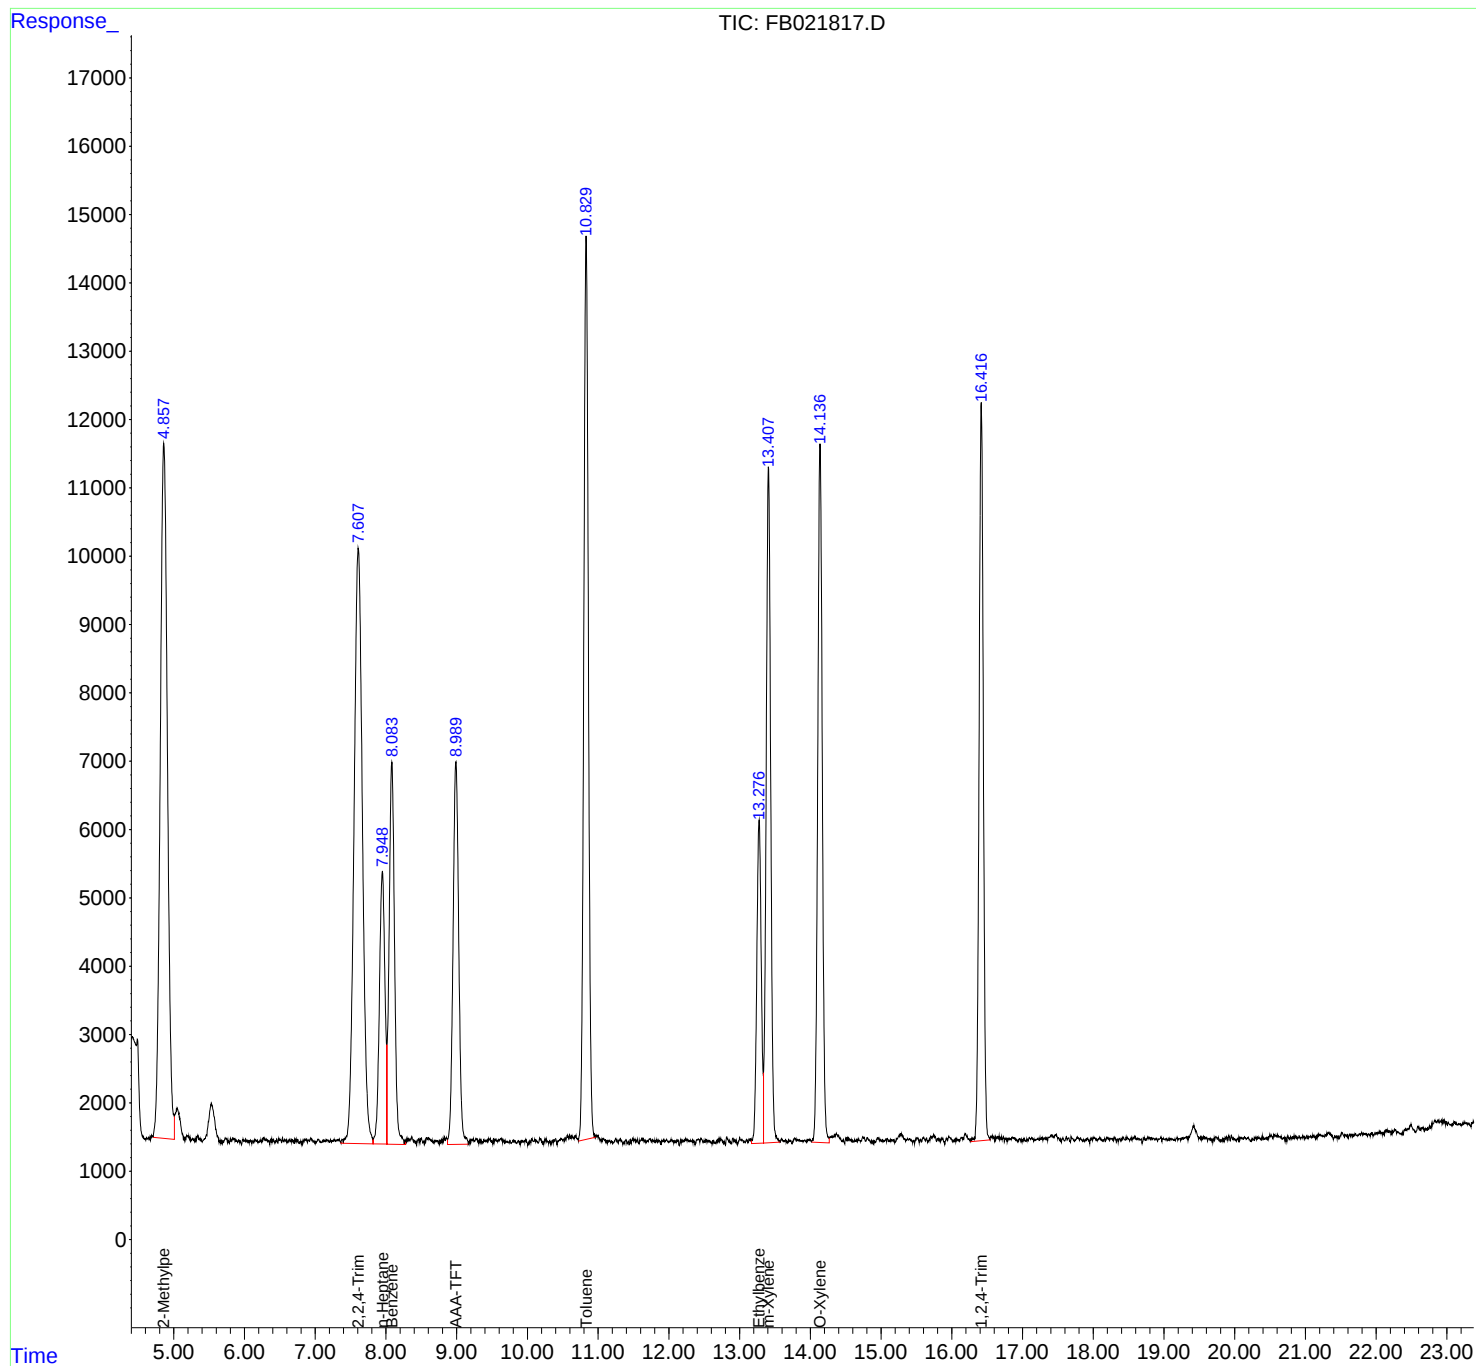

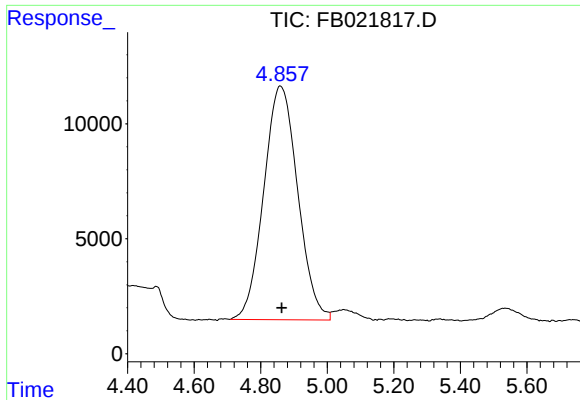


#1 2-Methylpentane

R.T.: 4.859 min
Delta R.T.: -0.004 min
Response: 721479
Conc: 26.16 ng/ml

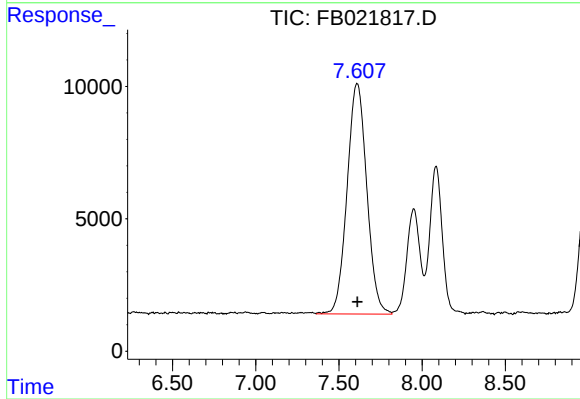


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.003 min
Response: 717502
Conc: 27.14 ng/ml

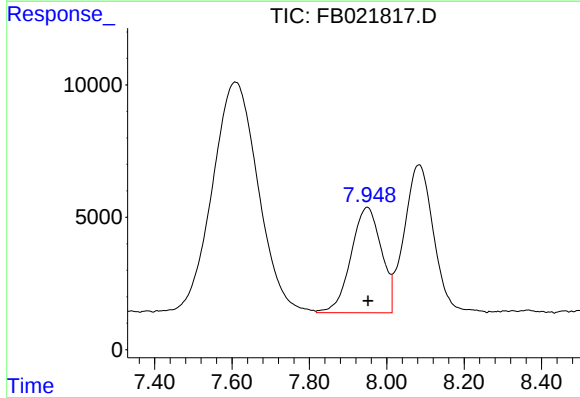


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 216603
Conc: 8.74 ng/ml

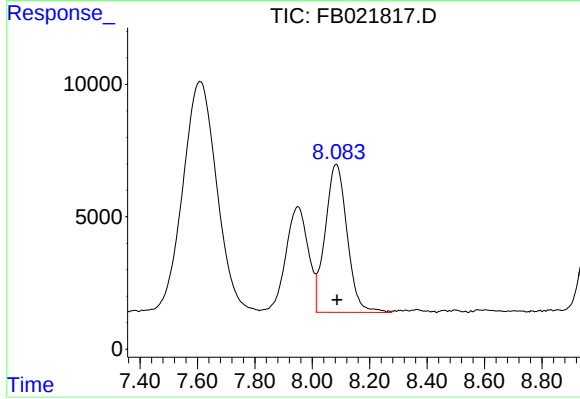


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 296325
Conc: 10.14 ng/ml

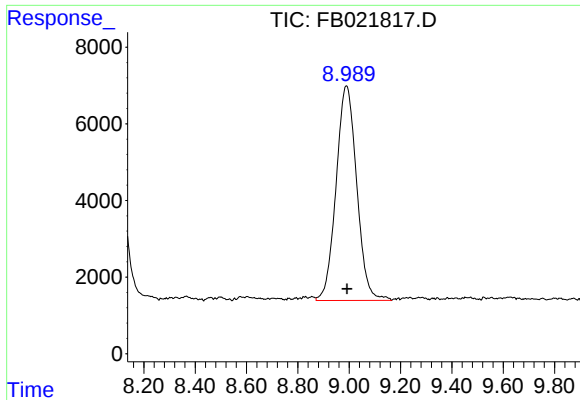


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.002 min
Response: 312348
Conc: 22.89 ng/ml

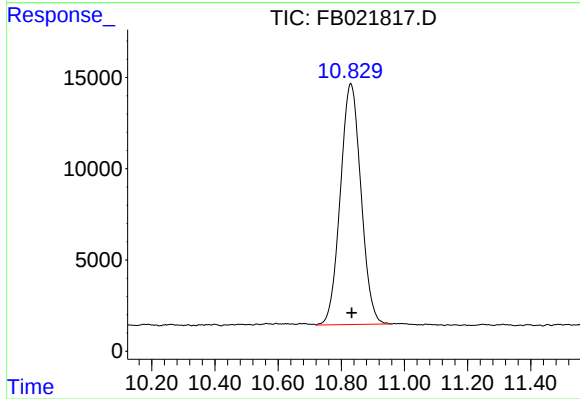


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 598587
Conc: 29.09 ng/ml

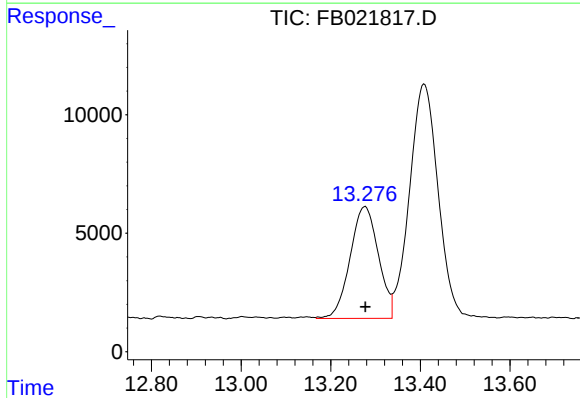


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.001 min
Response: 206323
Conc: 9.92 ng/ml

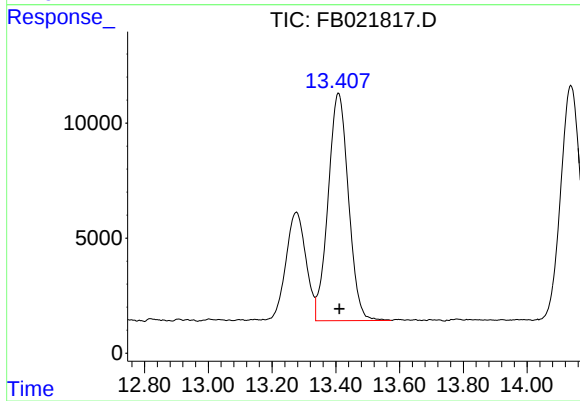

#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 437952
Conc: 19.71 ng/ml

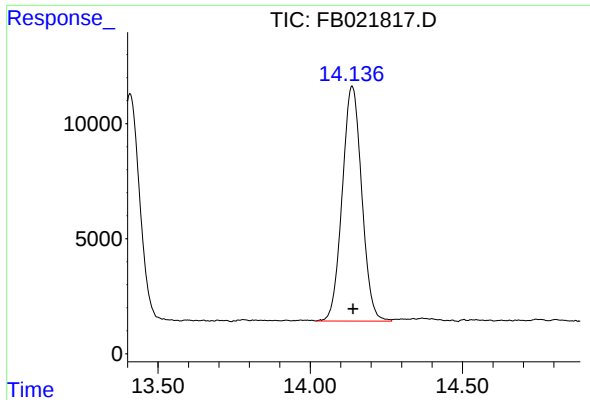


#9 O-Xylene

R.T.: 14.138 min

Delta R.T.: -0.002 min

Response: 454308

Conc: 19.75 ng/ml

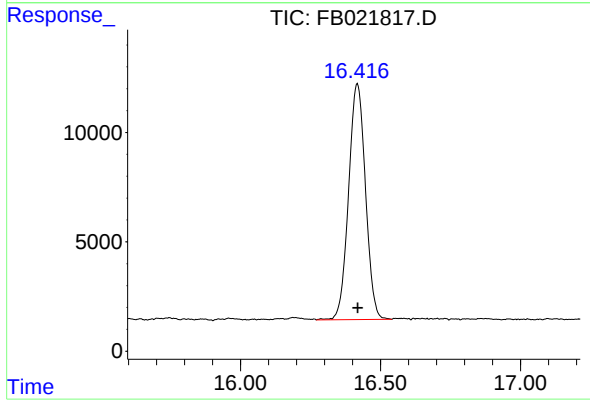

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min

Delta R.T.: -0.002 min

Response: 451403

Conc: 19.15 ng/ml