

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072619\
 Data File : FB021818.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jul 2019 15:51
 Operator : DD/AJ
 Sample : K3620-11MSD
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 26 23:28:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	293586	21.513 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	668206	24.231 ng/ml
2) t 2,2,4-Trimethylpentane	7.609	629940	23.830 ng/ml
3) t n-Heptane	7.949	190366	7.678 ng/ml
4) t Benzene	8.084	281200	9.625 ng/ml
6) t Toluene	10.831	584682	28.415 ng/ml
7) t Ethylbenzene	13.277	197426	9.490 ng/ml
8) t m-Xylene	13.409	409981	18.455 ng/ml
9) t O-Xylene	14.138	425693	18.506 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	434588	18.433 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072619\
Data File : FB021818.D
Signal(s) : FID2B.CH
Acq On : 26 Jul 2019 15:51
Operator : DD/AJ
Sample : K3620-11MSD
Misc : 5.03/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 26 23:28:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

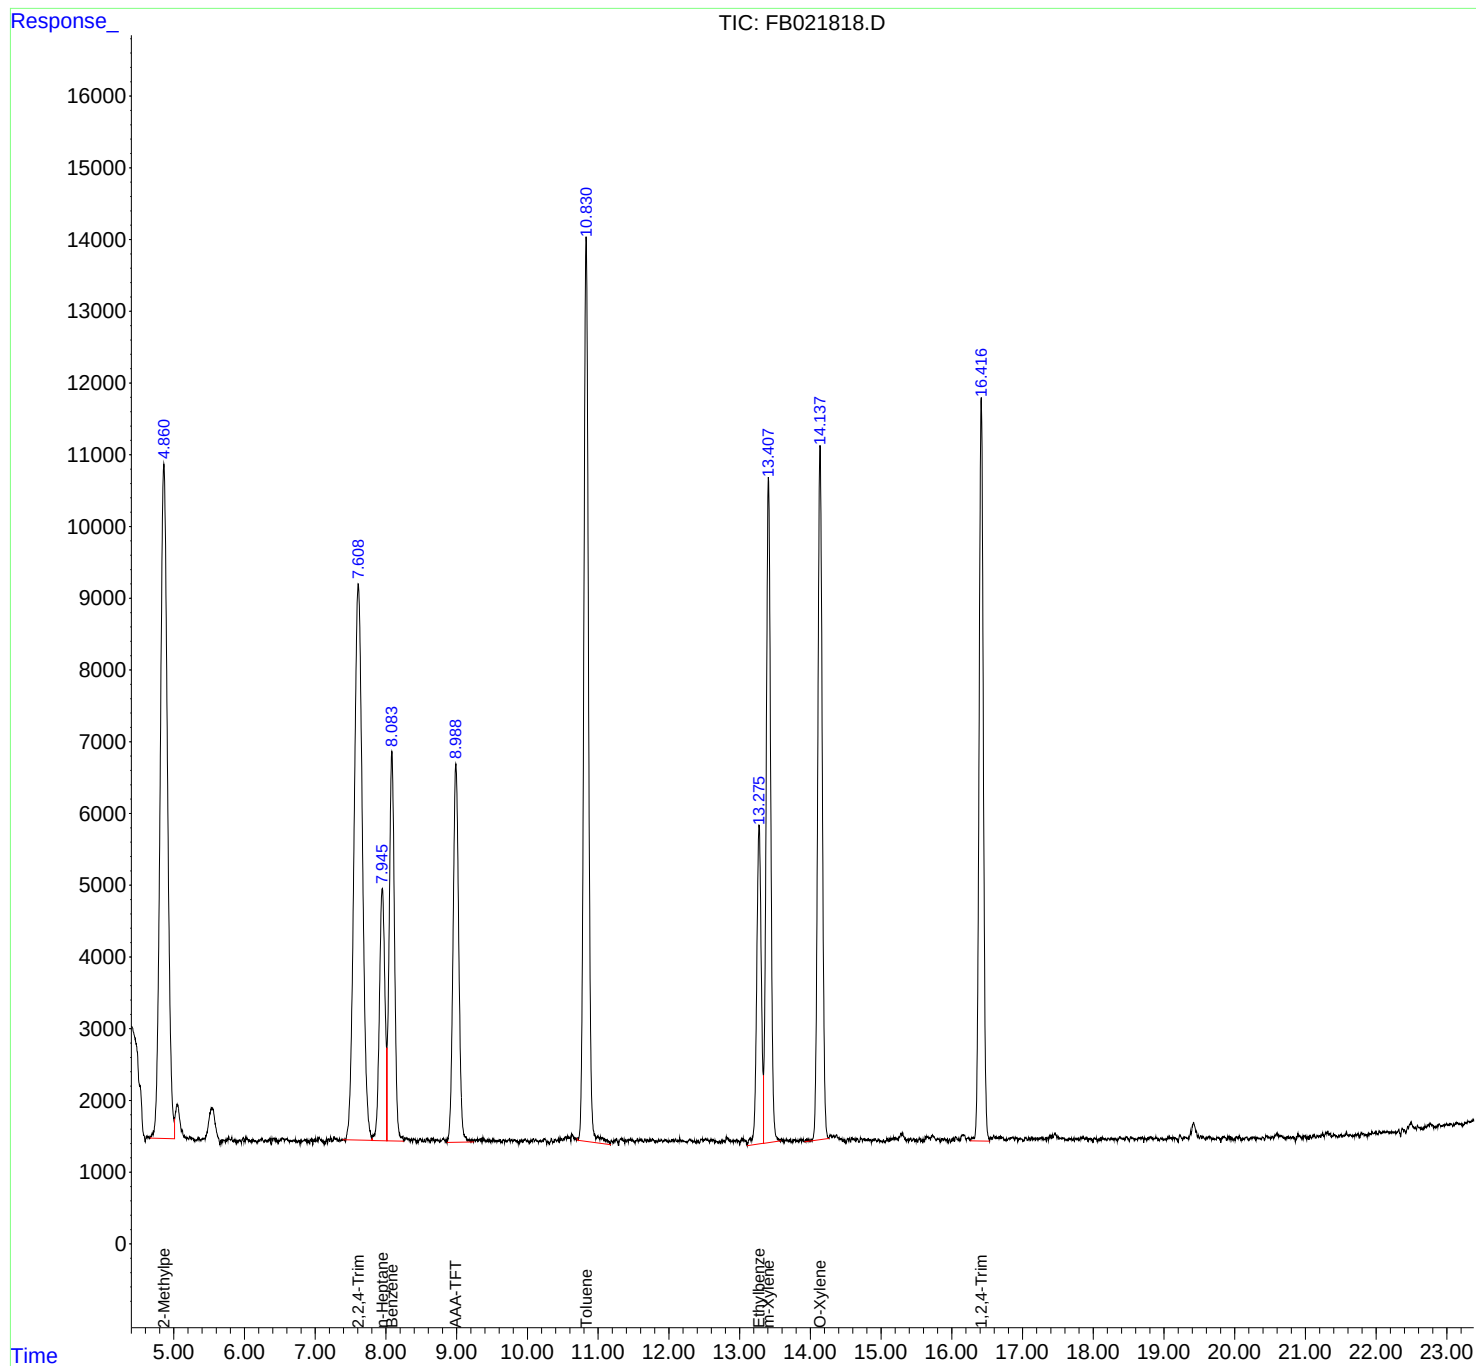

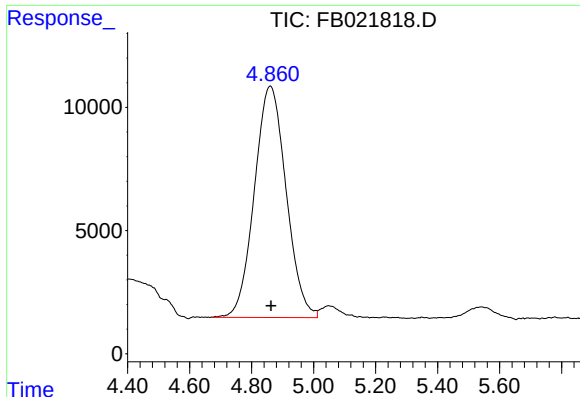


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 668206
Conc: 24.23 ng/ml

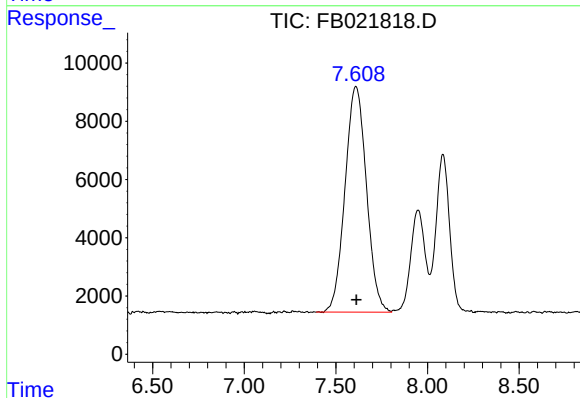


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.003 min
Response: 629940
Conc: 23.83 ng/ml

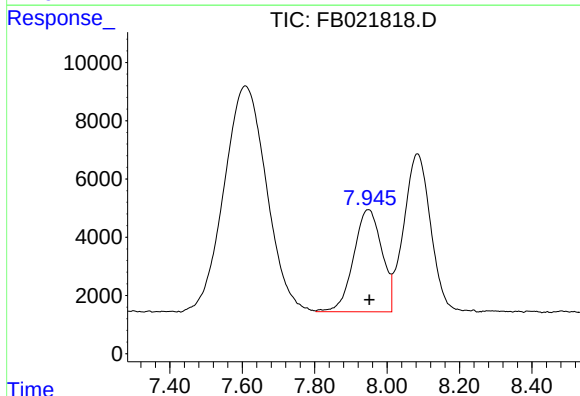


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 190366
Conc: 7.68 ng/ml

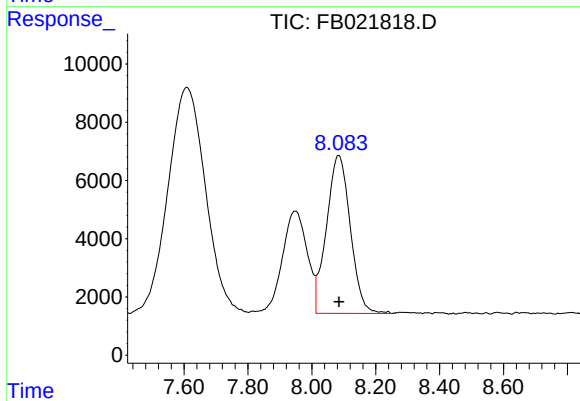


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.001 min
Response: 281200
Conc: 9.63 ng/ml

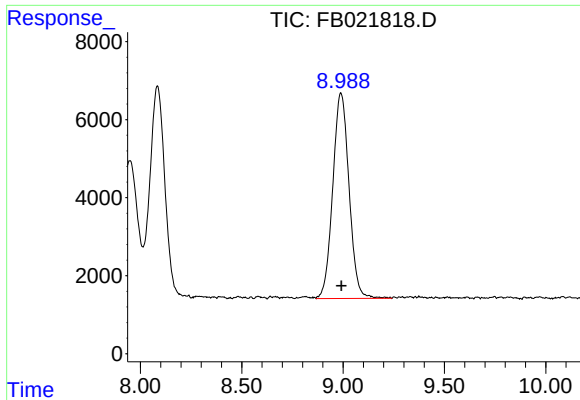


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.003 min
Response: 293586
Conc: 21.51 ng/ml

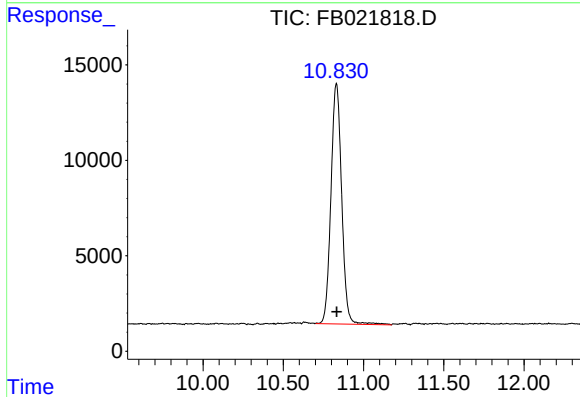


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 584682
Conc: 28.42 ng/ml

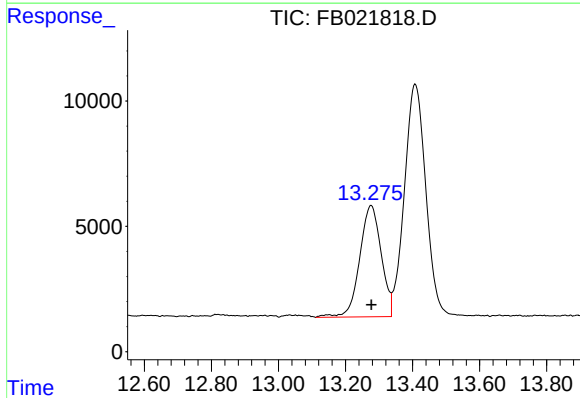


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: -0.001 min
Response: 197426
Conc: 9.49 ng/ml

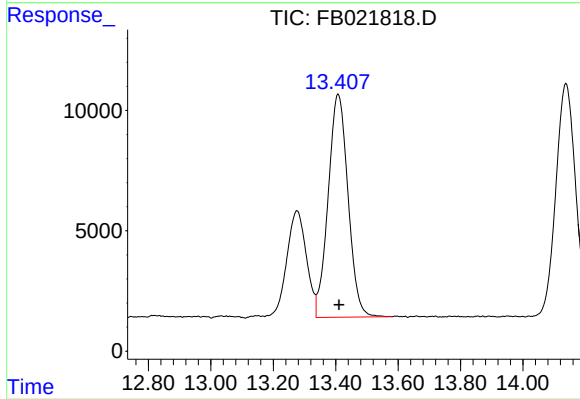


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 409981
Conc: 18.45 ng/ml

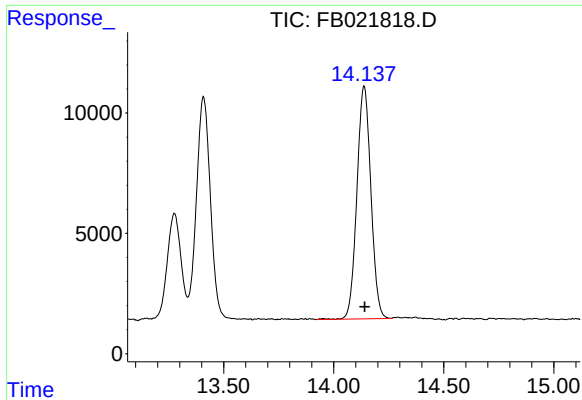

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.002 min
Response: 425693
Conc: 18.51 ng/ml

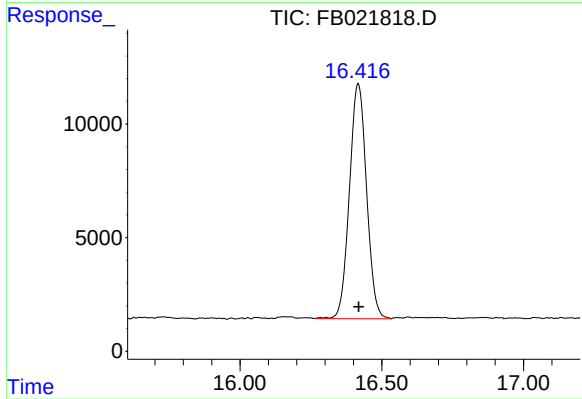

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.002 min
Response: 434588
Conc: 18.43 ng/ml