

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072619\
 Data File : FB021815.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jul 2019 14:20
 Operator : DD/AJ
 Sample : BSF0726S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 26 23:28:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.989	278078	20.377 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.859	765659	27.765 ng/ml
2) t	2,2,4-Trimethylpentane	7.608	808404	30.582 ng/ml
3) t	n-Heptane	7.948	242801	9.793 ng/ml
4) t	Benzene	8.083	288760	9.884 ng/ml
6) t	Toluene	10.830	608284	29.562 ng/ml
7) t	Ethylbenzene	13.275	212454	10.212 ng/ml
8) t	m-Xylene	13.408	449314	20.225 ng/ml
9) t	O-Xylene	14.138	468636	20.373 ng/ml
10) t	1,2,4-Trimethylbenzene	16.416	485147	20.577 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072619\
Data File : FB021815.D
Signal(s) : FID2B.CH
Acq On : 26 Jul 2019 14:20
Operator : DD/AJ
Sample : BSF0726S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 26 23:28:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

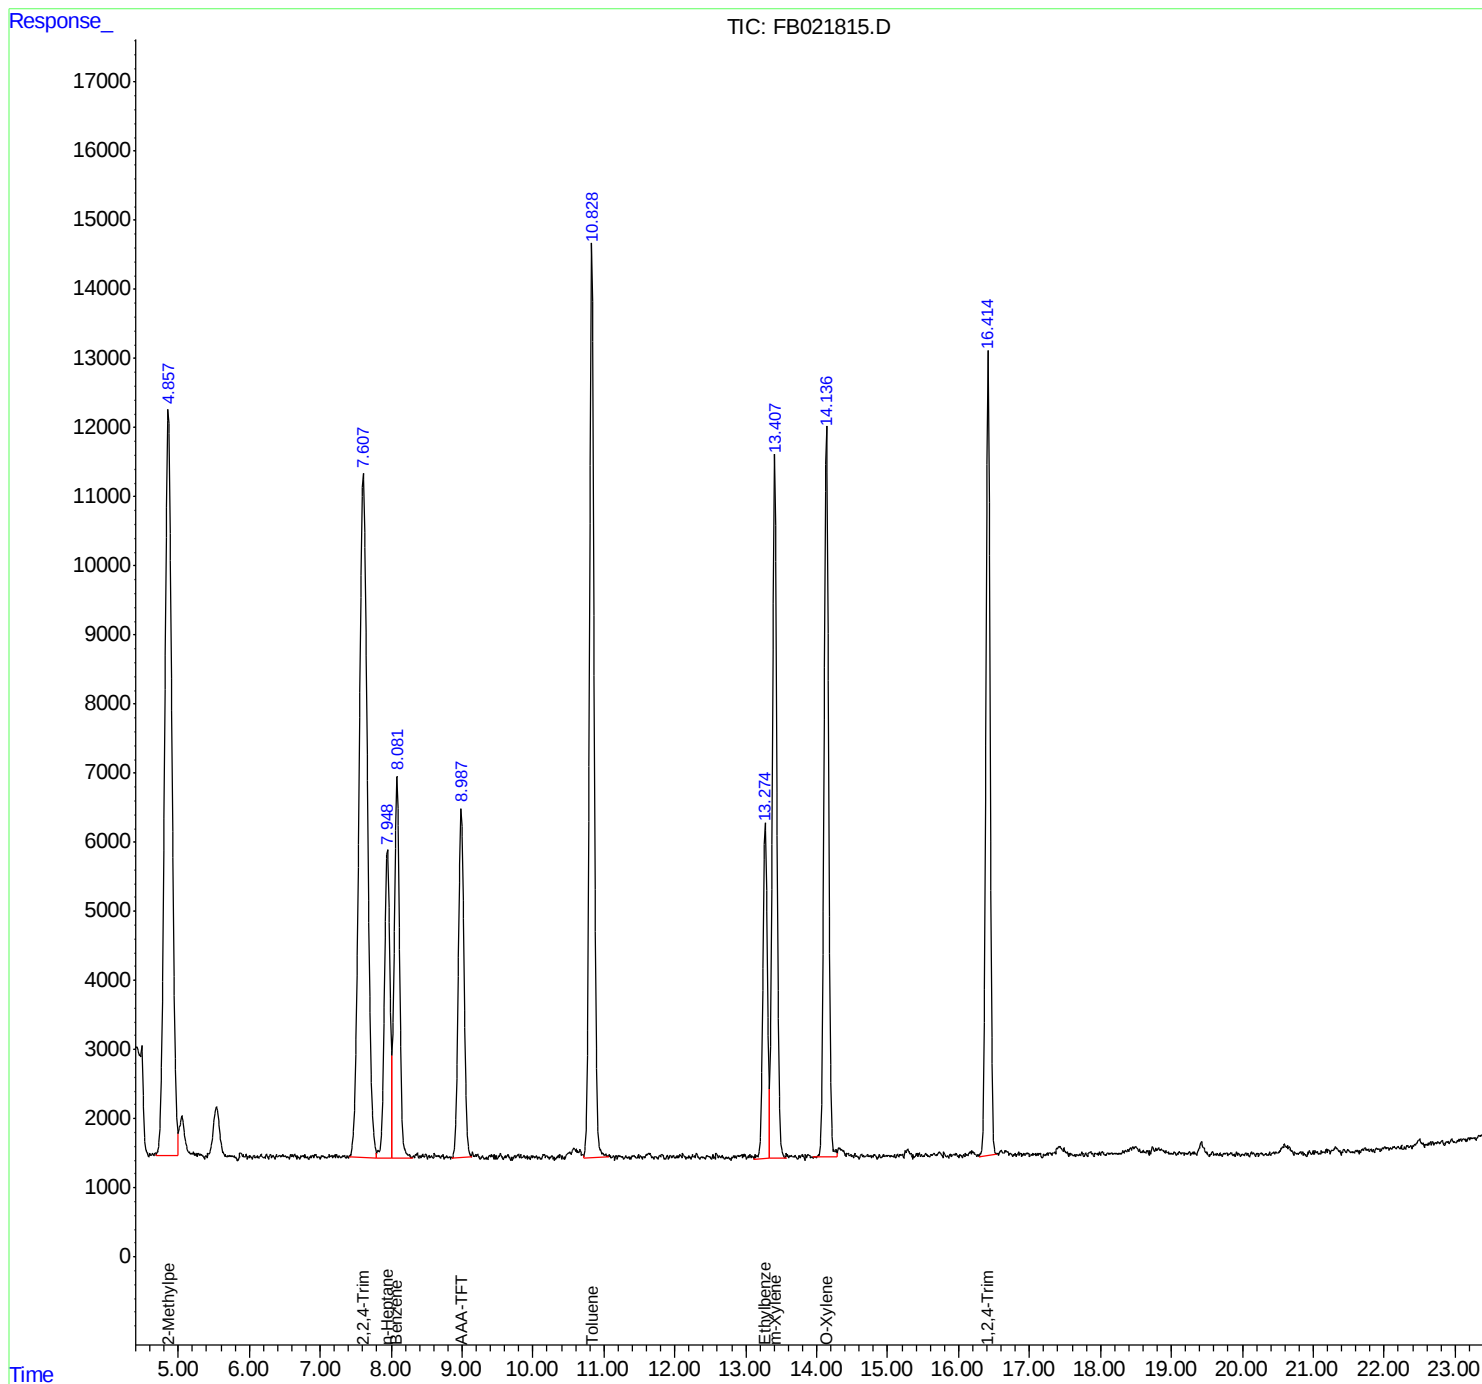

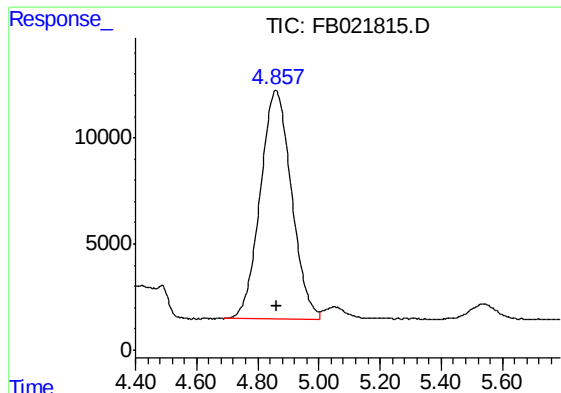


#1 2-Methylpentane

R.T.: 4.859 min
Delta R.T.: -0.004 min
Response: 765659
Conc: 27.77 ng/ml

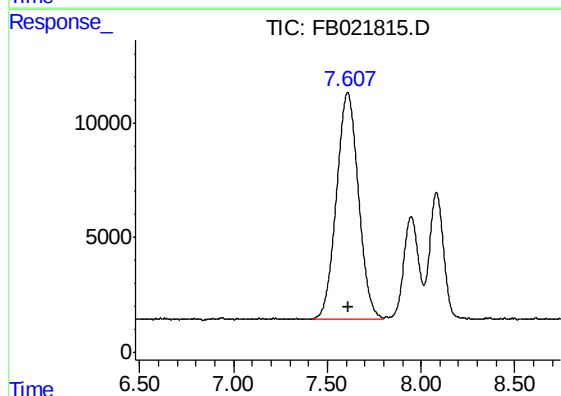


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: -0.004 min
Response: 808404
Conc: 30.58 ng/ml

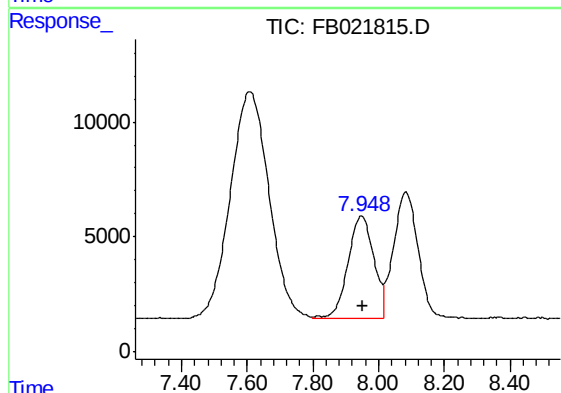


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: -0.003 min
Response: 242801
Conc: 9.79 ng/ml

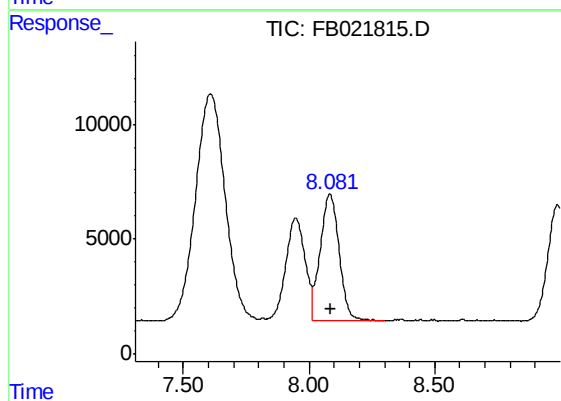


#4 Benzene

R.T.: 8.083 min
Delta R.T.: -0.003 min
Response: 288760
Conc: 9.88 ng/ml

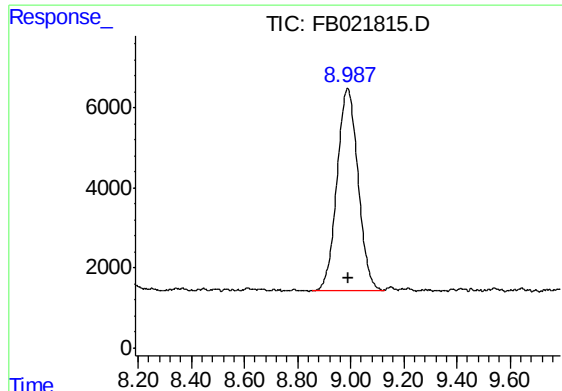


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.003 min
Response: 278078
Conc: 20.38 ng/ml

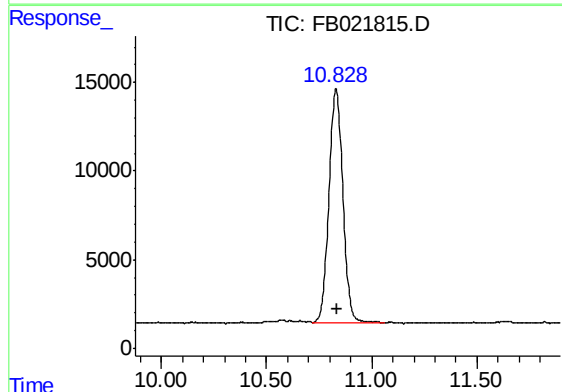


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.003 min
Response: 608284
Conc: 29.56 ng/ml

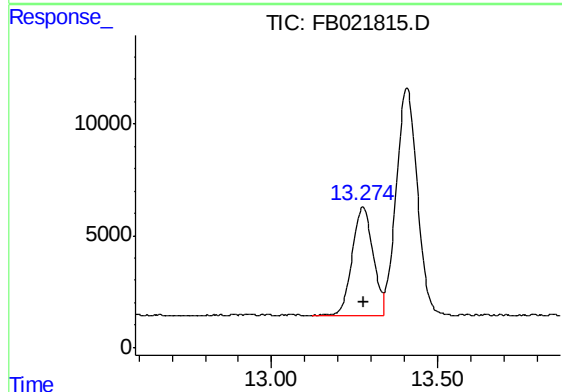


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: -0.002 min
Response: 212454
Conc: 10.21 ng/ml

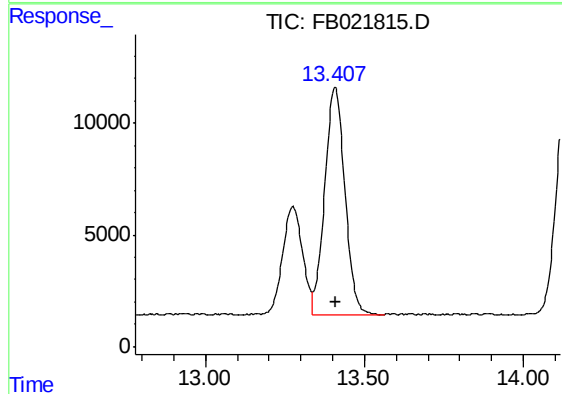


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: -0.003 min
Response: 449314
Conc: 20.23 ng/ml

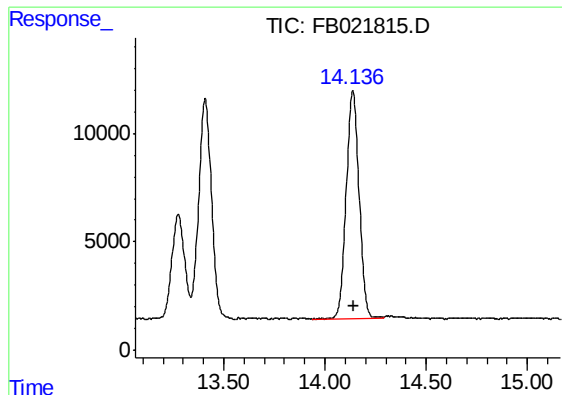

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.003 min
Response: 468636
Conc: 20.37 ng/ml

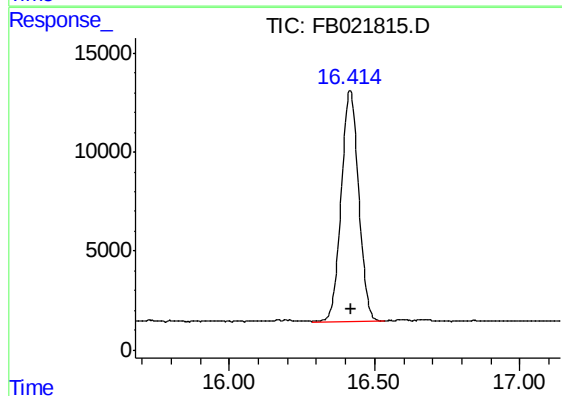

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: -0.003 min
Response: 485147
Conc: 20.58 ng/ml