

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB072619\  
Data File : FB021830.D  
Signal(s) : FID2B.CH  
Acq On : 26 Jul 2019 22:26  
Operator : DD/AJ  
Sample : K4021-06  
Misc : 5.01/5.00ml DI WATER  
ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Jul 26 23:30:48 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB071519.M  
Quant Title :  
QLast Update : Mon Jul 15 13:30:07 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.  | Response | Conc Units   |
|-----------------------------|-------|----------|--------------|
| -----                       |       |          |              |
| System Monitoring Compounds |       |          |              |
| 5) s AAA-TFT                | 8.990 | 269525   | 19.750 ng/ml |

Target Compounds

-----


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB072619\  
Data File : FB021830.D  
Signal(s) : FID2B.CH  
Acq On : 26 Jul 2019 22:26  
Operator : DD/AJ  
Sample : K4021-06  
Misc : 5.01/5.00ml DI WATER  
ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Jul 26 23:30:48 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB071519.M  
Quant Title :  
QLast Update : Mon Jul 15 13:30:07 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

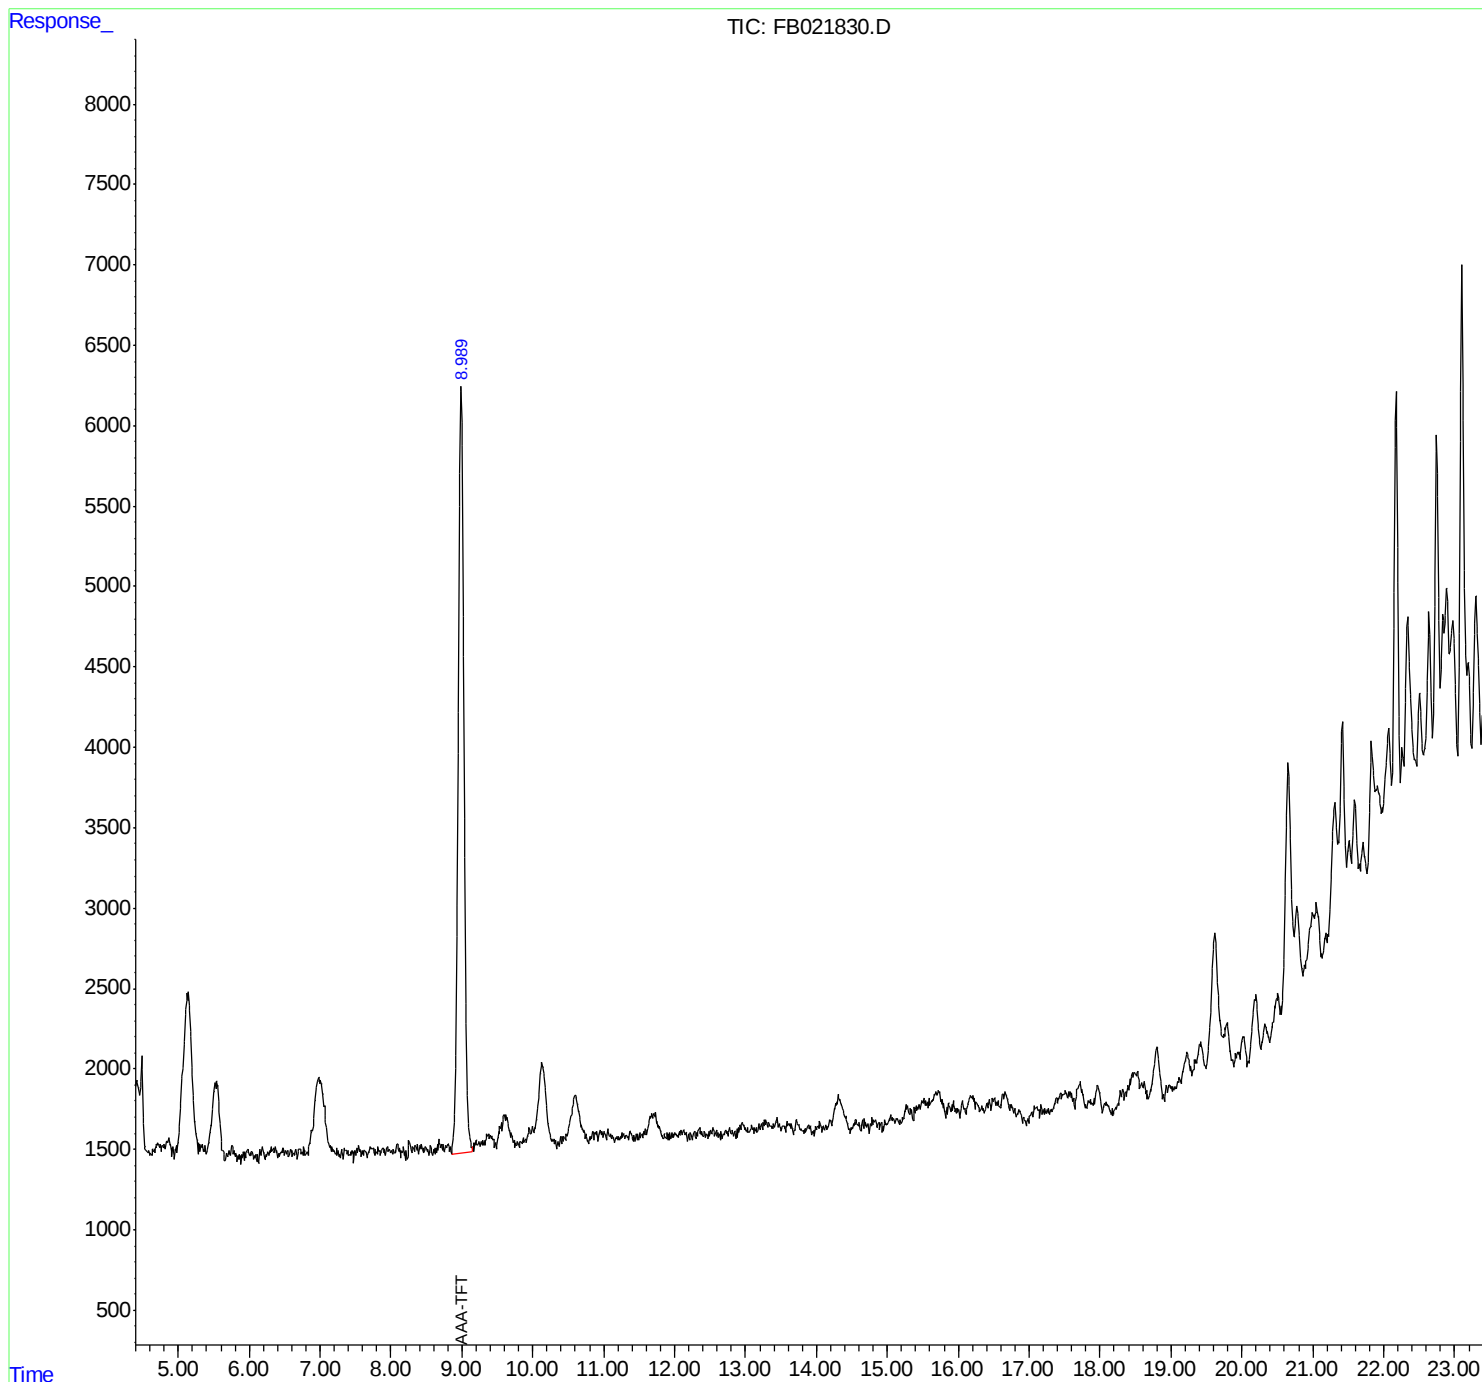

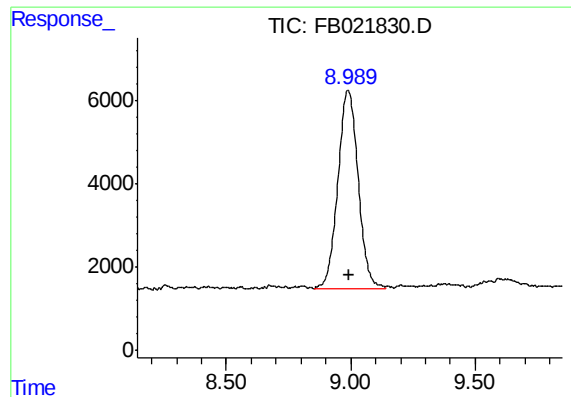

#5 AAA-TFT

R.T.: 8.990 min  
Delta R.T.: -0.002 min  
Response: 269525  
Conc: 19.75 ng/ml