

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072623\
 Data File : FB030219.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jul 2023 13:10
 Operator : YP/AJ
 Sample : BSF0726S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 27 01:13:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	233964	19.035 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	397113	24.039 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	469075	25.278 ng/ml
3) t n-Heptane	7.749	150913	7.844 ng/ml
4) t Benzene	7.886	195009	8.290 ng/ml
6) t Toluene	10.618	568543	24.809 ng/ml
7) t Ethylbenzene	13.054	183396	8.545 ng/ml
8) t m-Xylene	13.187	357084	16.980 ng/ml
9) t O-Xylene	13.913	348251	16.968 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	340114	17.376 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072623\
Data File : FB030219.D
Signal(s) : FID2B.CH
Acq On : 26 Jul 2023 13:10
Operator : YP/AJ
Sample : BSF0726S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 27 01:13:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

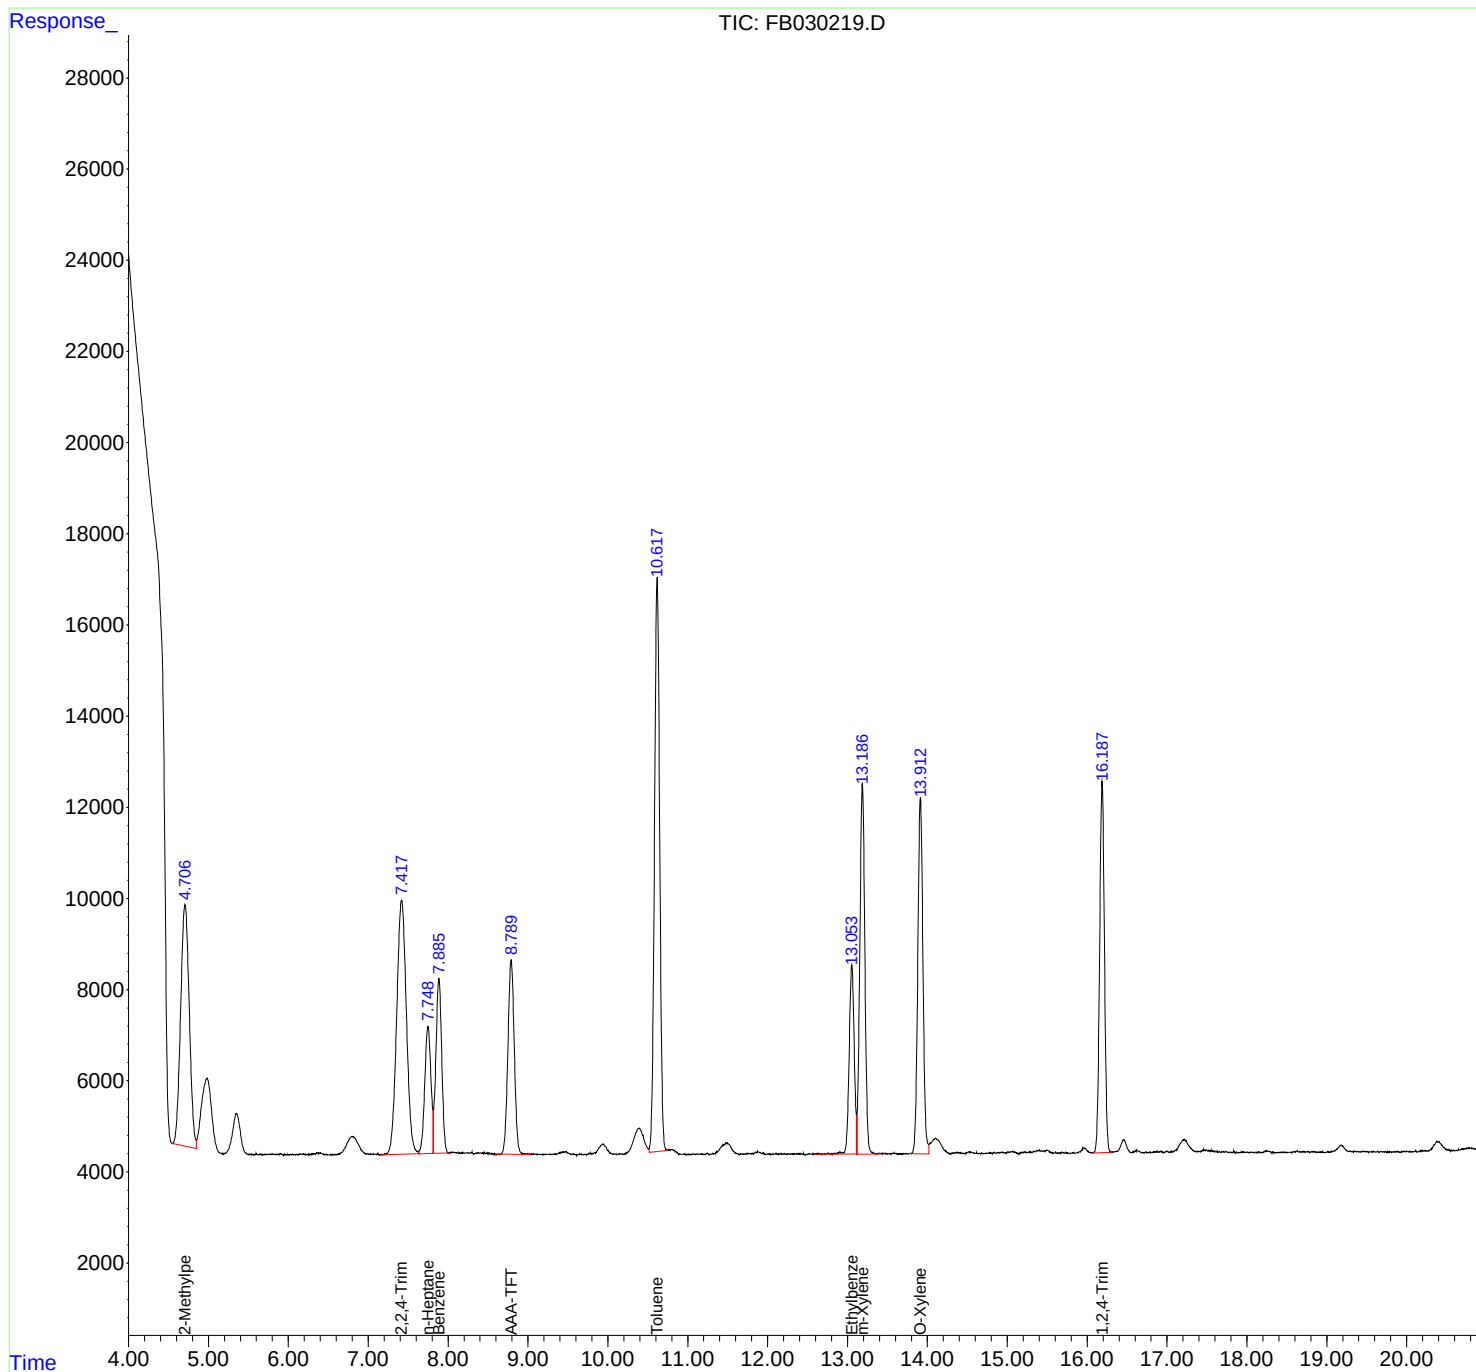


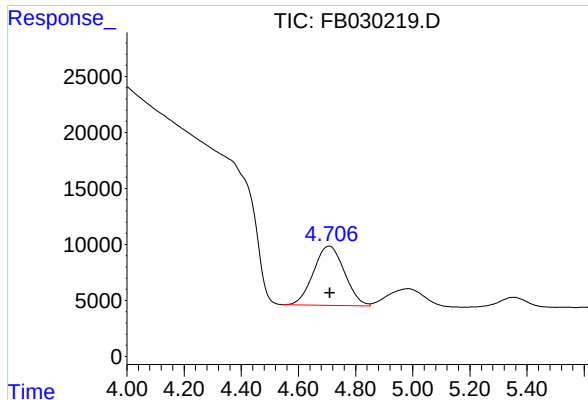

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.002 min
Response: 397113
Conc: 24.04 ng/ml

Instrument :
FID_B
ClientSampleId :

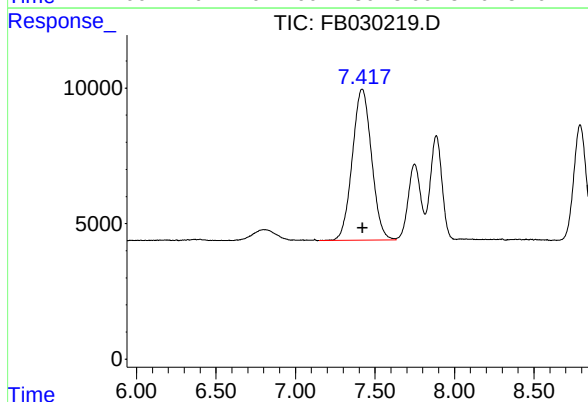


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.003 min
Response: 469075
Conc: 25.28 ng/ml

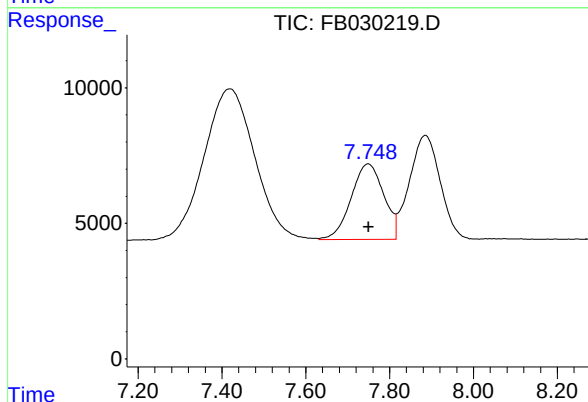


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 150913
Conc: 7.84 ng/ml

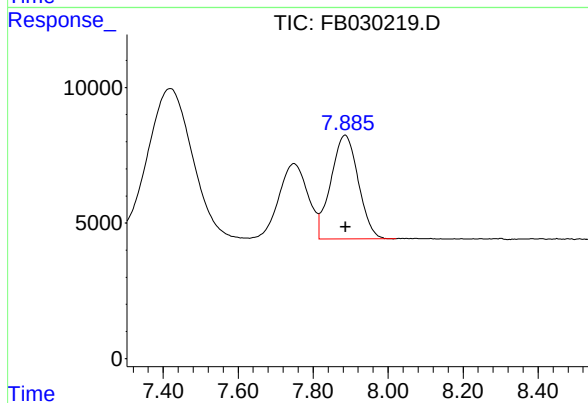

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.001 min
Response: 195009
Conc: 8.29 ng/ml

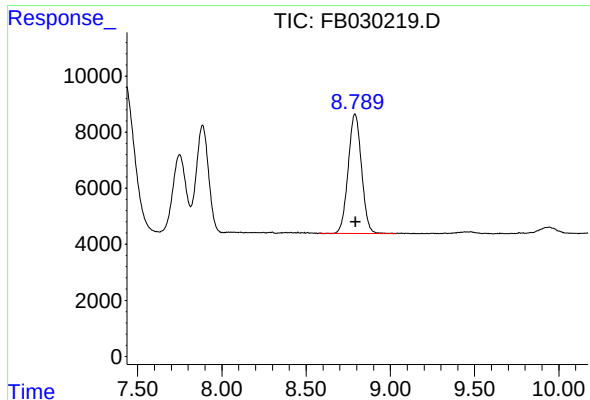

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.003 min
Response: 233964
Conc: 19.04 ng/ml

Instrument :
FID_B
ClientSampleId :

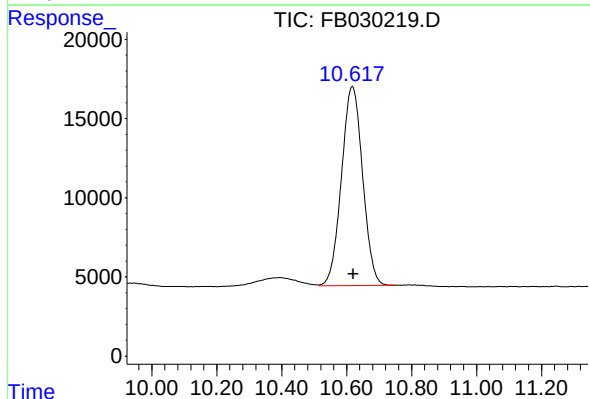


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.002 min
Response: 568543
Conc: 24.81 ng/ml

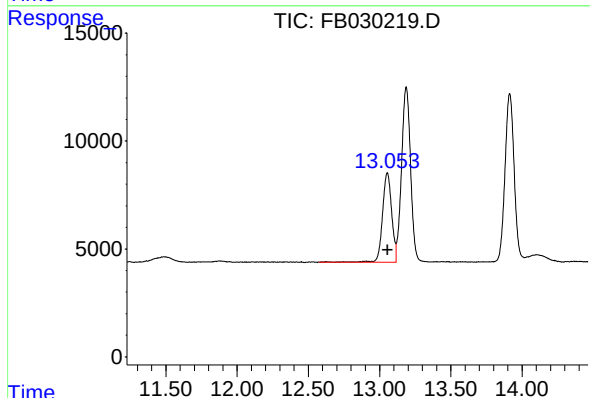


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.002 min
Response: 183396
Conc: 8.54 ng/ml

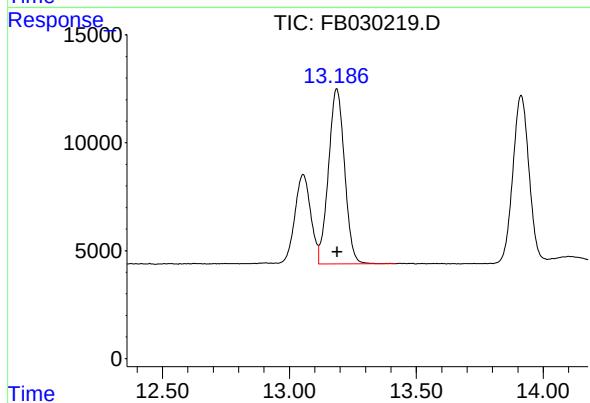

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.002 min
Response: 357084
Conc: 16.98 ng/ml

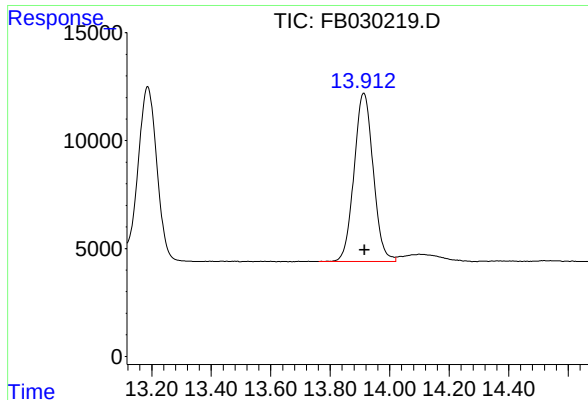

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.002 min
Response: 348251
Conc: 16.97 ng/ml

Instrument :
FID_B
ClientSampleId :

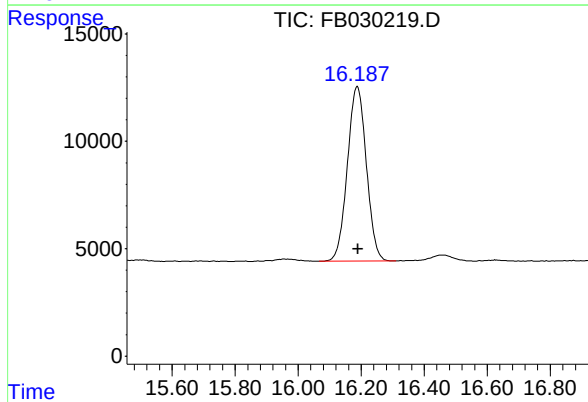

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.002 min
Response: 340114
Conc: 17.38 ng/ml