

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072623\
 Data File : FB030215.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jul 2023 10:28
 Operator : YP/AJ
 Sample : BSF0726S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0726S1

Integration File: Calibration.e
 Quant Time: Jul 27 01:12:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	232823	18.942 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	479054	28.999 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	521953	28.128 ng/ml
3) t n-Heptane	7.748	176347	9.167 ng/ml
4) t Benzene	7.885	222073	9.440 ng/ml
6) t Toluene	10.616	647103	28.237 ng/ml
7) t Ethylbenzene	13.052	207116	9.650 ng/ml
8) t m-Xylene	13.185	409168	19.456 ng/ml
9) t O-Xylene	13.912	399567	19.469 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	394510	20.155 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072623\
Data File : FB030215.D
Signal(s) : FID2B.CH
Acq On : 26 Jul 2023 10:28
Operator : YP/AJ
Sample : BSF0726S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0726S1

Integration File: Calibration.e
Quant Time: Jul 27 01:12:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

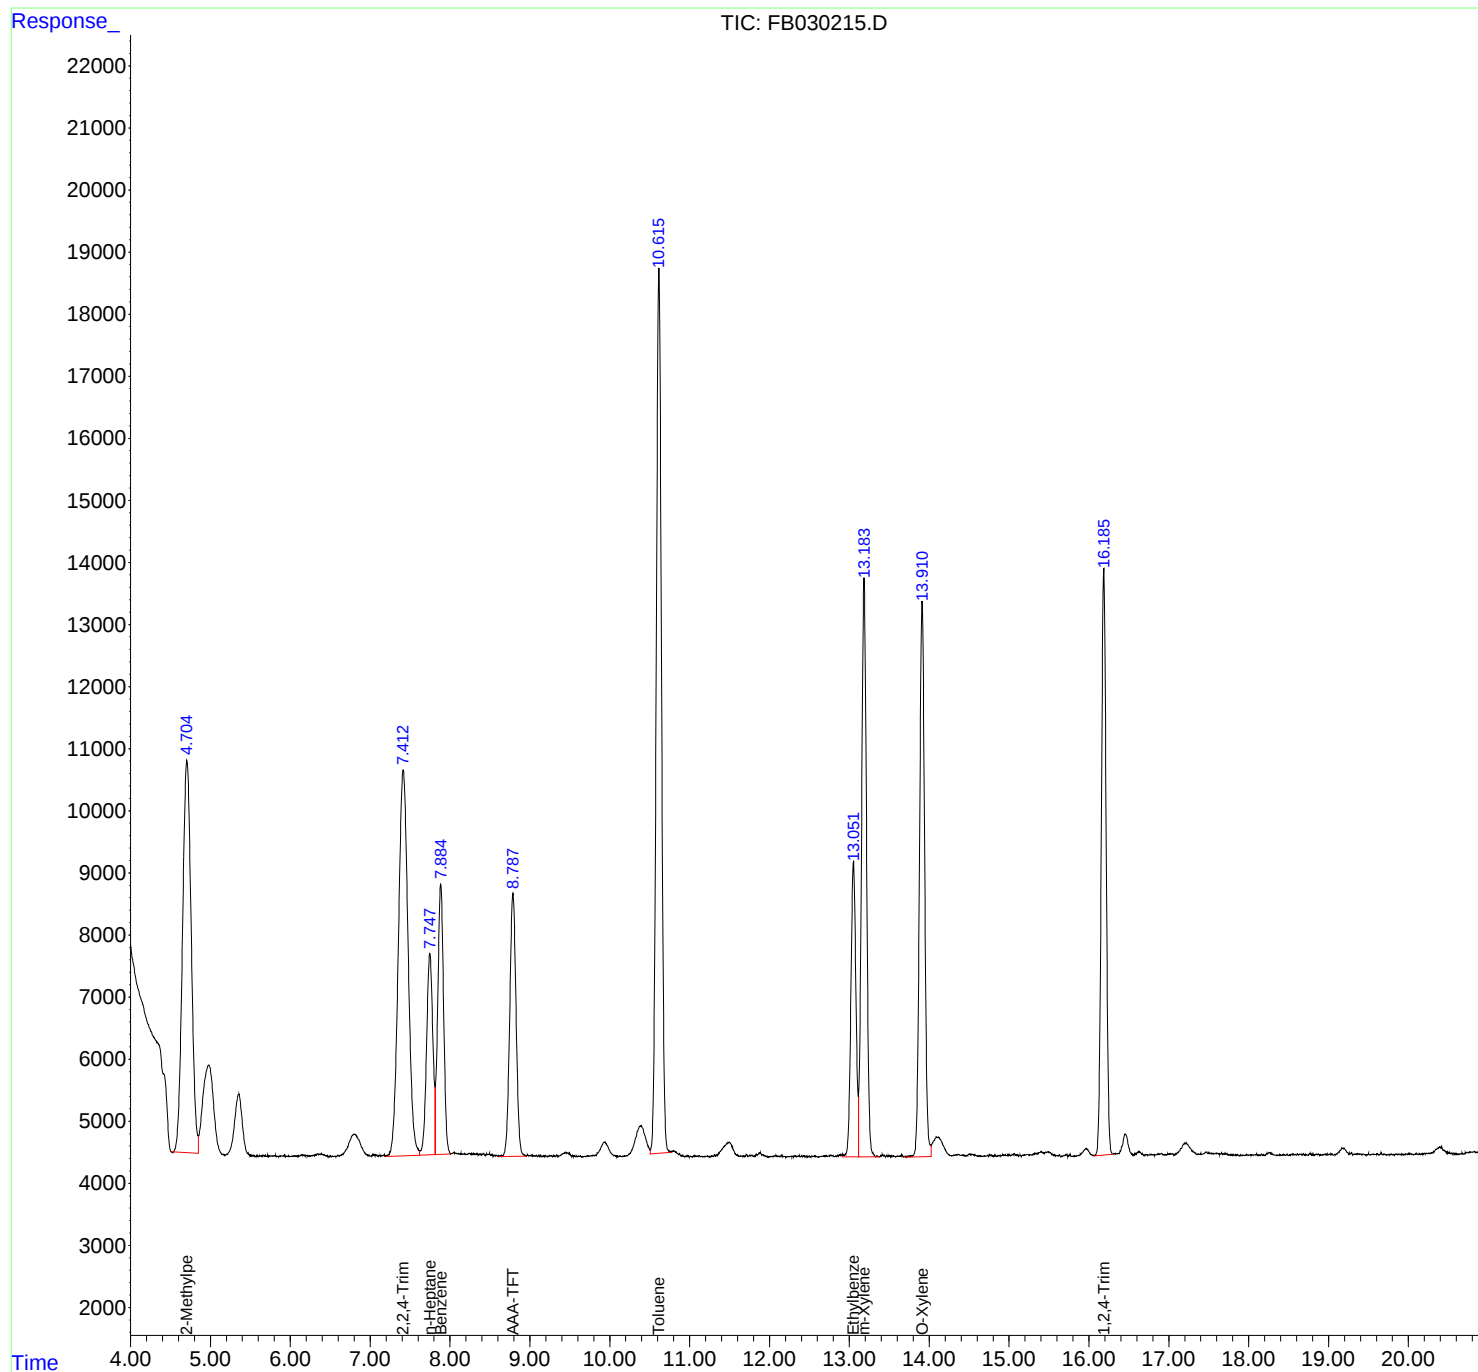


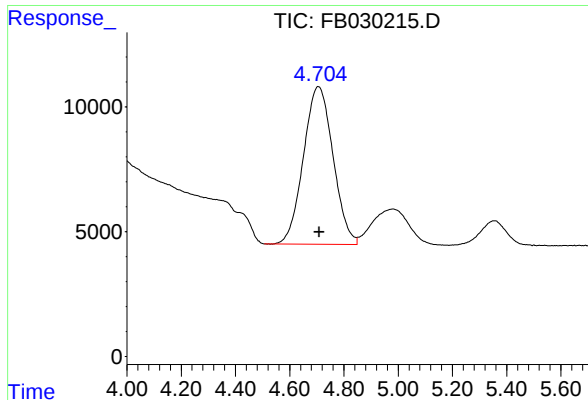

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.004 min
Response: 479054
Conc: 29.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0726S1

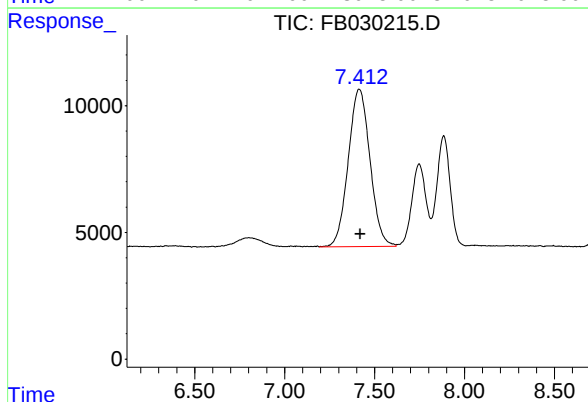


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.008 min
Response: 521953
Conc: 28.13 ng/ml

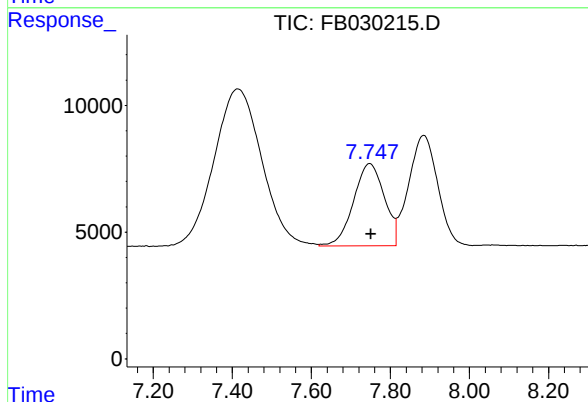


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.002 min
Response: 176347
Conc: 9.17 ng/ml

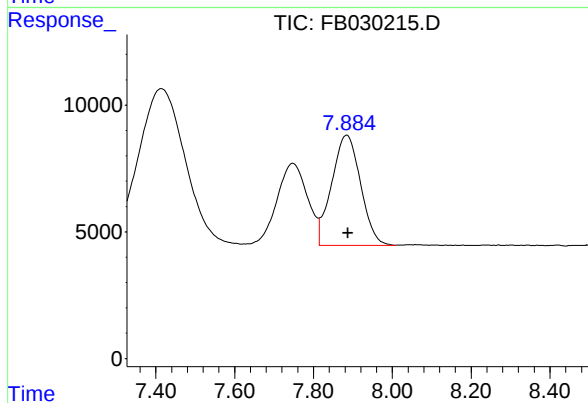

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.002 min
Response: 222073
Conc: 9.44 ng/ml

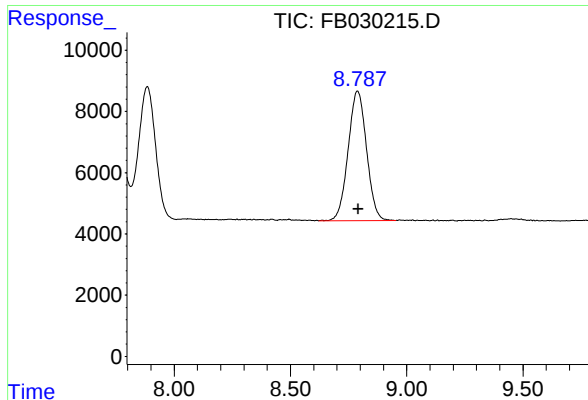

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.004 min
Response: 232823
Conc: 18.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0726S1

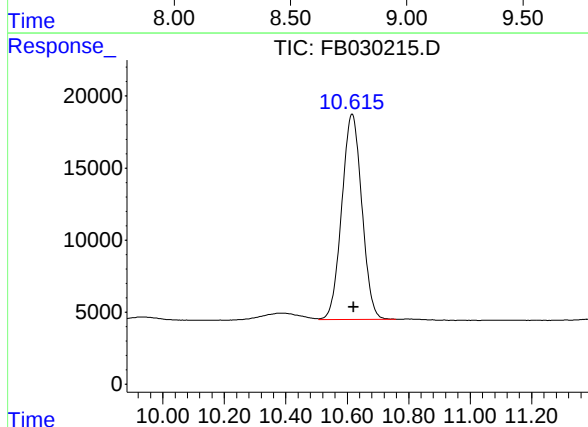


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.004 min
Response: 647103
Conc: 28.24 ng/ml

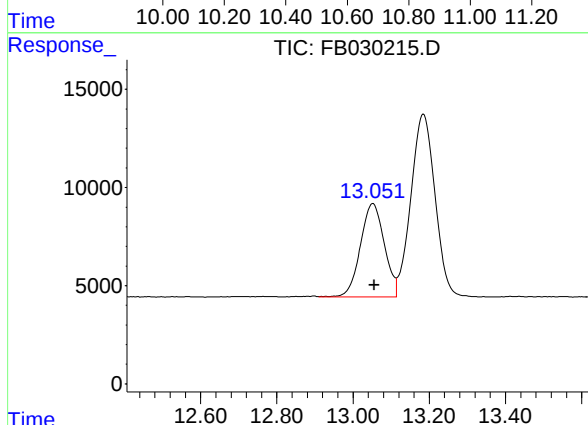


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.004 min
Response: 207116
Conc: 9.65 ng/ml

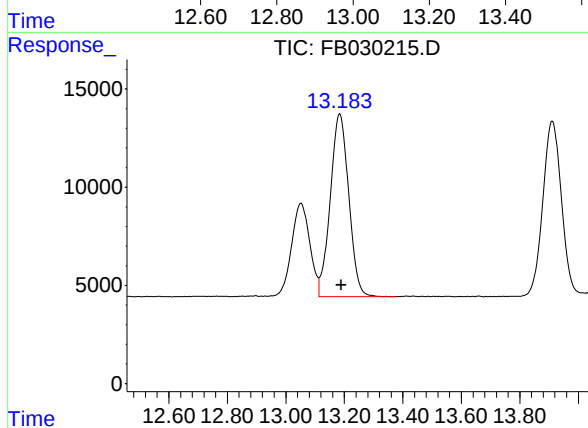

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.004 min
Response: 409168
Conc: 19.46 ng/ml

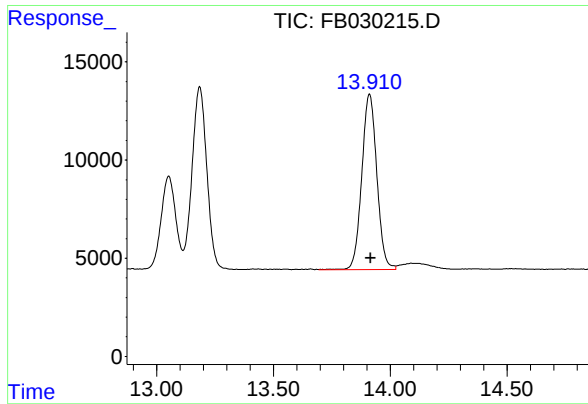

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.004 min
Response: 399567
Conc: 19.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0726S1

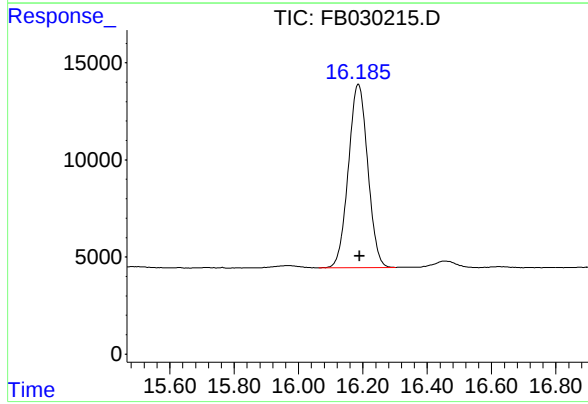

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.004 min
Response: 394510
Conc: 20.16 ng/ml