

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB072623\  
 Data File : FB030219.D  
 Signal(s) : FID2B.CH  
 Acq On : 26 Jul 2023 13:10  
 Operator : YP/AJ  
 Sample : BSF0726S2  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :  
 BSF0726S2

Integration File: Calibration.e  
 Quant Time: Jul 27 01:13:15 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB072423.M  
 Quant Title :  
 QLast Update : Tue Jul 25 06:41:02 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.790  | 233964   | 19.035 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.708  | 397113   | 24.039 ng/ml |
| 2) t 2,2,4-Trimethylpentane  | 7.419  | 469075   | 25.278 ng/ml |
| 3) t n-Heptane               | 7.749  | 150913   | 7.844 ng/ml  |
| 4) t Benzene                 | 7.886  | 195009   | 8.290 ng/ml  |
| 6) t Toluene                 | 10.618 | 568543   | 24.809 ng/ml |
| 7) t Ethylbenzene            | 13.054 | 183396   | 8.545 ng/ml  |
| 8) t m-Xylene                | 13.187 | 357084   | 16.980 ng/ml |
| 9) t O-Xylene                | 13.913 | 348251   | 16.968 ng/ml |
| 10) t 1,2,4-Trimethylbenzene | 16.188 | 340114   | 17.376 ng/ml |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB072623\  
Data File : FB030219.D  
Signal(s) : FID2B.CH  
Acq On : 26 Jul 2023 13:10  
Operator : YP/AJ  
Sample : BSF0726S2  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
BSF0726S2

Integration File: Calibration.e  
Quant Time: Jul 27 01:13:15 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB072423.M  
Quant Title :  
QLast Update : Tue Jul 25 06:41:02 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

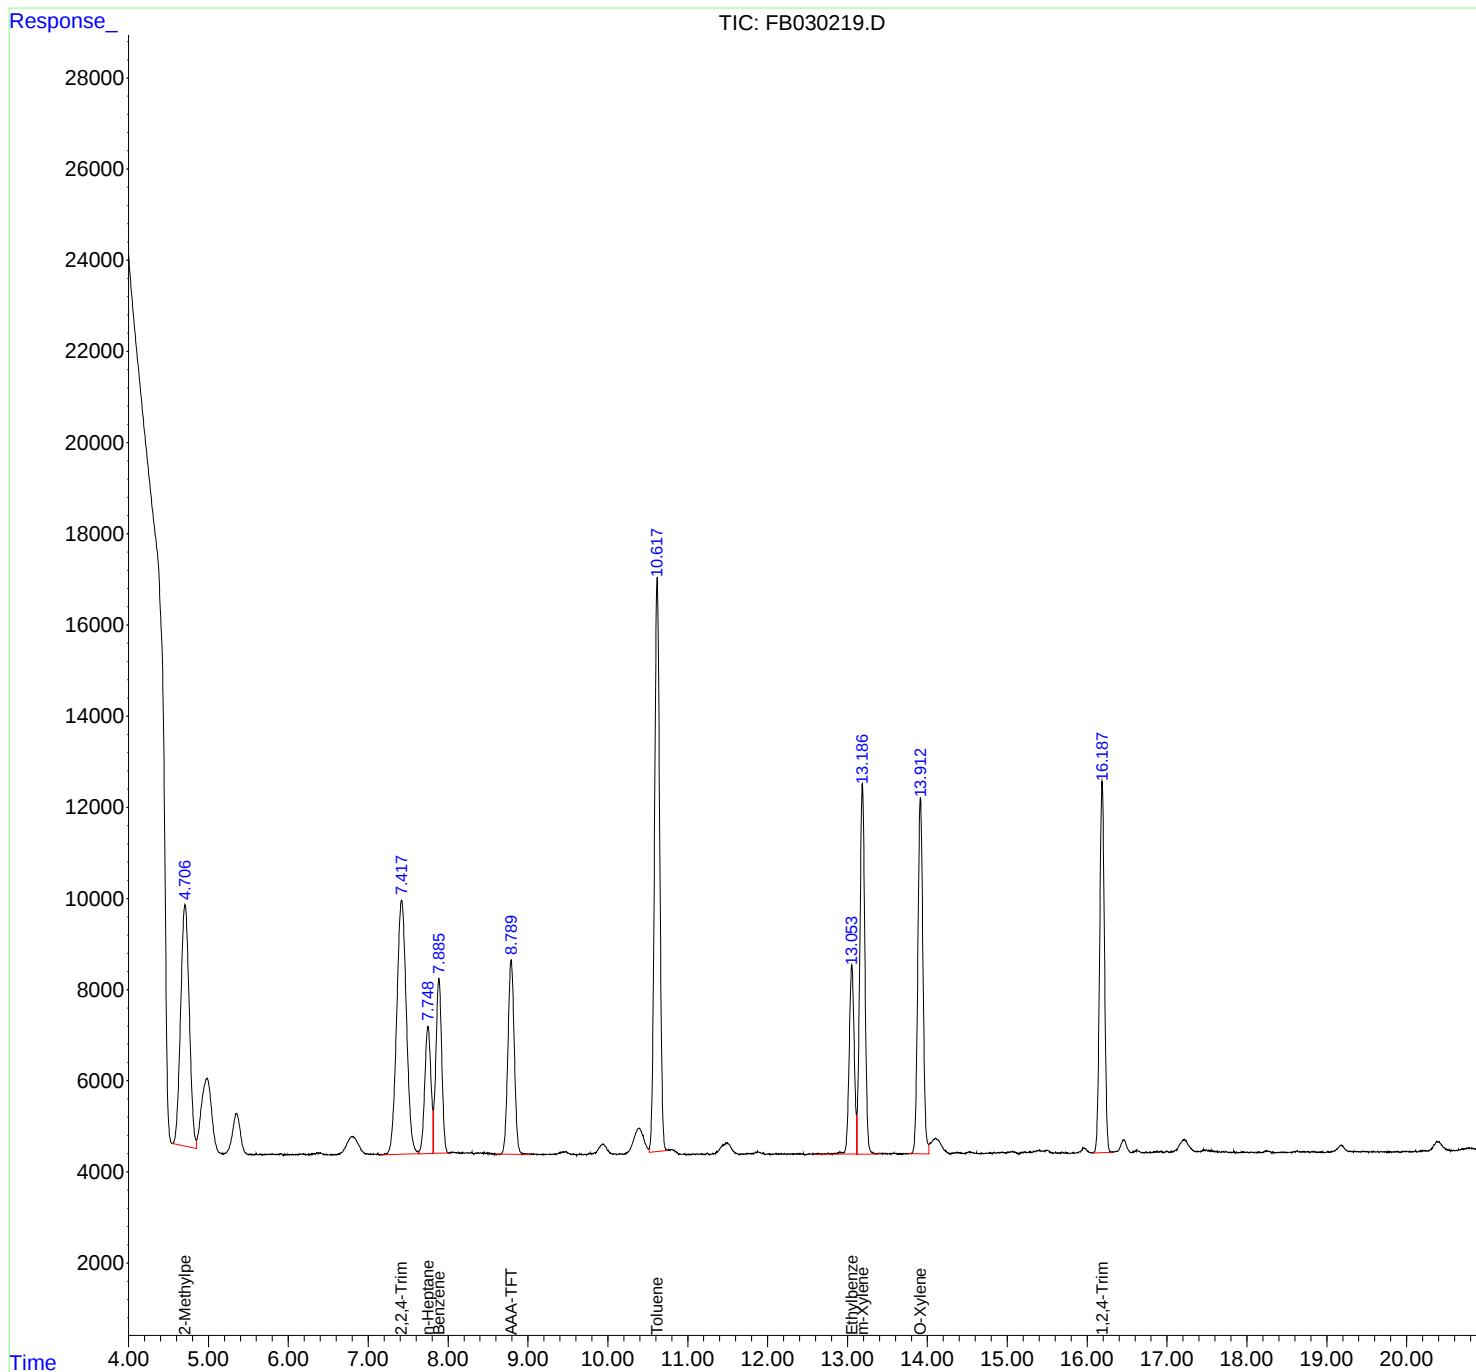


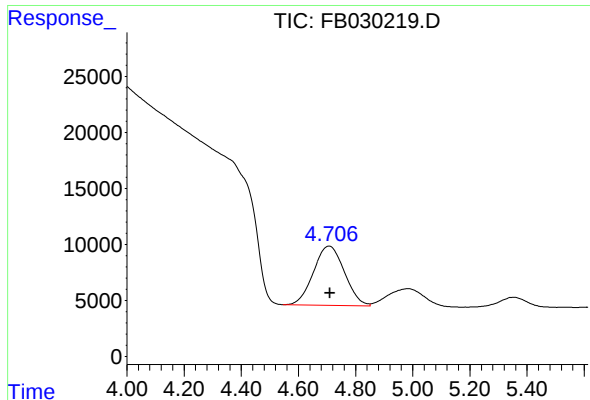

#1 2-Methylpentane


R.T.: 4.708 min  
Delta R.T.: -0.002 min  
Response: 397113  
Conc: 24.04 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF0726S2

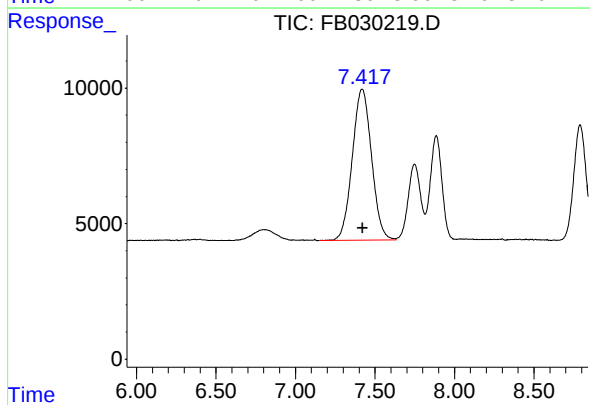


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min  
Delta R.T.: -0.003 min  
Response: 469075  
Conc: 25.28 ng/ml

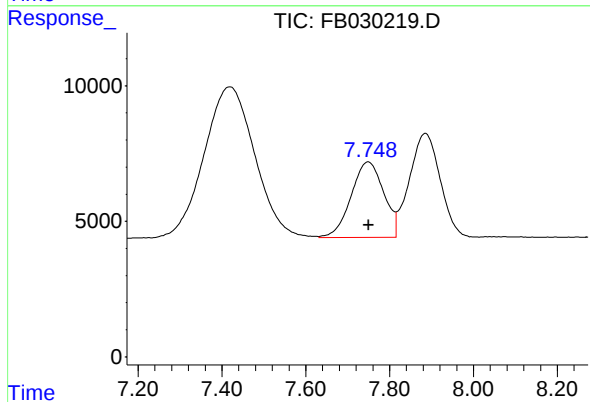


#3 n-Heptane

R.T.: 7.749 min  
Delta R.T.: 0.000 min  
Response: 150913  
Conc: 7.84 ng/ml

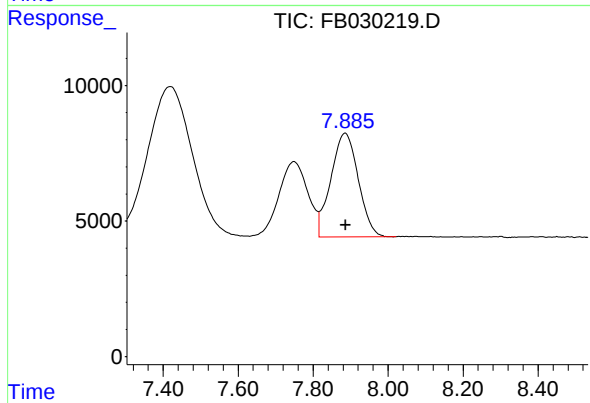

#4 Benzene


R.T.: 7.886 min  
Delta R.T.: -0.001 min  
Response: 195009  
Conc: 8.29 ng/ml

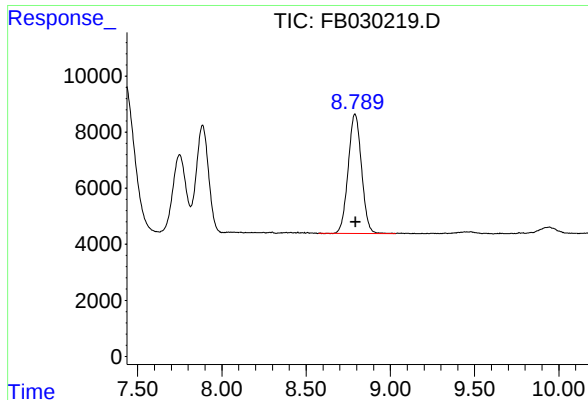

#5 AAA-TFT


R.T.: 8.790 min  
Delta R.T.: -0.003 min  
Response: 233964  
Conc: 19.04 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF0726S2

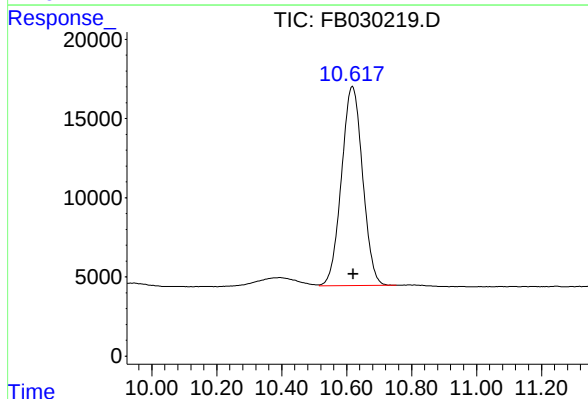


#6 Toluene

R.T.: 10.618 min  
Delta R.T.: -0.002 min  
Response: 568543  
Conc: 24.81 ng/ml

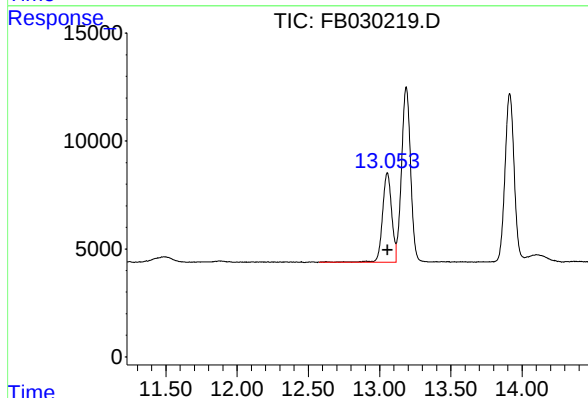


#7 Ethylbenzene

R.T.: 13.054 min  
Delta R.T.: -0.002 min  
Response: 183396  
Conc: 8.54 ng/ml

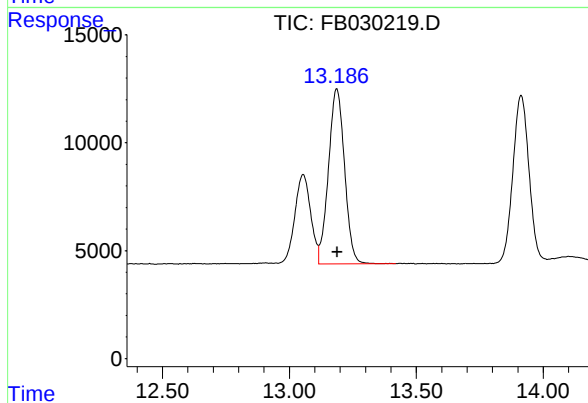

#8 m-Xylene


R.T.: 13.187 min  
Delta R.T.: -0.002 min  
Response: 357084  
Conc: 16.98 ng/ml

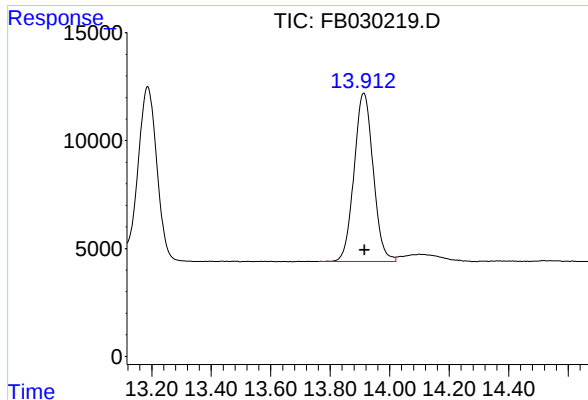

#9 O-Xylene

R.T.: 13.913 min  
Delta R.T.: -0.002 min  
Response: 348251  
Conc: 16.97 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF0726S2

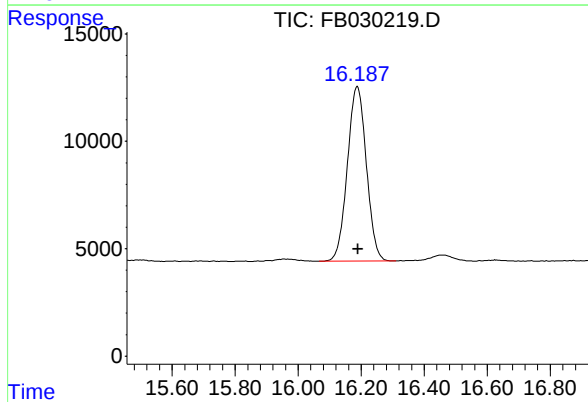

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min  
Delta R.T.: -0.002 min  
Response: 340114  
Conc: 17.38 ng/ml