

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072721\
 Data File : FB026096.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jul 2021 9:16
 Operator : AJ/MA
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 27 11:13:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
 Quant Title :
 QLast Update : Tue Jul 27 11:12:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.839	143916	5.453 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.846	283761	8.617 ng/ml
2) t 2,2,4-Trimethylpentane	7.494	292412	9.055 ng/ml
3) t n-Heptane	7.816	132186	2.899 ng/ml
4) t Benzene	7.954	141090	2.952 ng/ml
6) t Toluene	10.647	390275	8.744 ng/ml
7) t Ethylbenzene	13.066	108364	2.885 ng/ml
8) t m-Xylene	13.197	206278	5.796 ng/ml
9) t O-Xylene	13.921	177000	5.722 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	143598	5.458 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072721\
Data File : FB026096.D
Signal(s) : FID2B.CH
Acq On : 27 Jul 2021 9:16
Operator : AJ/MA
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 27 11:13:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
Quant Title :
QLast Update : Tue Jul 27 11:12:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

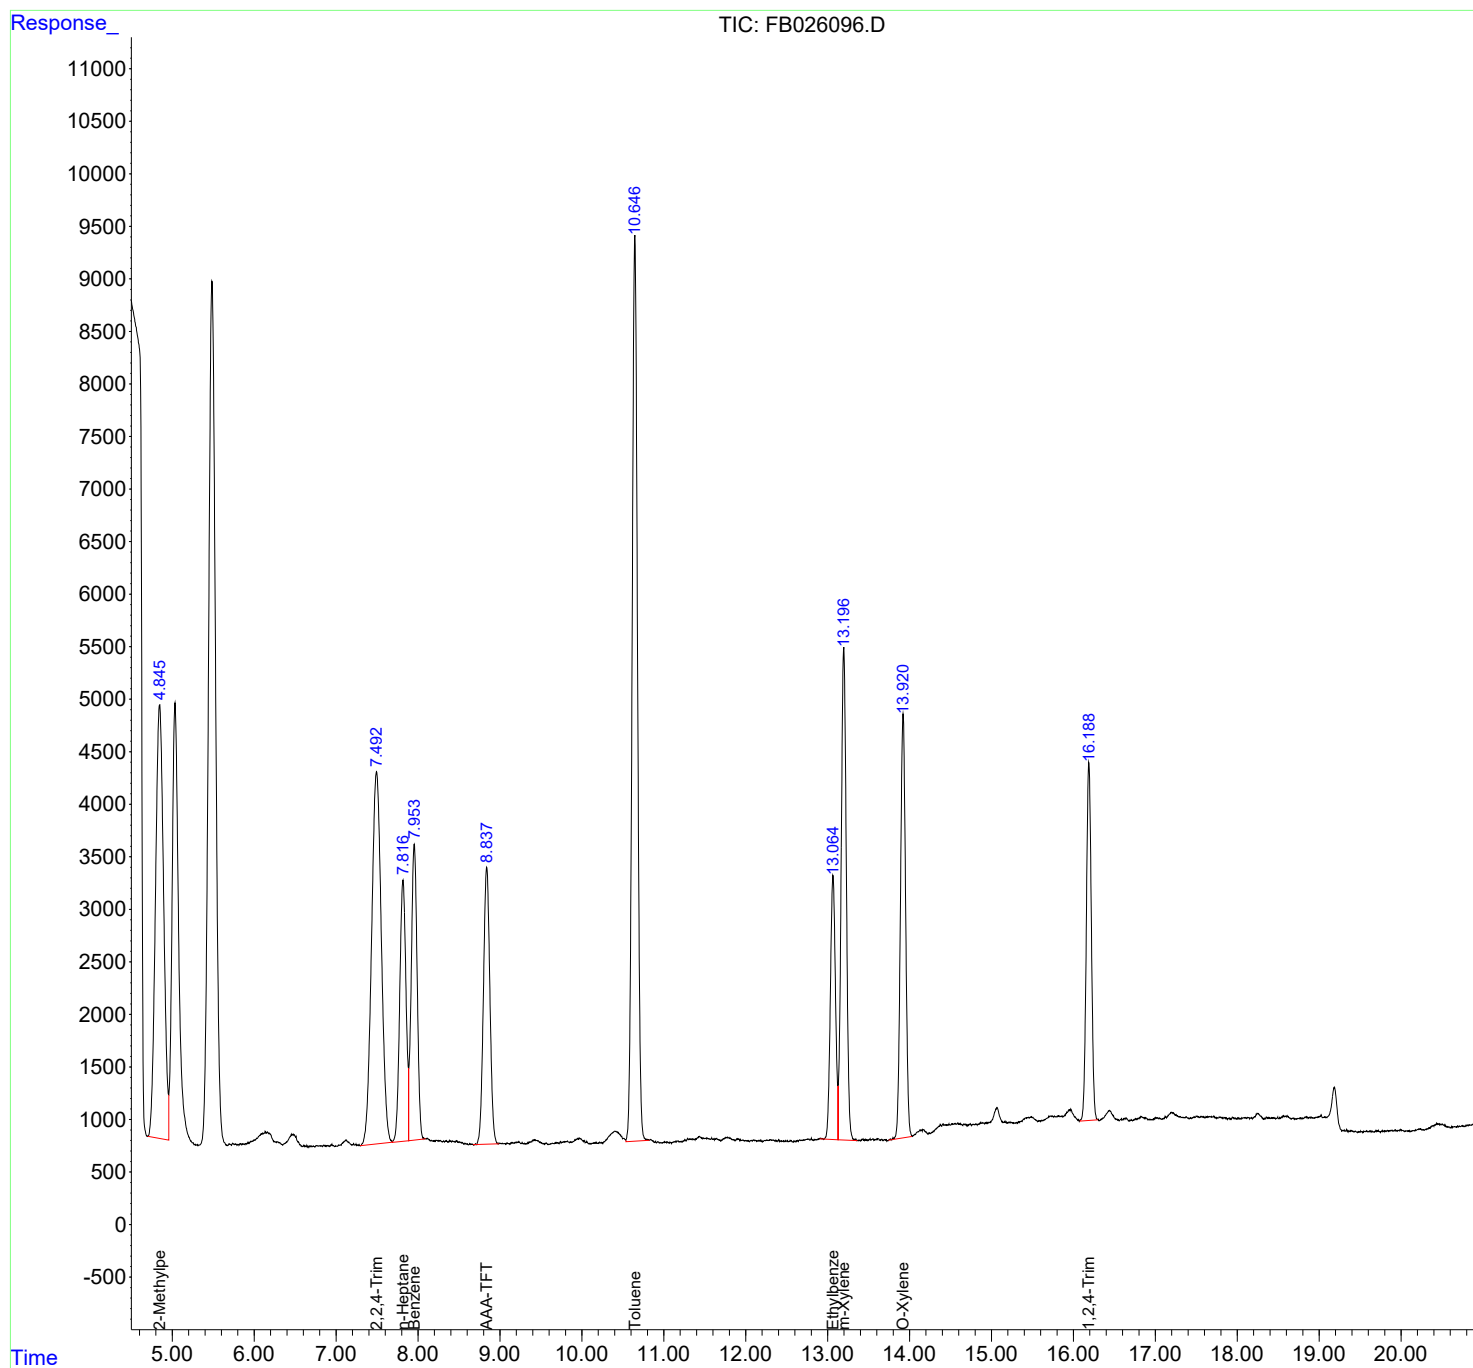


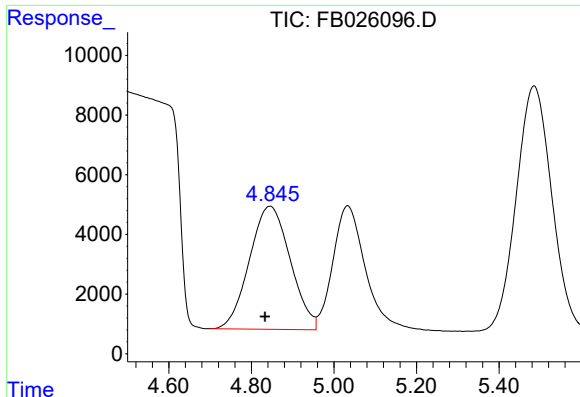

#1 2-Methylpentane


R.T.: 4.846 min
Delta R.T.: 0.013 min
Response: 283761
Conc: 8.62 ng/ml

Instrument :
FID_B
ClientSampleId :

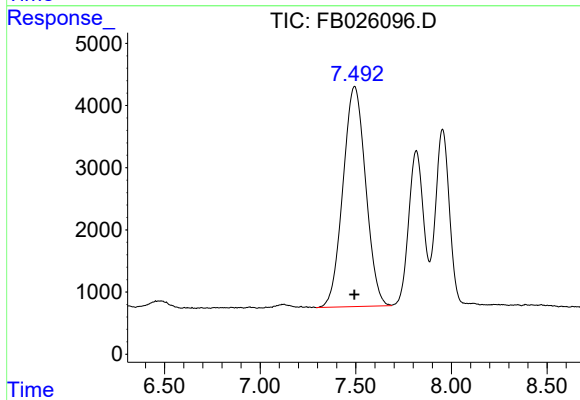


#2 2,2,4-Trimethylpentane

R.T.: 7.494 min
Delta R.T.: 0.000 min
Response: 292412
Conc: 9.05 ng/ml

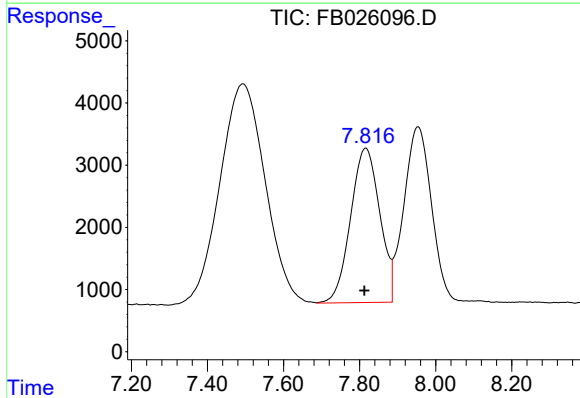


#3 n-Heptane

R.T.: 7.816 min
Delta R.T.: 0.004 min
Response: 132186
Conc: 2.90 ng/ml

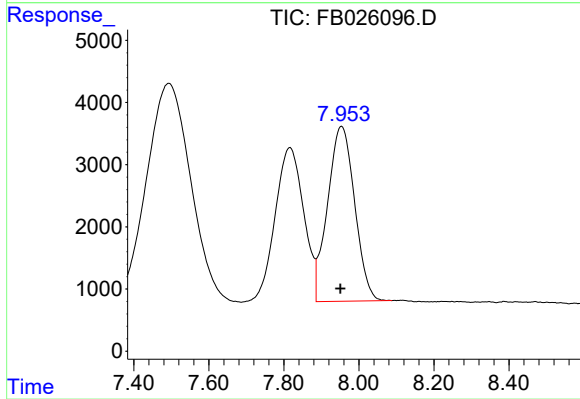

#4 Benzene


R.T.: 7.954 min
Delta R.T.: 0.004 min
Response: 141090
Conc: 2.95 ng/ml

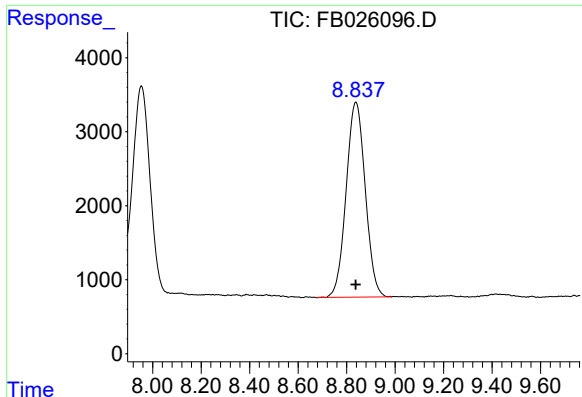

#5 AAA-TFT


R.T.: 8.839 min
Delta R.T.: 0.001 min
Response: 143916
Conc: 5.45 ng/ml

Instrument :
FID_B
ClientSampleId :

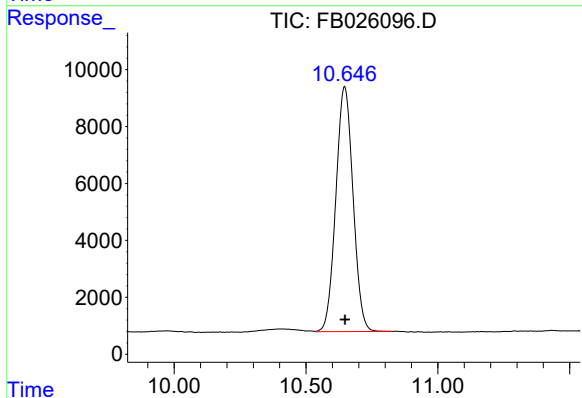


#6 Toluene

R.T.: 10.647 min
Delta R.T.: -0.001 min
Response: 390275
Conc: 8.74 ng/ml

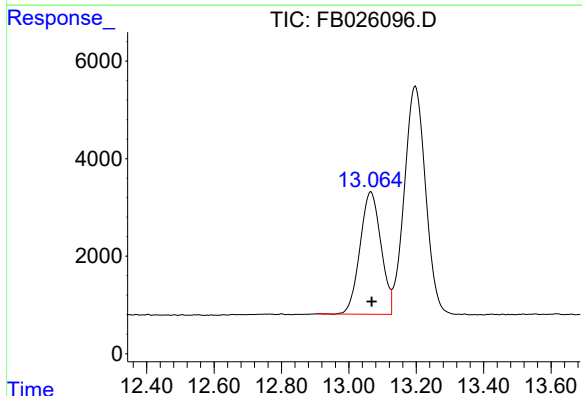


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.002 min
Response: 108364
Conc: 2.88 ng/ml

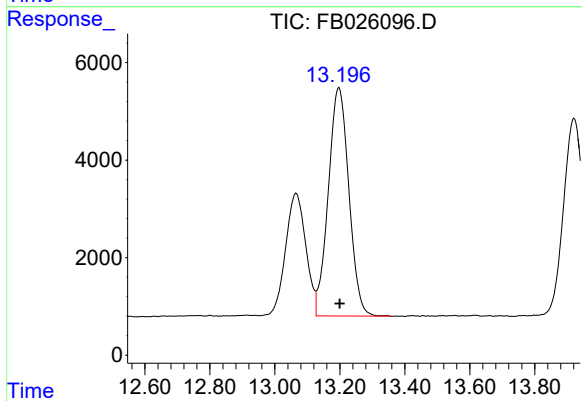

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: -0.003 min
Response: 206278
Conc: 5.80 ng/ml

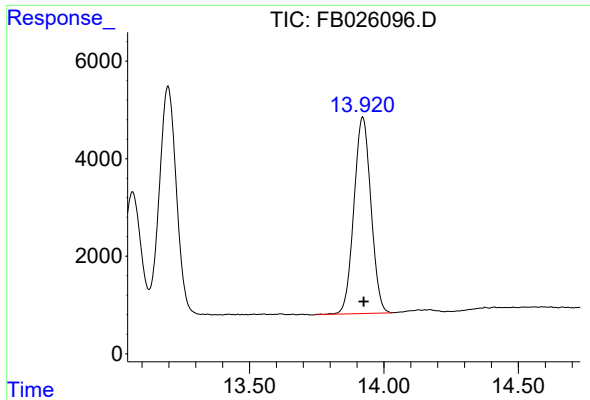

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: -0.003 min
Response: 177000
Conc: 5.72 ng/ml

Instrument :
FID_B
ClientSampleId :

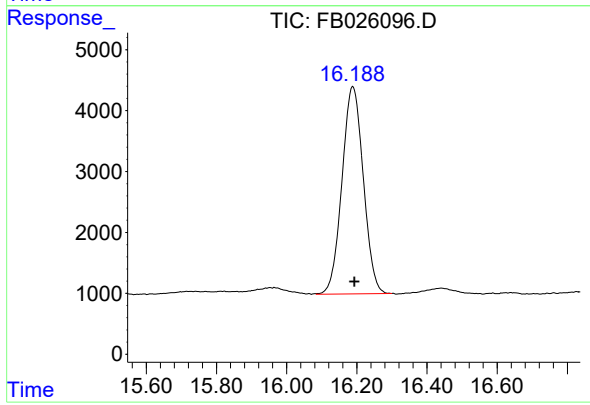

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.004 min
Response: 143598
Conc: 5.46 ng/ml