

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB072721\  
 Data File : FB026102.D  
 Signal(s) : FID2B.CH  
 Acq On : 27 Jul 2021 12:55  
 Operator : AJ/MA  
 Sample : VBF0727S1  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Jul 28 01:25:14 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB072721.M  
 Quant Title :  
 QLast Update : Tue Jul 27 12:01:49 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.846  | 541506   | 19.514 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.654 | 14070    | 0.309 ng/ml  |
| 8) t m-Xylene                | 13.211 | 15346    | 0.426 ng/ml  |
| 9) t O-Xylene                | 13.934 | 10620    | 0.343 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.205 | 11280    | 0.440 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB072721\  
Data File : FB026102.D  
Signal(s) : FID2B.CH  
Acq On : 27 Jul 2021 12:55  
Operator : AJ/MA  
Sample : VBF0727S1  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Jul 28 01:25:14 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB072721.M  
Quant Title :  
QLast Update : Tue Jul 27 12:01:49 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

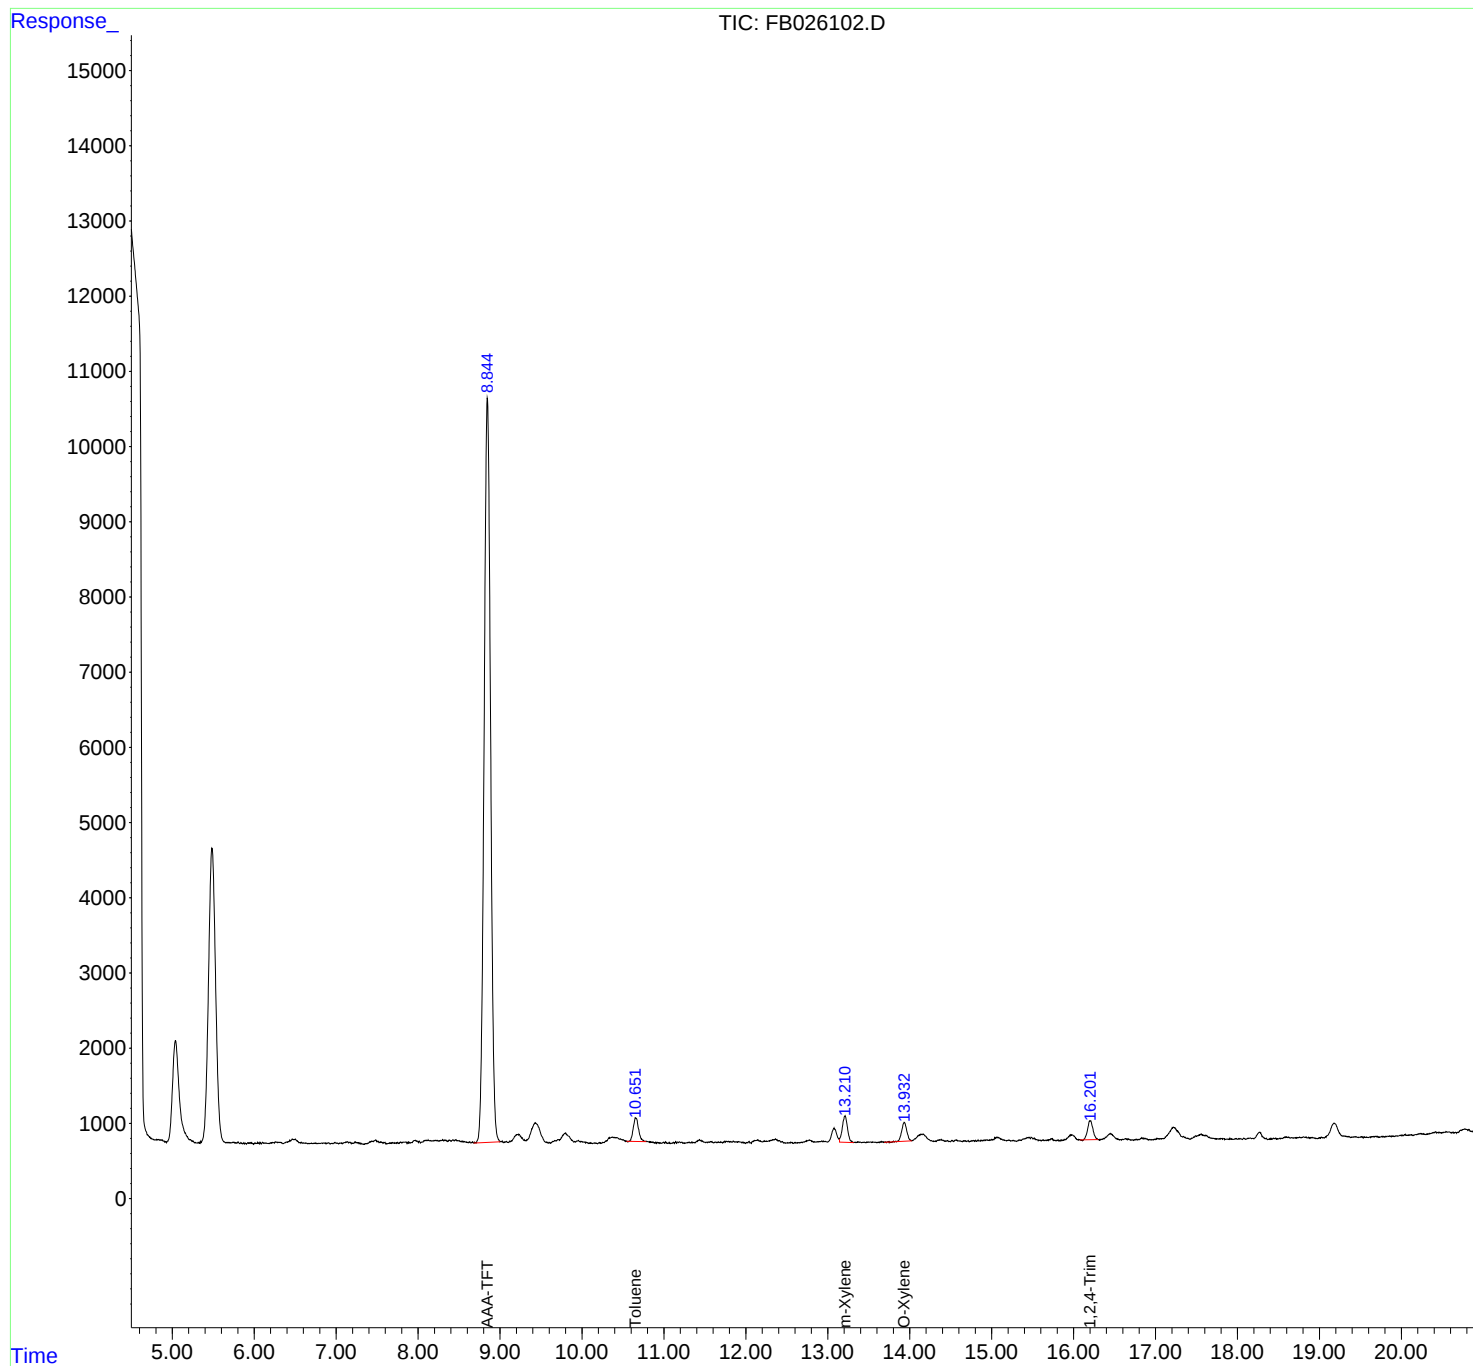


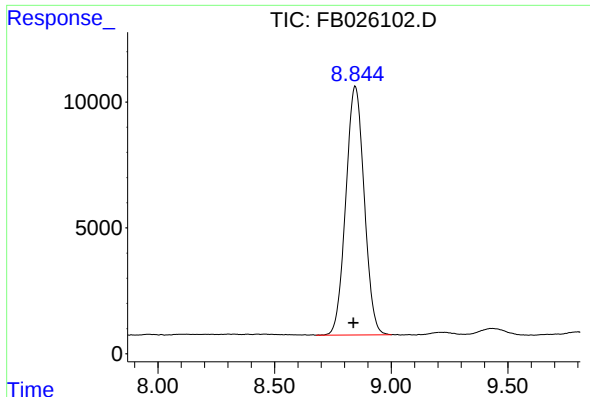

#5 AAA-TFT


R.T.: 8.846 min  
Delta R.T.: 0.008 min  
Response: 541506  
Conc: 19.51 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

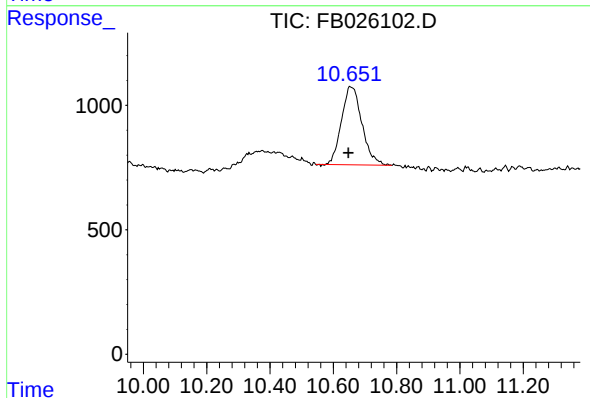


#6 Toluene

R.T.: 10.654 min  
Delta R.T.: 0.006 min  
Response: 14070  
Conc: 0.31 ng/ml

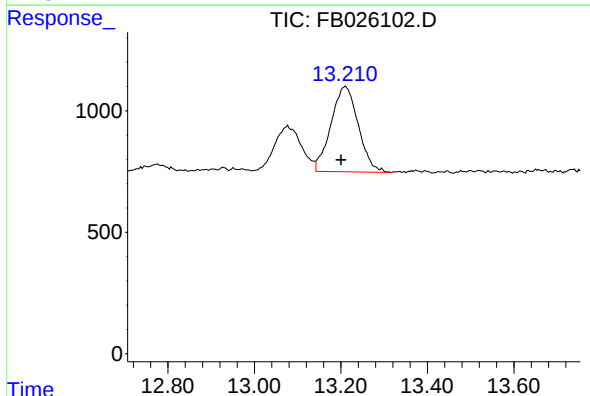


#8 m-Xylene

R.T.: 13.211 min  
Delta R.T.: 0.011 min  
Response: 15346  
Conc: 0.43 ng/ml

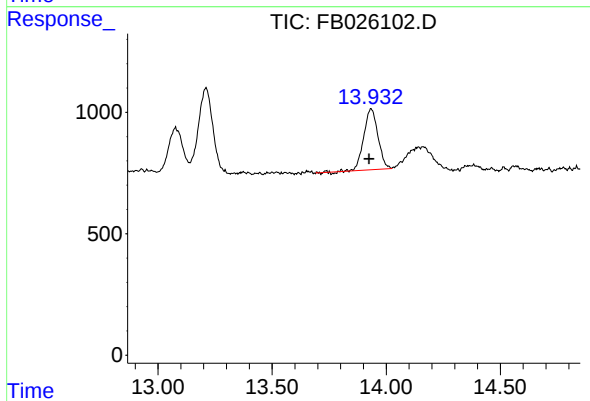

#9 O-Xylene

R.T.: 13.934 min  
Delta R.T.: 0.009 min  
Response: 10620  
Conc: 0.34 ng/ml

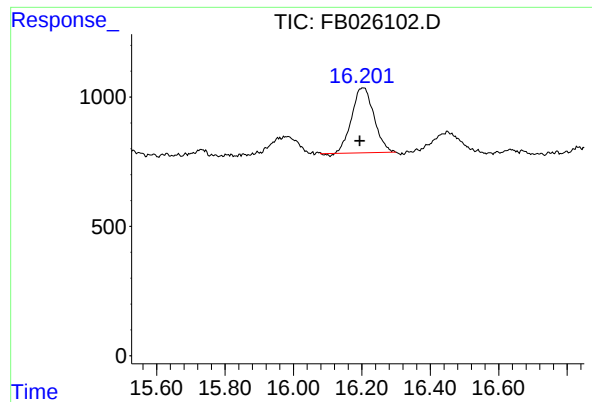

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min  
Delta R.T.: 0.012 min  
Response: 11280  
Conc: 0.44 ng/ml

Instrument :  
FID\_B  
ClientSampleId :