

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072721\
 Data File : FB026104.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jul 2021 14:09
 Operator : AJ/MA
 Sample : M3143-02
 Misc : 6.14G/5.00ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 28 01:25:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
 Quant Title :
 QLast Update : Tue Jul 27 12:01:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.844	374159	13.483 ng/ml
Target Compounds			
6) t Toluene	10.658	11680	0.257 ng/ml
8) t m-Xylene	13.206	11673	0.324 ng/ml
9) t O-Xylene	13.939	10696	0.345 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	9509	0.371 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072721\
Data File : FB026104.D
Signal(s) : FID2B.CH
Acq On : 27 Jul 2021 14:09
Operator : AJ/MA
Sample : M3143-02
Misc : 6.14G/5.00ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 28 01:25:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
Quant Title :
QLast Update : Tue Jul 27 12:01:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

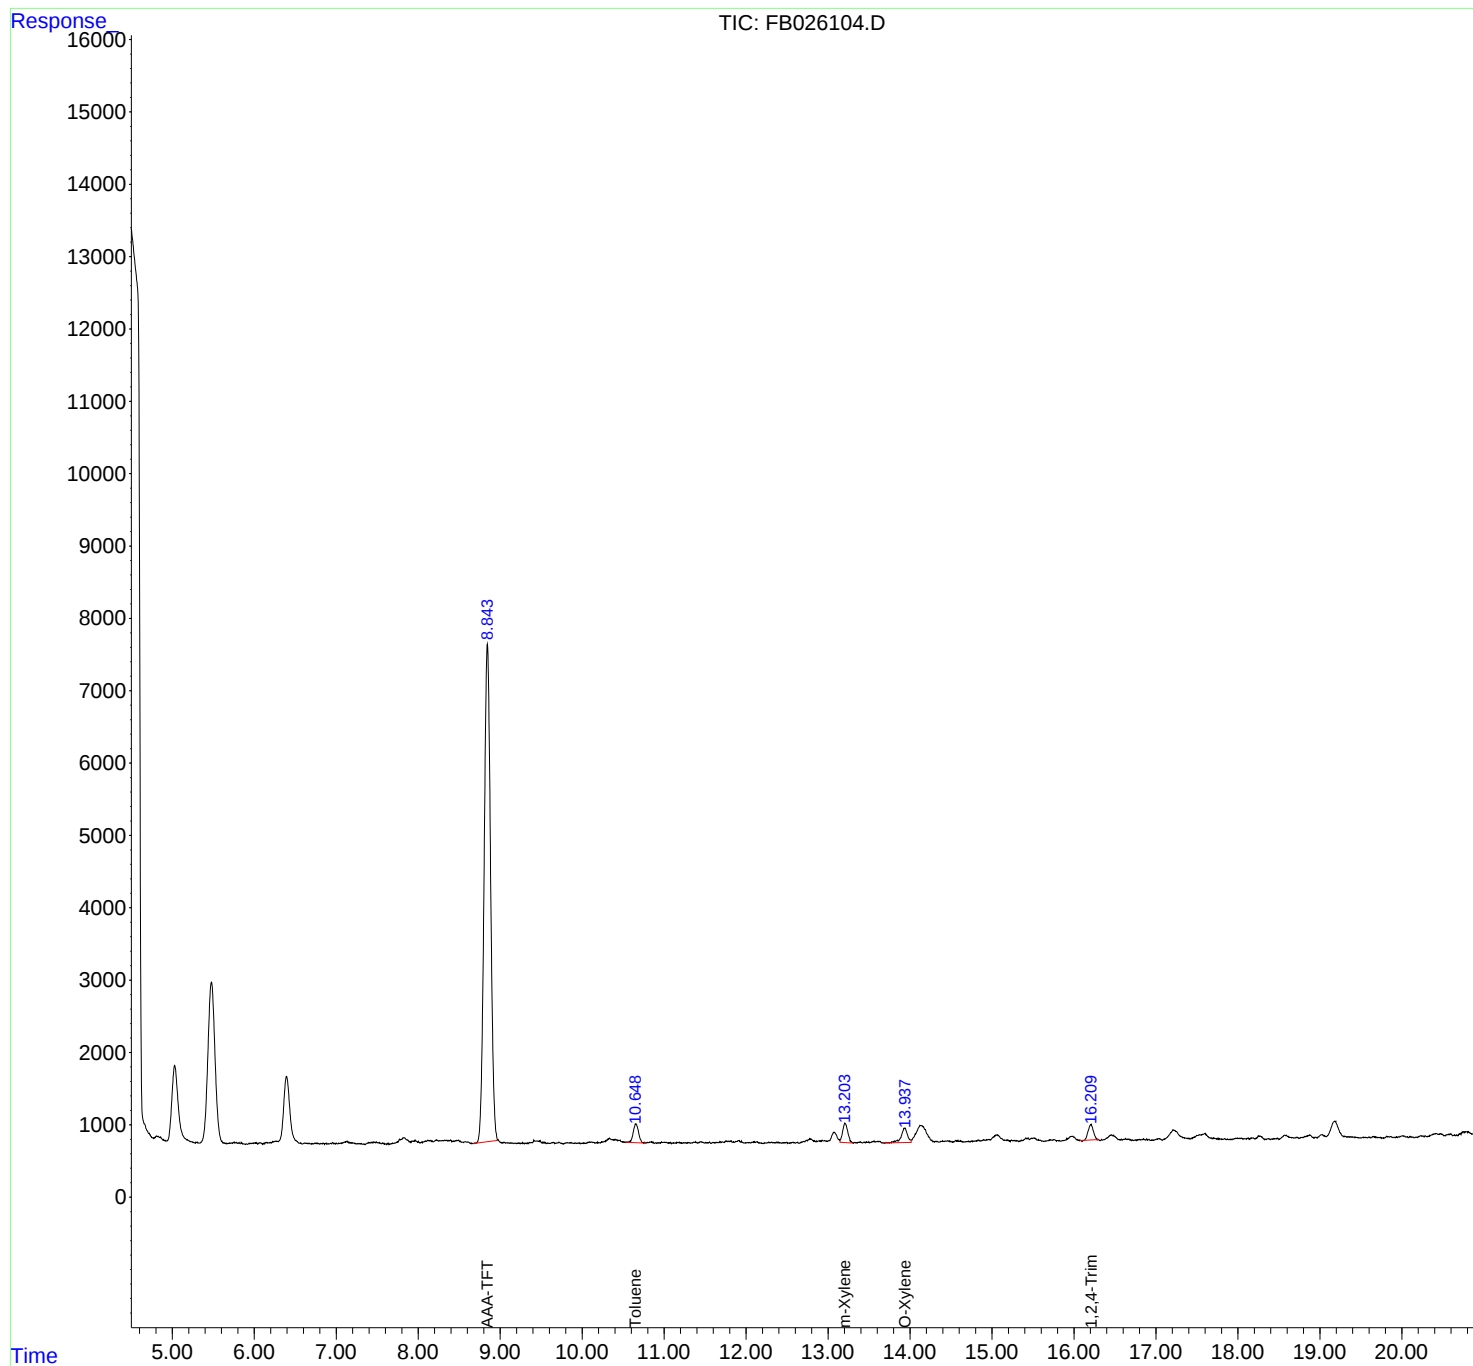


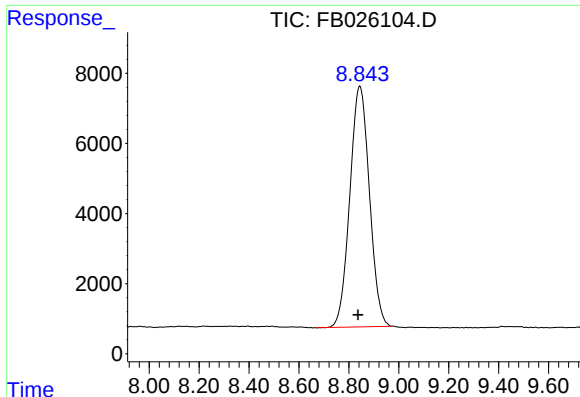

#5 AAA-TFT


R.T.: 8.844 min
Delta R.T.: 0.007 min
Response: 374159
Conc: 13.48 ng/ml

Instrument :
FID_B
ClientSampleId :

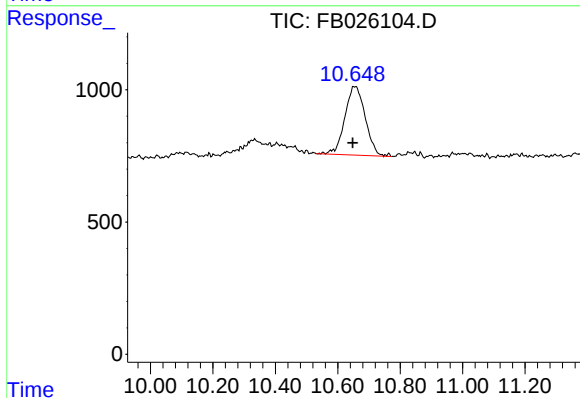


#6 Toluene

R.T.: 10.658 min
Delta R.T.: 0.010 min
Response: 11680
Conc: 0.26 ng/ml

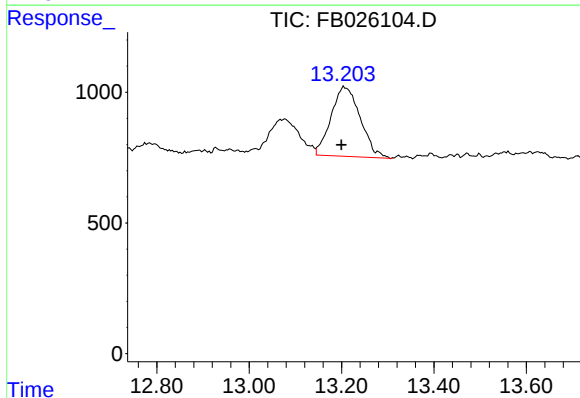


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.006 min
Response: 11673
Conc: 0.32 ng/ml

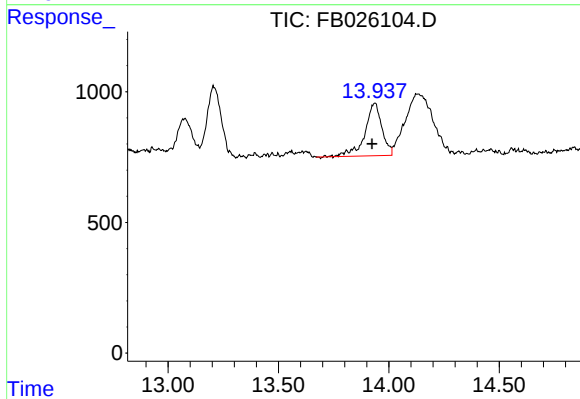

#9 O-Xylene

R.T.: 13.939 min
Delta R.T.: 0.014 min
Response: 10696
Conc: 0.34 ng/ml

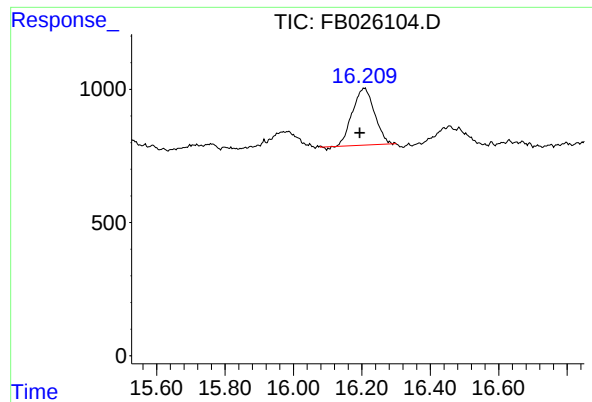

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.015 min
Response: 9509
Conc: 0.37 ng/ml

Instrument :
FID_B
ClientSampleId :