

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072722\
 Data File : FB027766.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jul 2022 10:55
 Operator : AJ/MA
 Sample : BSF0727S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0727S1

Integration File: Calibration.e
 Quant Time: Jul 28 03:55:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	235651	20.248 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	399715	18.980 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	515767	24.854 ng/ml
3) t n-Heptane	7.748	126354	6.146 ng/ml
4) t Benzene	7.887	210966	8.990 ng/ml
6) t Toluene	10.620	614222	27.507 ng/ml
7) t Ethylbenzene	13.058	208625	9.956 ng/ml
8) t m-Xylene	13.191	402347	19.216 ng/ml
9) t O-Xylene	13.918	387680	18.946 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	408736	19.668 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072722\
Data File : FB072766.D
Signal(s) : FID2B.CH
Acq On : 27 Jul 2022 10:55
Operator : AJ/MA
Sample : BSF0727S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0727S1

Integration File: Calibration.e
Quant Time: Jul 28 03:55:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

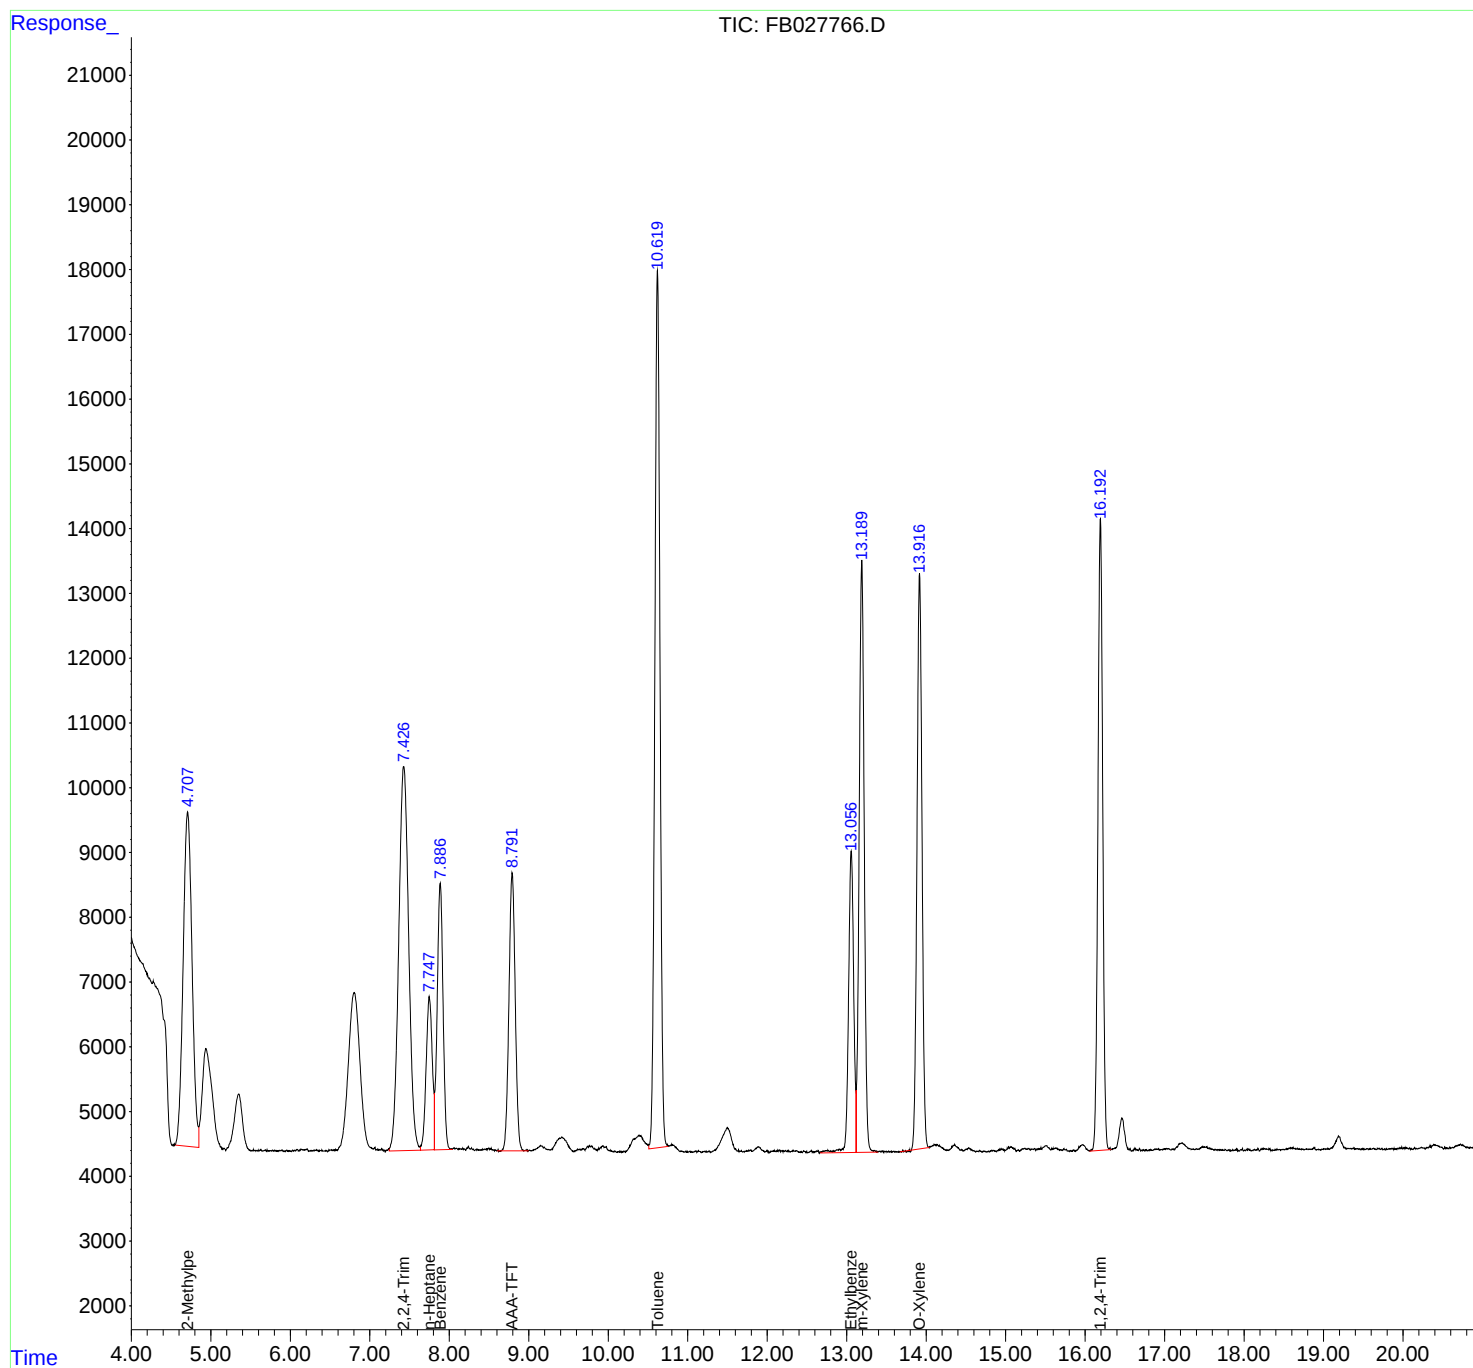


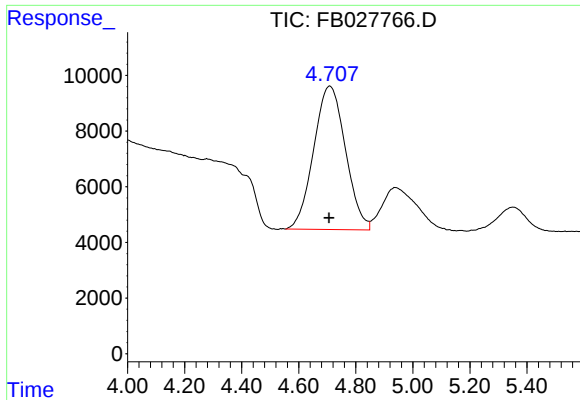

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.002 min
Response: 399715
Conc: 18.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0727S1

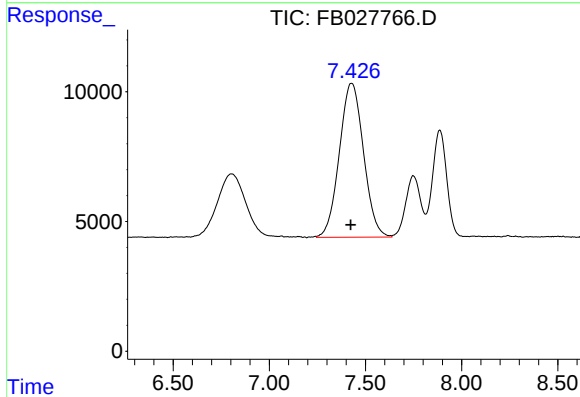


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: 0.004 min
Response: 515767
Conc: 24.85 ng/ml

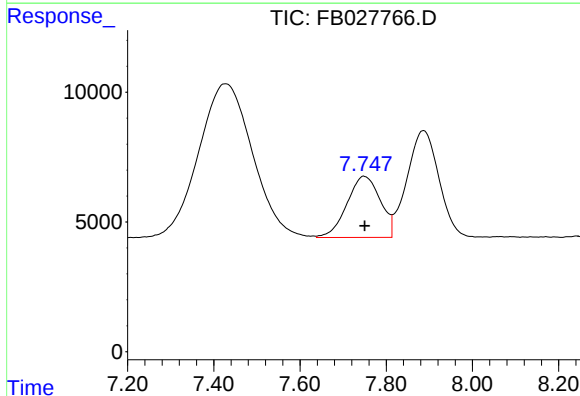


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.002 min
Response: 126354
Conc: 6.15 ng/ml

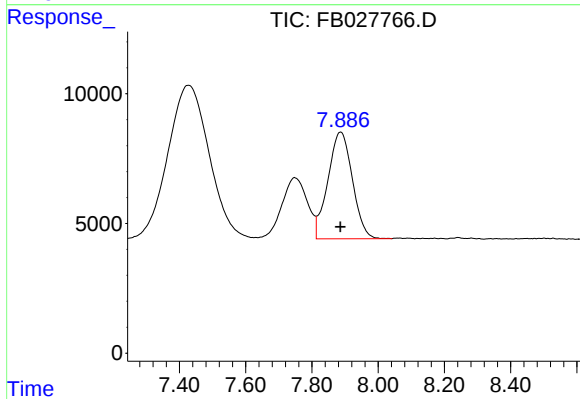

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 210966
Conc: 8.99 ng/ml

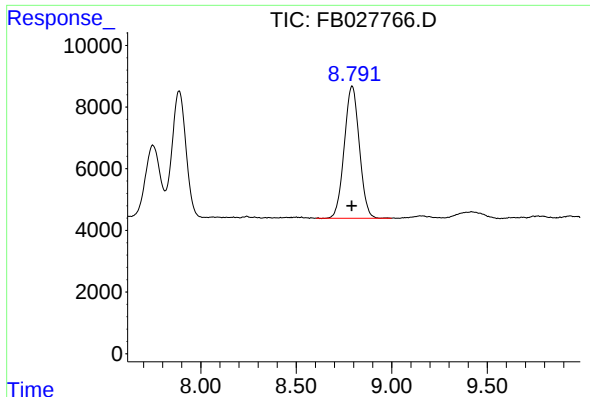

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.002 min
Response: 235651
Conc: 20.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0727S1

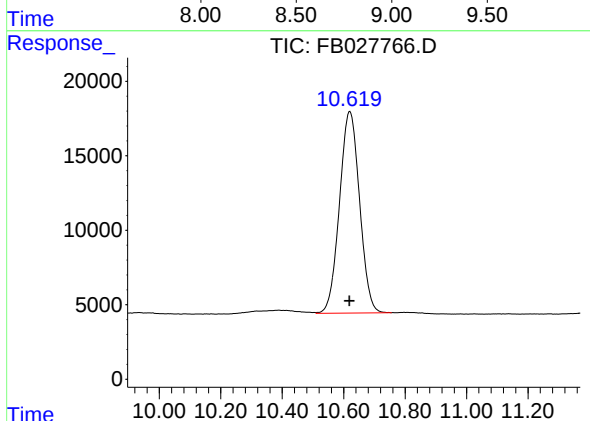


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.001 min
Response: 614222
Conc: 27.51 ng/ml

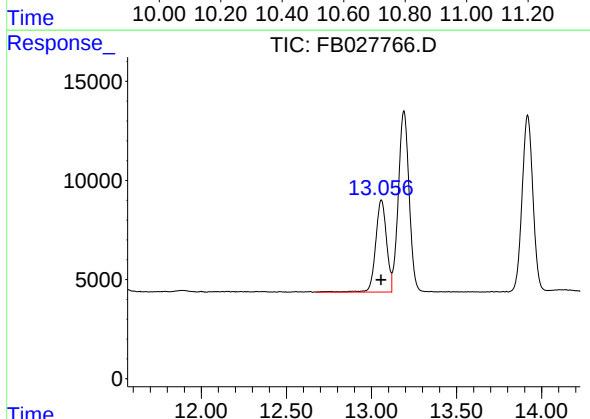


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.002 min
Response: 208625
Conc: 9.96 ng/ml

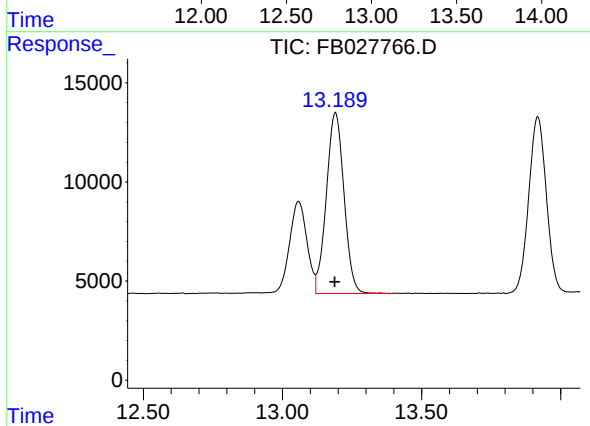

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.003 min
Response: 402347
Conc: 19.22 ng/ml

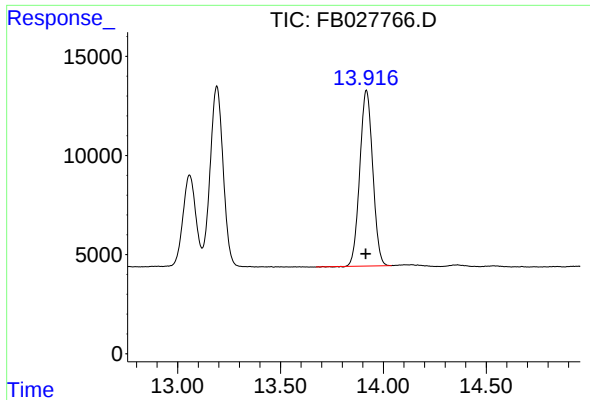

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 387680
Conc: 18.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0727S1

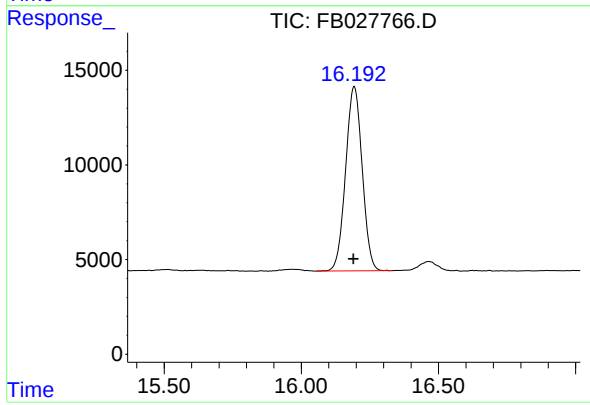

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.003 min
Response: 408736
Conc: 19.67 ng/ml