

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072722\
 Data File : FB027767.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jul 2022 11:31
 Operator : AJ/MA
 Sample : BSF0727S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0727S2

Integration File: Calibration.e
 Quant Time: Jul 28 03:55:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	256379	22.029 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	403957	19.182 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	514772	24.806 ng/ml
3) t n-Heptane	7.751	127906	6.222 ng/ml
4) t Benzene	7.888	215959	9.203 ng/ml
6) t Toluene	10.622	622872	27.894 ng/ml
7) t Ethylbenzene	13.059	205586	9.811 ng/ml
8) t m-Xylene	13.192	407460	19.460 ng/ml
9) t O-Xylene	13.919	399350	19.516 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	403735	19.428 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072722\
Data File : FB072767.D
Signal(s) : FID2B.CH
Acq On : 27 Jul 2022 11:31
Operator : AJ/MA
Sample : BSF0727S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0727S2

Integration File: Calibration.e
Quant Time: Jul 28 03:55:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

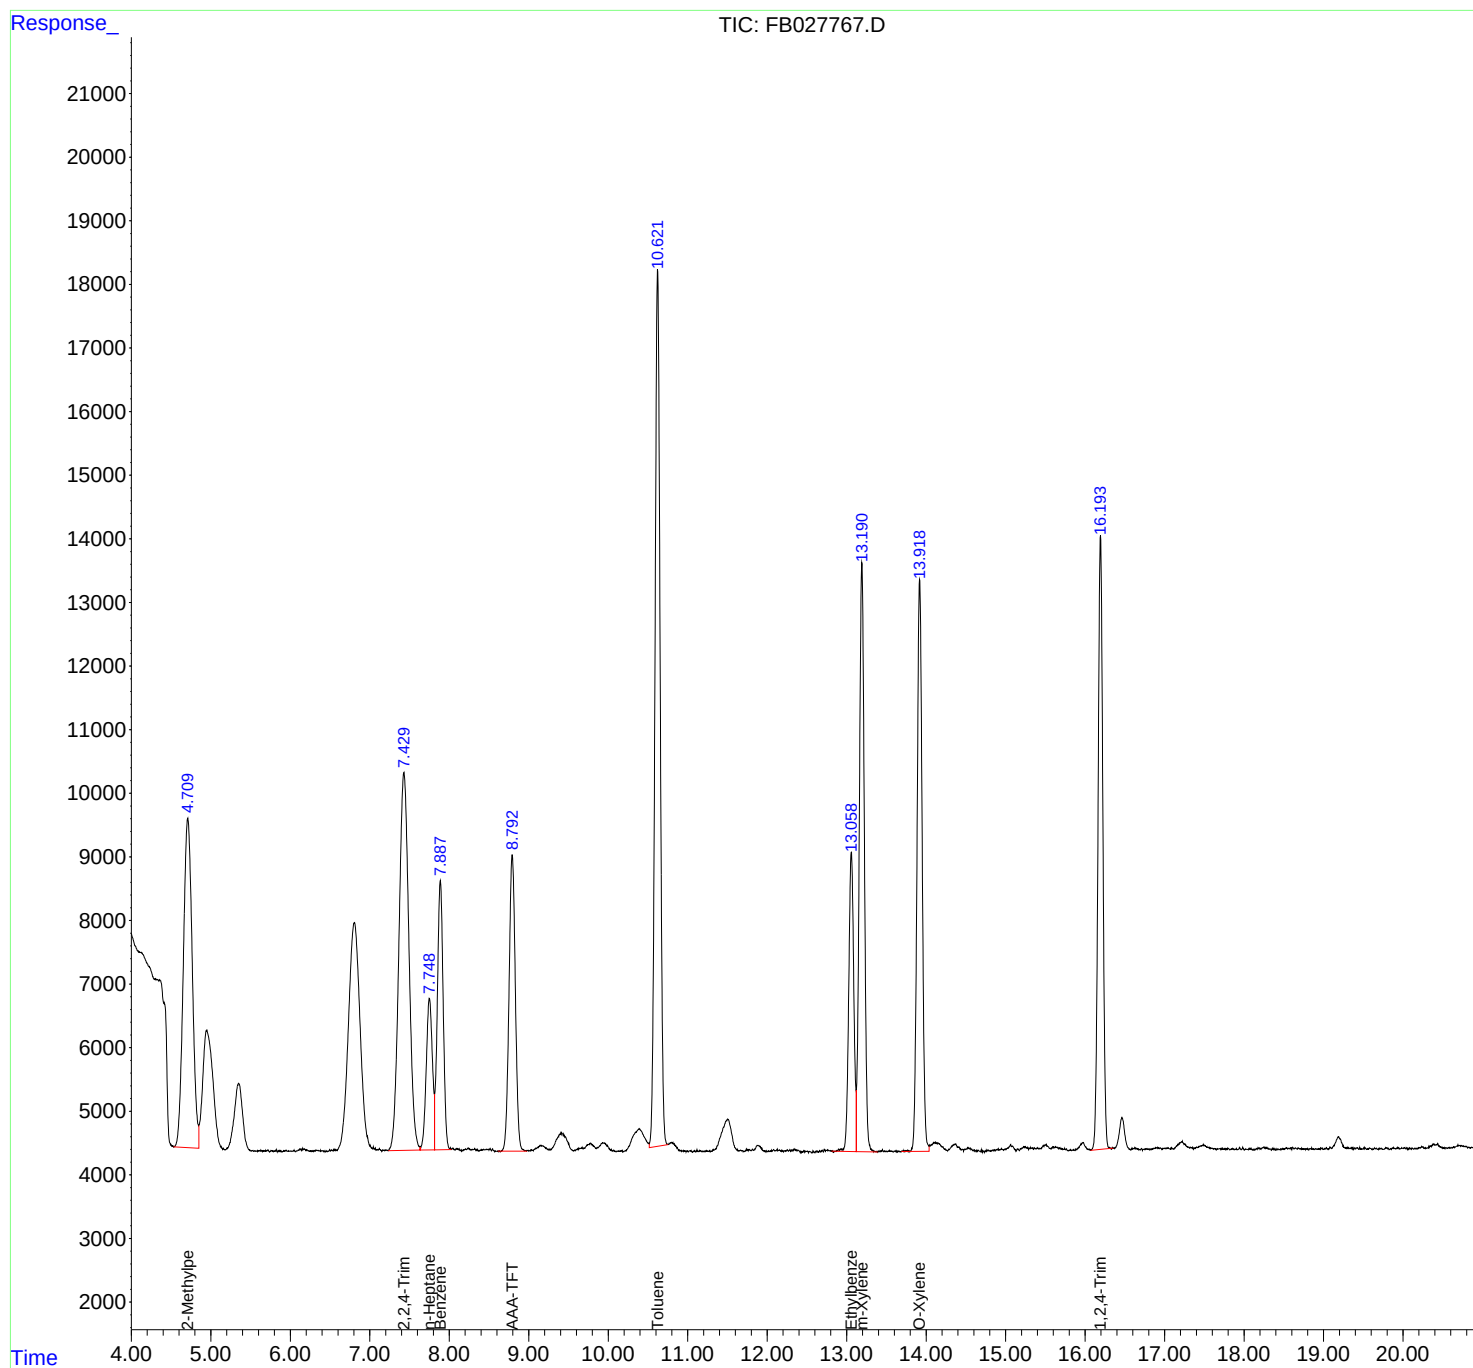


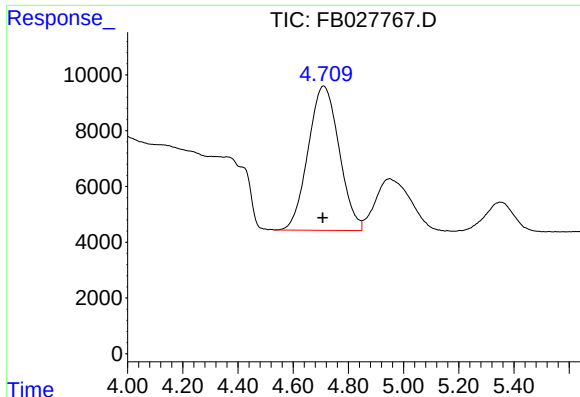

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.004 min
Response: 403957
Conc: 19.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0727S2

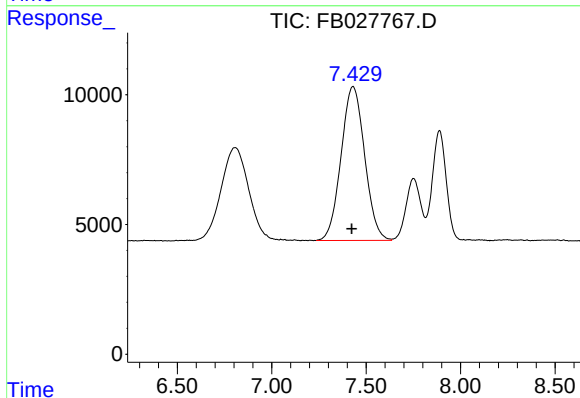


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: 0.007 min
Response: 514772
Conc: 24.81 ng/ml

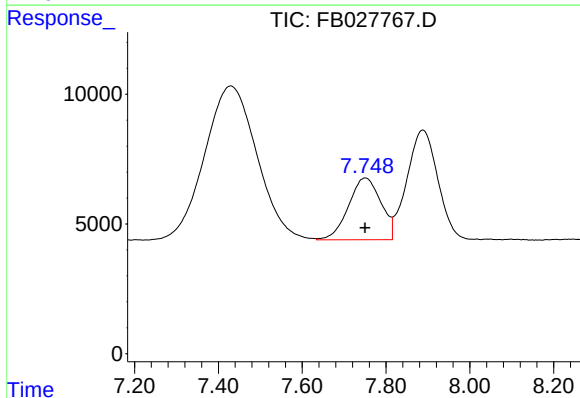


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.001 min
Response: 127906
Conc: 6.22 ng/ml

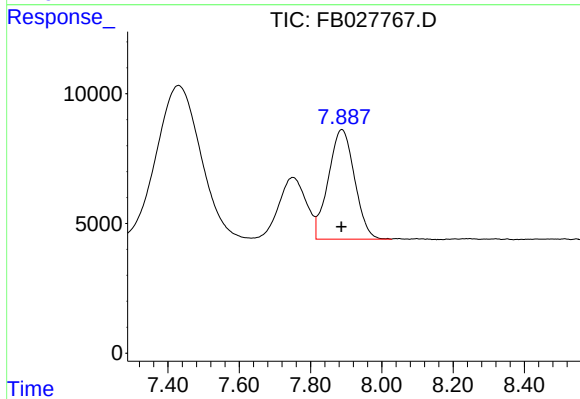

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 215959
Conc: 9.20 ng/ml

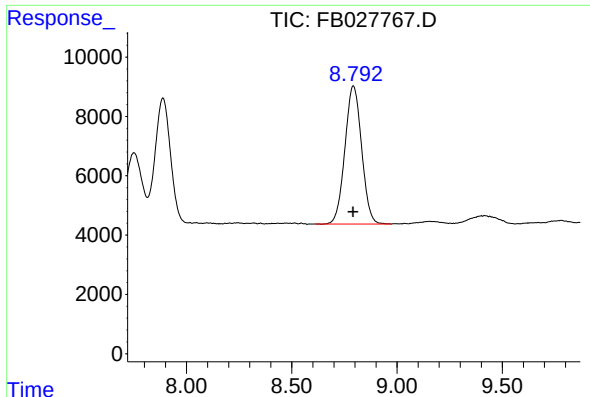

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.002 min
Response: 256379
Conc: 22.03 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0727S2

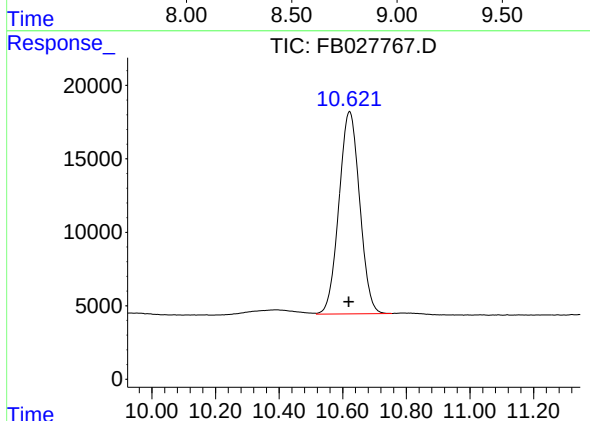


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.003 min
Response: 622872
Conc: 27.89 ng/ml

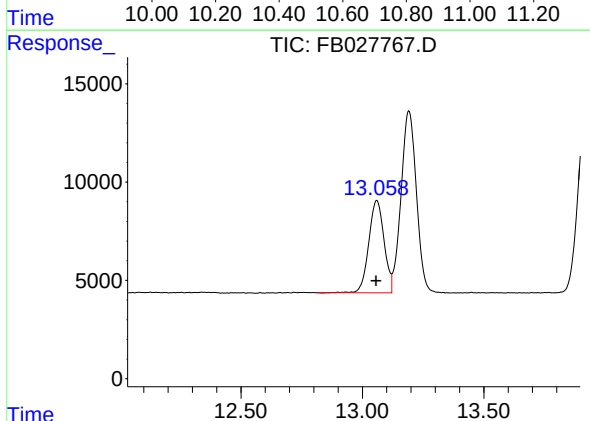


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.004 min
Response: 205586
Conc: 9.81 ng/ml

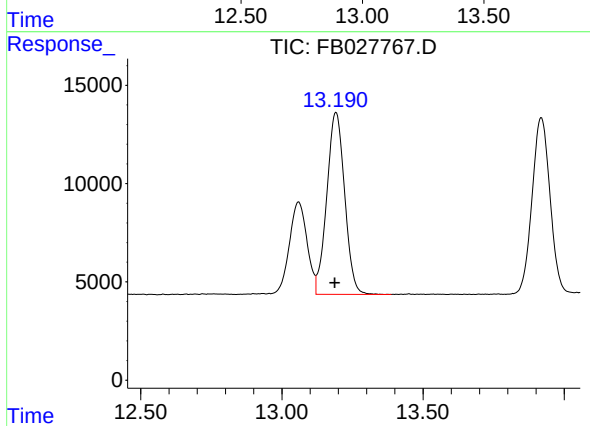

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.004 min
Response: 407460
Conc: 19.46 ng/ml

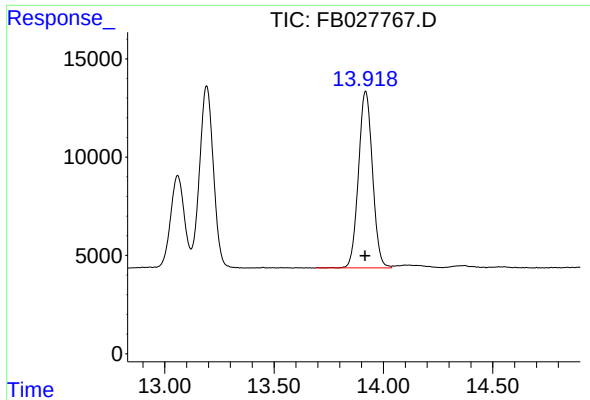

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.004 min
Response: 399350
Conc: 19.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0727S2

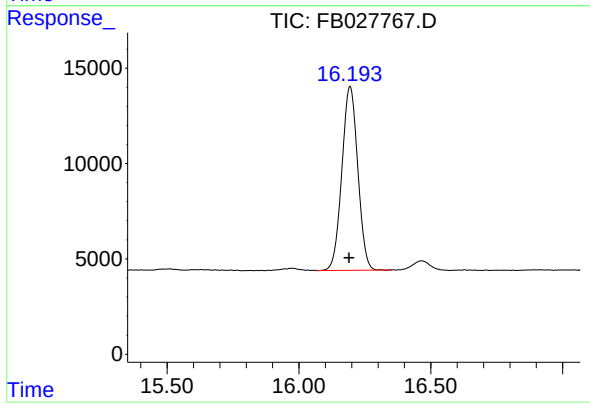

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.004 min
Response: 403735
Conc: 19.43 ng/ml