

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072919\
 Data File : FB021843.D
 Signal(s) : FID2B.CH
 Acq On : 29 Jul 2019 12:47
 Operator : DD/AJ
 Sample : BSF0729S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 30 00:48:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.990	293065	21.475 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.864	759927	27.557 ng/ml
2) t	2,2,4-Trimethylpentane	7.609	796240	30.121 ng/ml
3) t	n-Heptane	7.949	240418	9.696 ng/ml
4) t	Benzene	8.084	298205	10.207 ng/ml
6) t	Toluene	10.830	618931	30.080 ng/ml
7) t	Ethylbenzene	13.275	218349	10.495 ng/ml
8) t	m-Xylene	13.408	464317	20.901 ng/ml
9) t	O-Xylene	14.137	481782	20.945 ng/ml
10) t	1,2,4-Trimethylbenzene	16.417	496459	21.057 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072919\
Data File : FB021843.D
Signal(s) : FID2B.CH
Acq On : 29 Jul 2019 12:47
Operator : DD/AJ
Sample : BSF0729S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 30 00:48:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

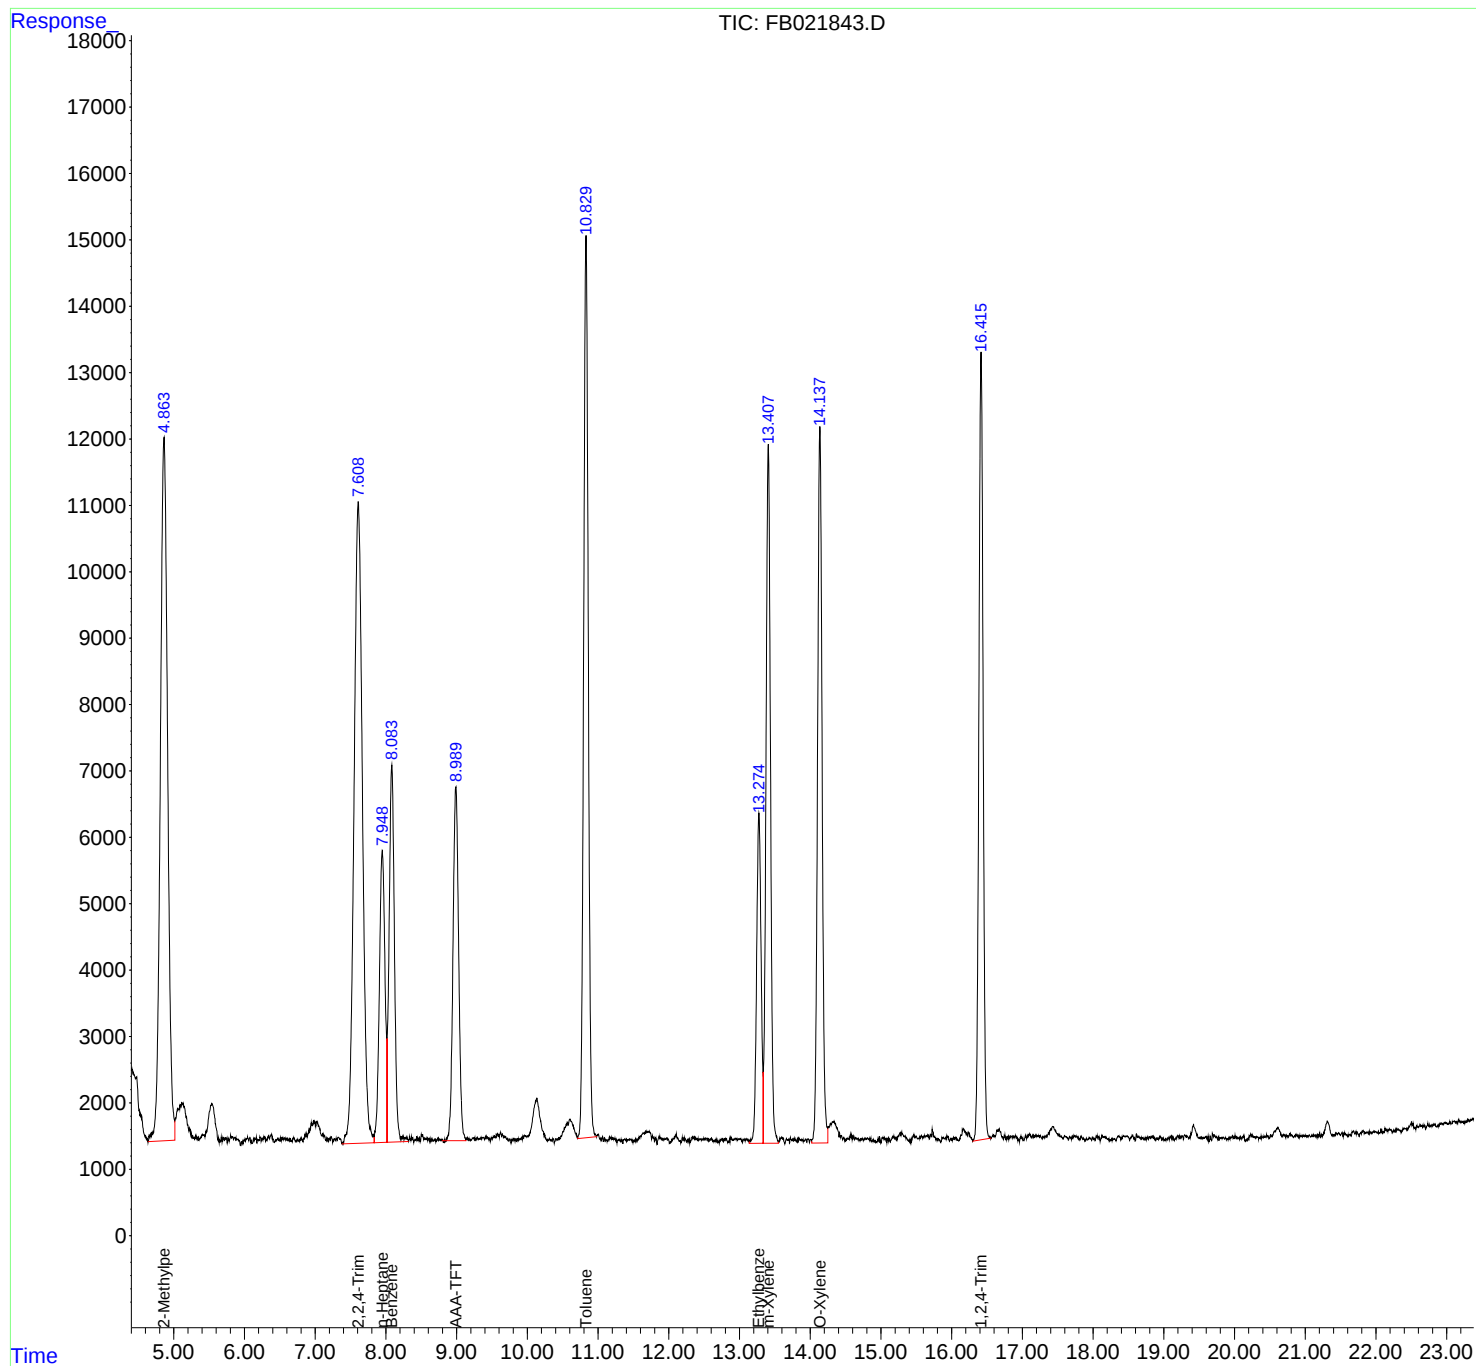

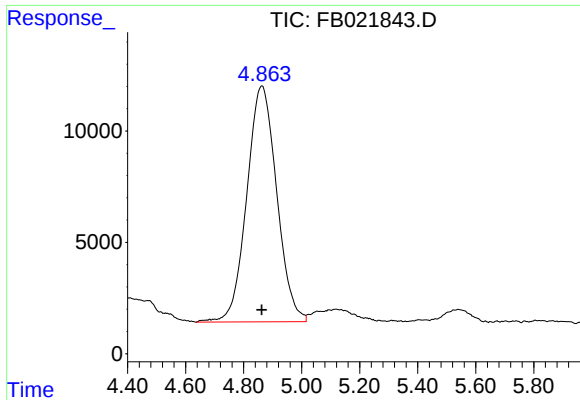


#1 2-Methylpentane

R.T.: 4.864 min
Delta R.T.: 0.001 min
Response: 759927
Conc: 27.56 ng/ml

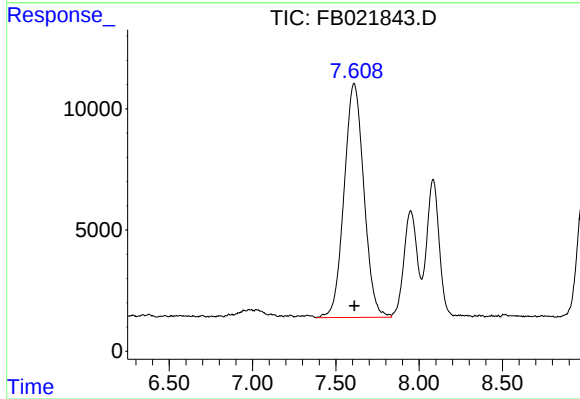


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.003 min
Response: 796240
Conc: 30.12 ng/ml

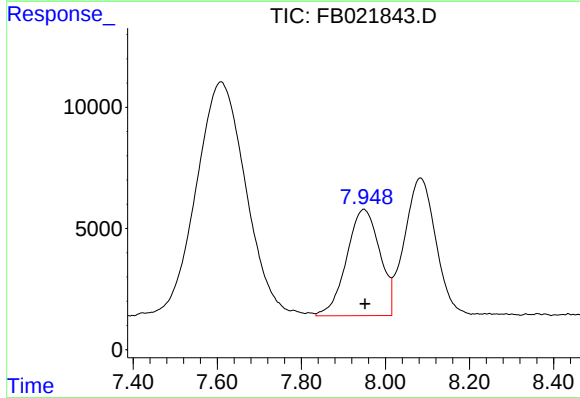


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 240418
Conc: 9.70 ng/ml

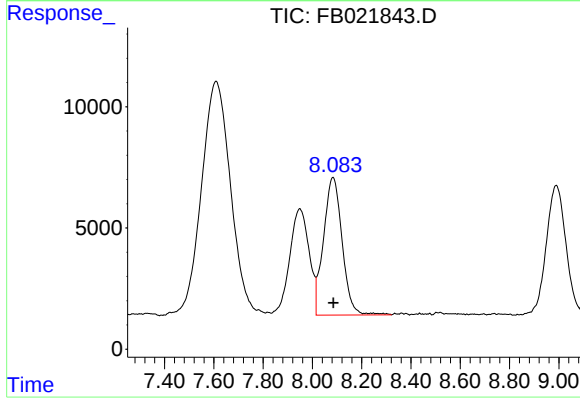


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 298205
Conc: 10.21 ng/ml

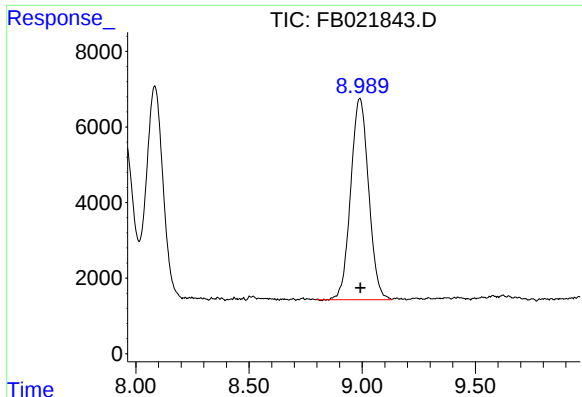


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.002 min
Response: 293065
Conc: 21.48 ng/ml

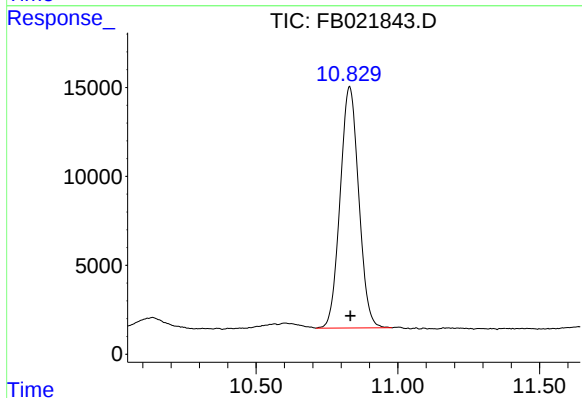


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.003 min
Response: 618931
Conc: 30.08 ng/ml

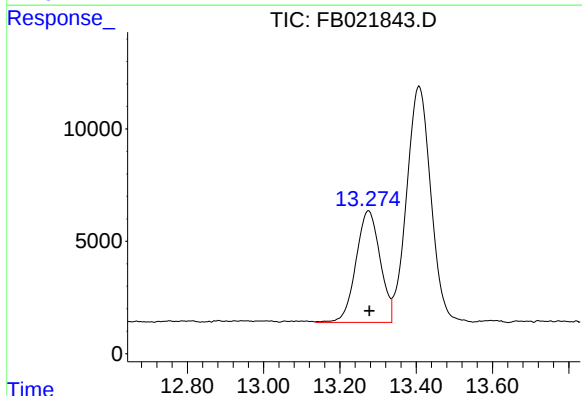


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: -0.002 min
Response: 218349
Conc: 10.50 ng/ml

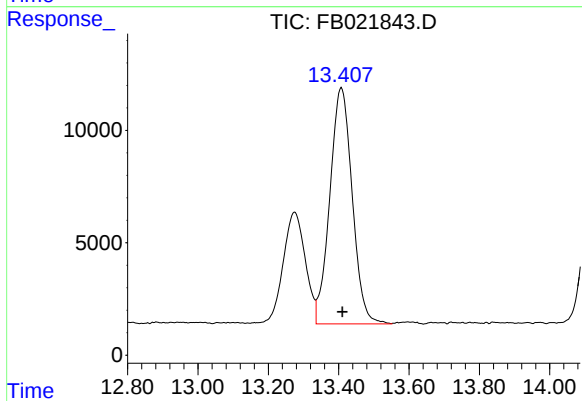


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: -0.003 min
Response: 464317
Conc: 20.90 ng/ml

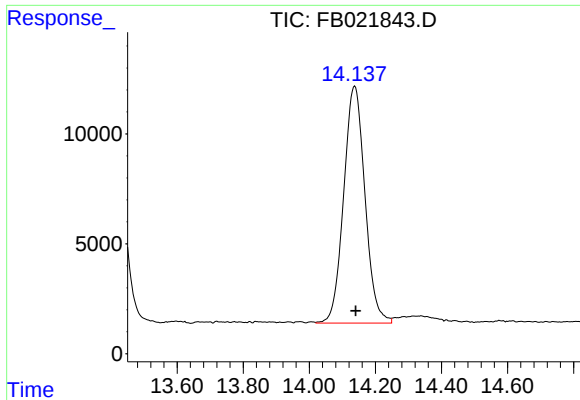

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: -0.003 min
Response: 481782
Conc: 20.94 ng/ml

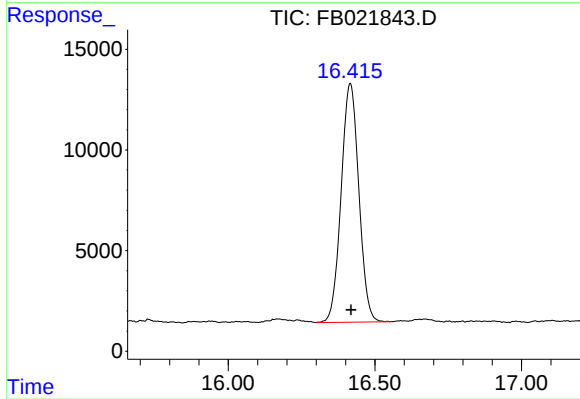

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.003 min
Response: 496459
Conc: 21.06 ng/ml