

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072919\
 Data File : FB021845.D
 Signal(s) : FID2B.CH
 Acq On : 29 Jul 2019 13:47
 Operator : DD/AJ
 Sample : K4044-01MS
 Misc : 5.04/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 30 00:48:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.990	309996	22.716 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.863	729348	26.449 ng/ml
2) t	2,2,4-Trimethylpentane	7.611	728401	27.555 ng/ml
3) t	n-Heptane	7.949	223505	9.014 ng/ml
4) t	Benzene	8.084	297229	10.174 ng/ml
6) t	Toluene	10.831	613007	29.792 ng/ml
7) t	Ethylbenzene	13.277	207824	9.989 ng/ml
8) t	m-Xylene	13.409	451387	20.319 ng/ml
9) t	O-Xylene	14.138	470433	20.451 ng/ml
10) t	1,2,4-Trimethylbenzene	16.417	483714	20.517 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072919\
Data File : FB021845.D
Signal(s) : FID2B.CH
Acq On : 29 Jul 2019 13:47
Operator : DD/AJ
Sample : K4044-01MS
Misc : 5.04/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 30 00:48:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

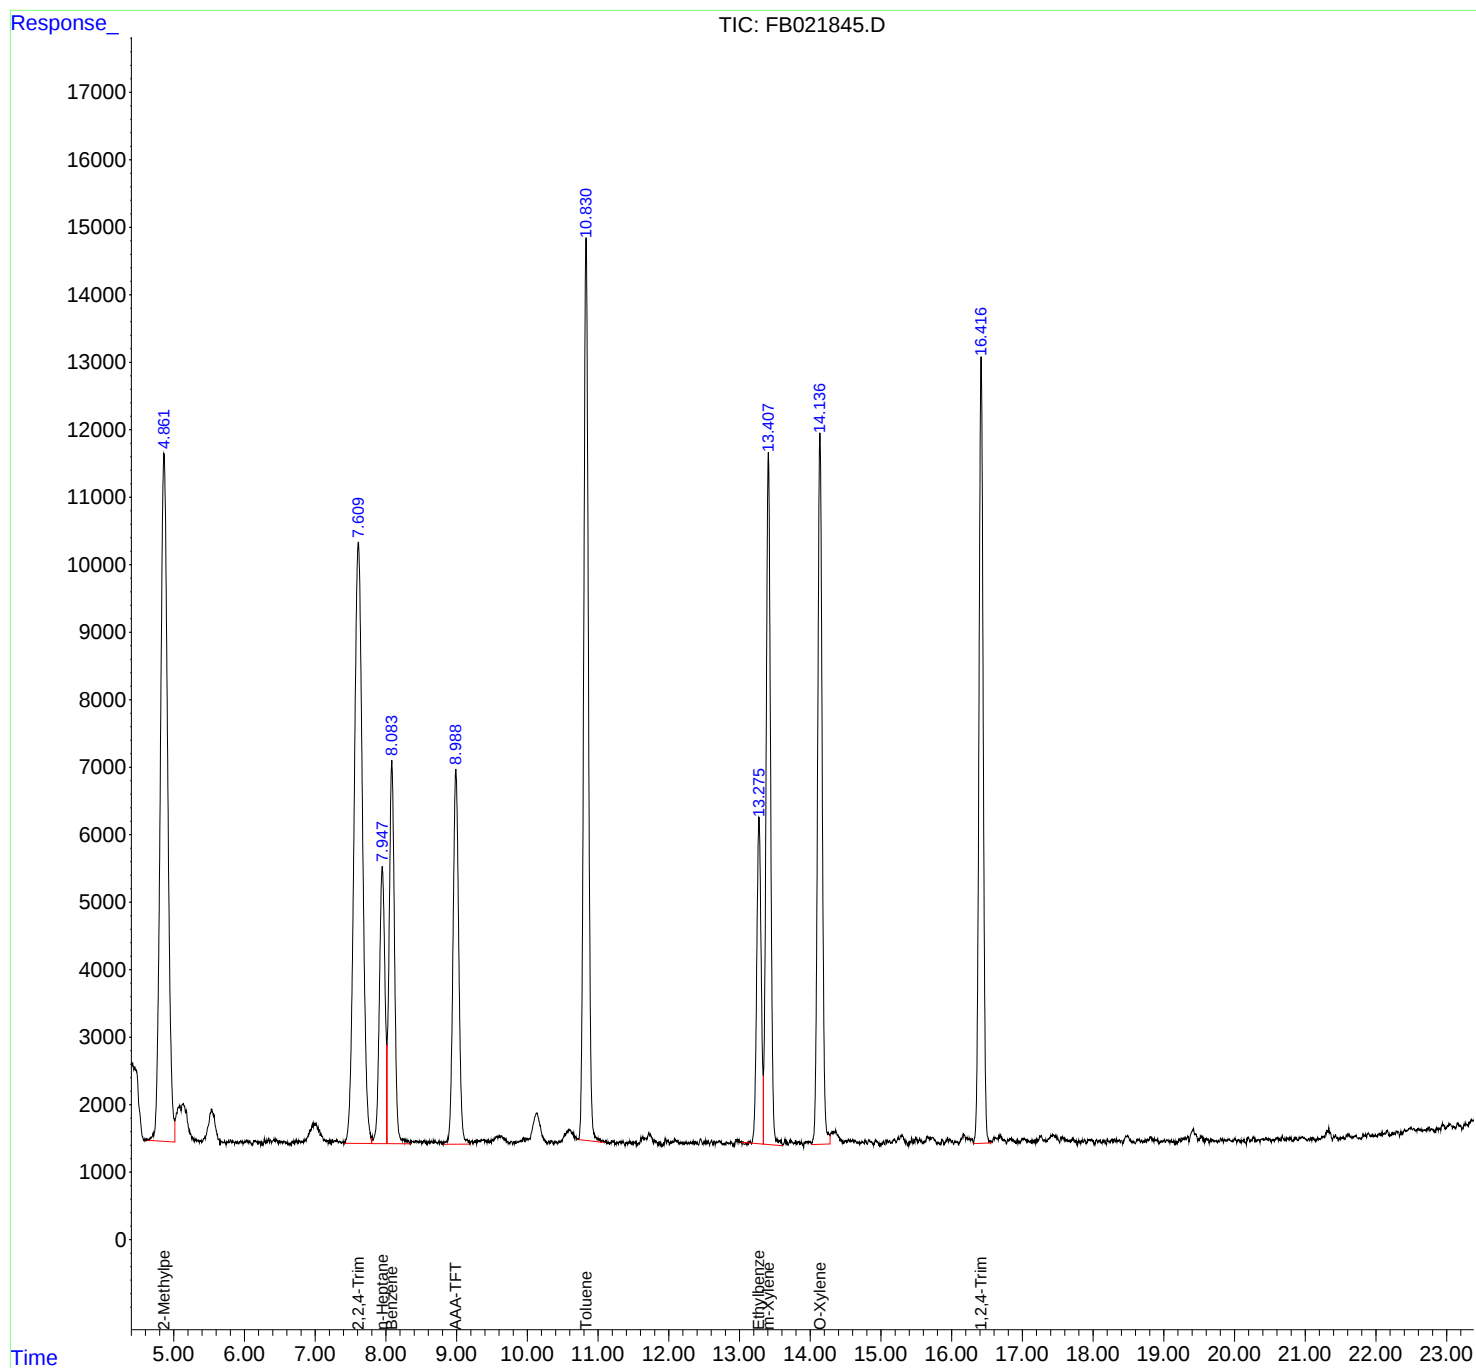

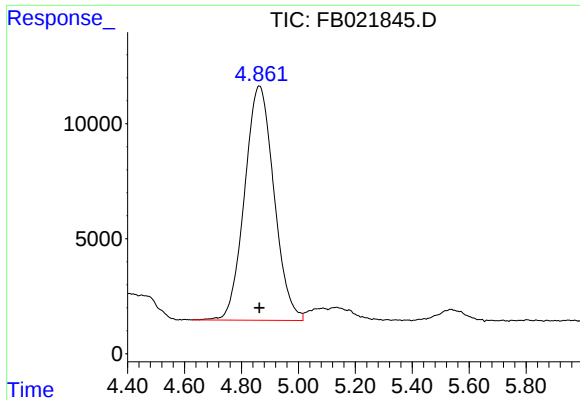


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 729348
Conc: 26.45 ng/ml

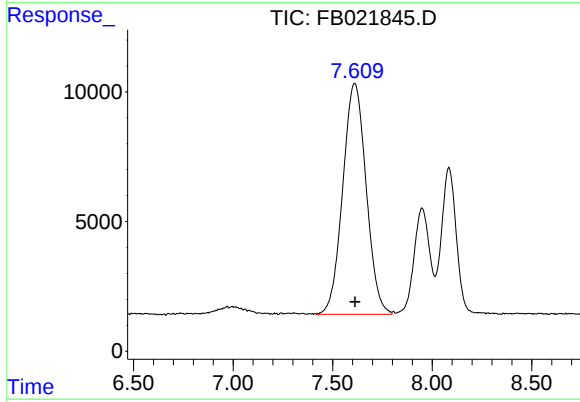


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.001 min
Response: 728401
Conc: 27.56 ng/ml

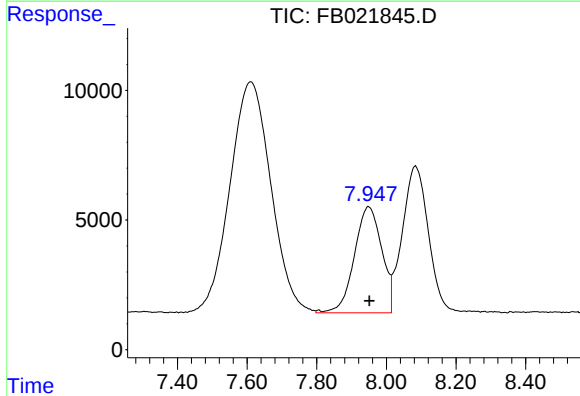


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 223505
Conc: 9.01 ng/ml

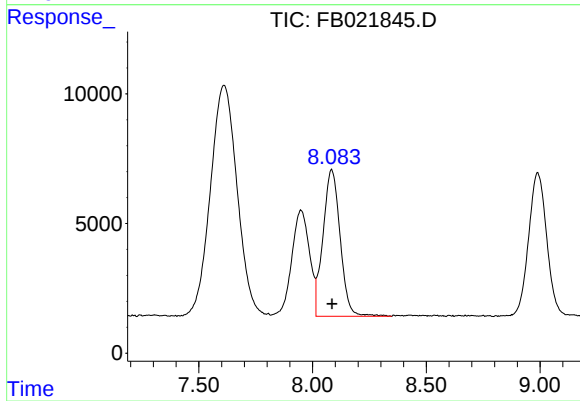


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 297229
Conc: 10.17 ng/ml

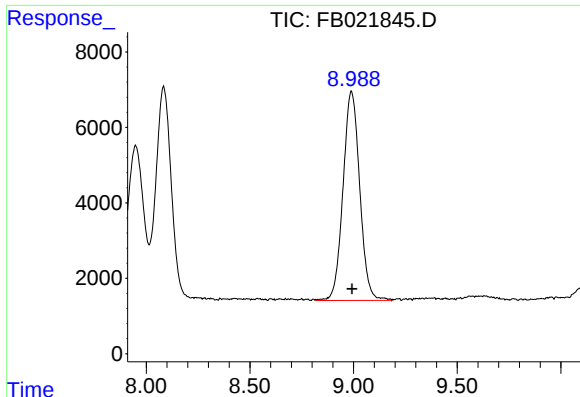


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.002 min
Response: 309996
Conc: 22.72 ng/ml

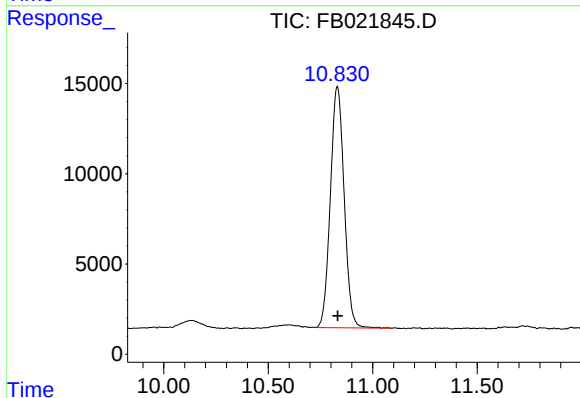


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 613007
Conc: 29.79 ng/ml

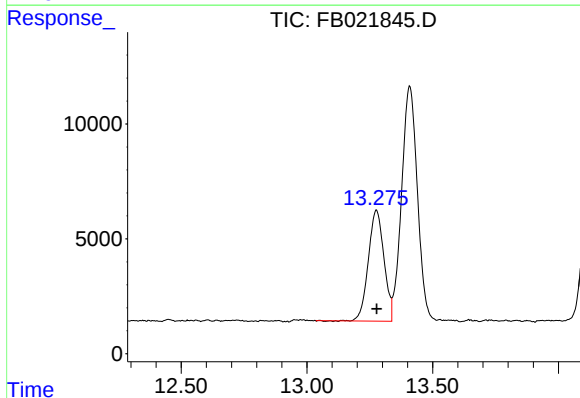


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: -0.001 min
Response: 207824
Conc: 9.99 ng/ml

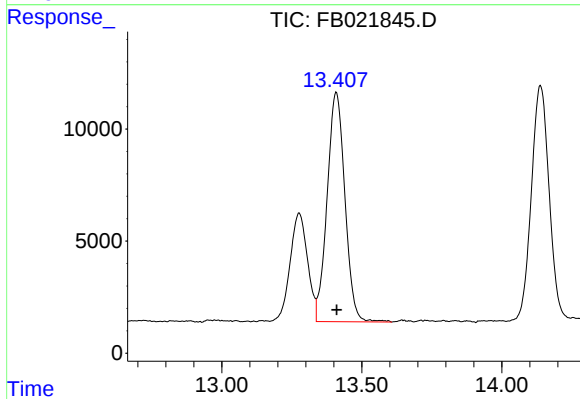

#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 451387
Conc: 20.32 ng/ml

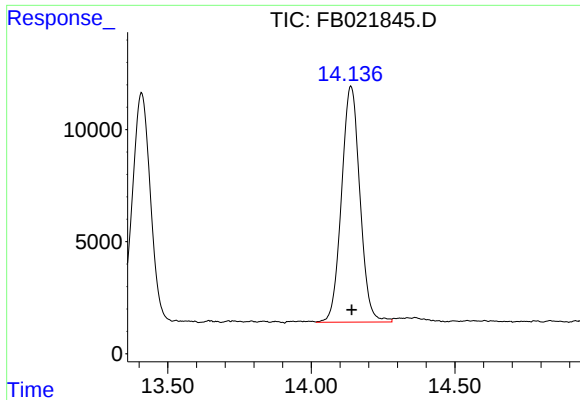


#9 O-Xylene

R.T.: 14.138 min

Delta R.T.: -0.002 min

Response: 470433

Conc: 20.45 ng/ml

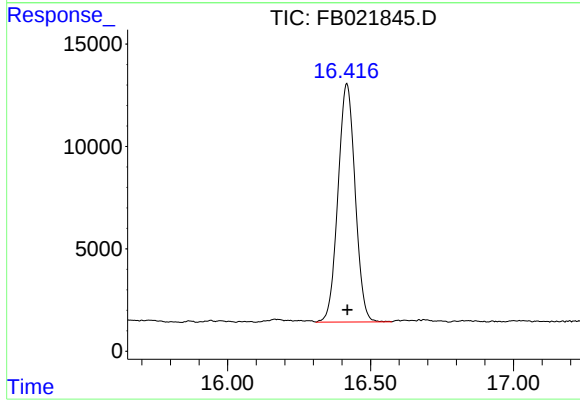

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min

Delta R.T.: -0.002 min

Response: 483714

Conc: 20.52 ng/ml