

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072919\
 Data File : FB021846.D
 Signal(s) : FID2B.CH
 Acq On : 29 Jul 2019 14:18
 Operator : DD/AJ
 Sample : K4044-01MSD
 Misc : 5.05/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 30 00:49:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.990	341476	25.023 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.864	728034	26.401 ng/ml
2) t 2,2,4-Trimethylpentane	7.613	718480	27.180 ng/ml
3) t n-Heptane	7.950	218707	8.821 ng/ml
4) t Benzene	8.084	297438	10.181 ng/ml
6) t Toluene	10.831	633316	30.779 ng/ml
7) t Ethylbenzene	13.276	211964	10.188 ng/ml
8) t m-Xylene	13.409	444073	19.990 ng/ml
9) t O-Xylene	14.138	472144	20.526 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	471156	19.984 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072919\
Data File : FB021846.D
Signal(s) : FID2B.CH
Acq On : 29 Jul 2019 14:18
Operator : DD/AJ
Sample : K4044-01MSD
Misc : 5.05/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 30 00:49:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

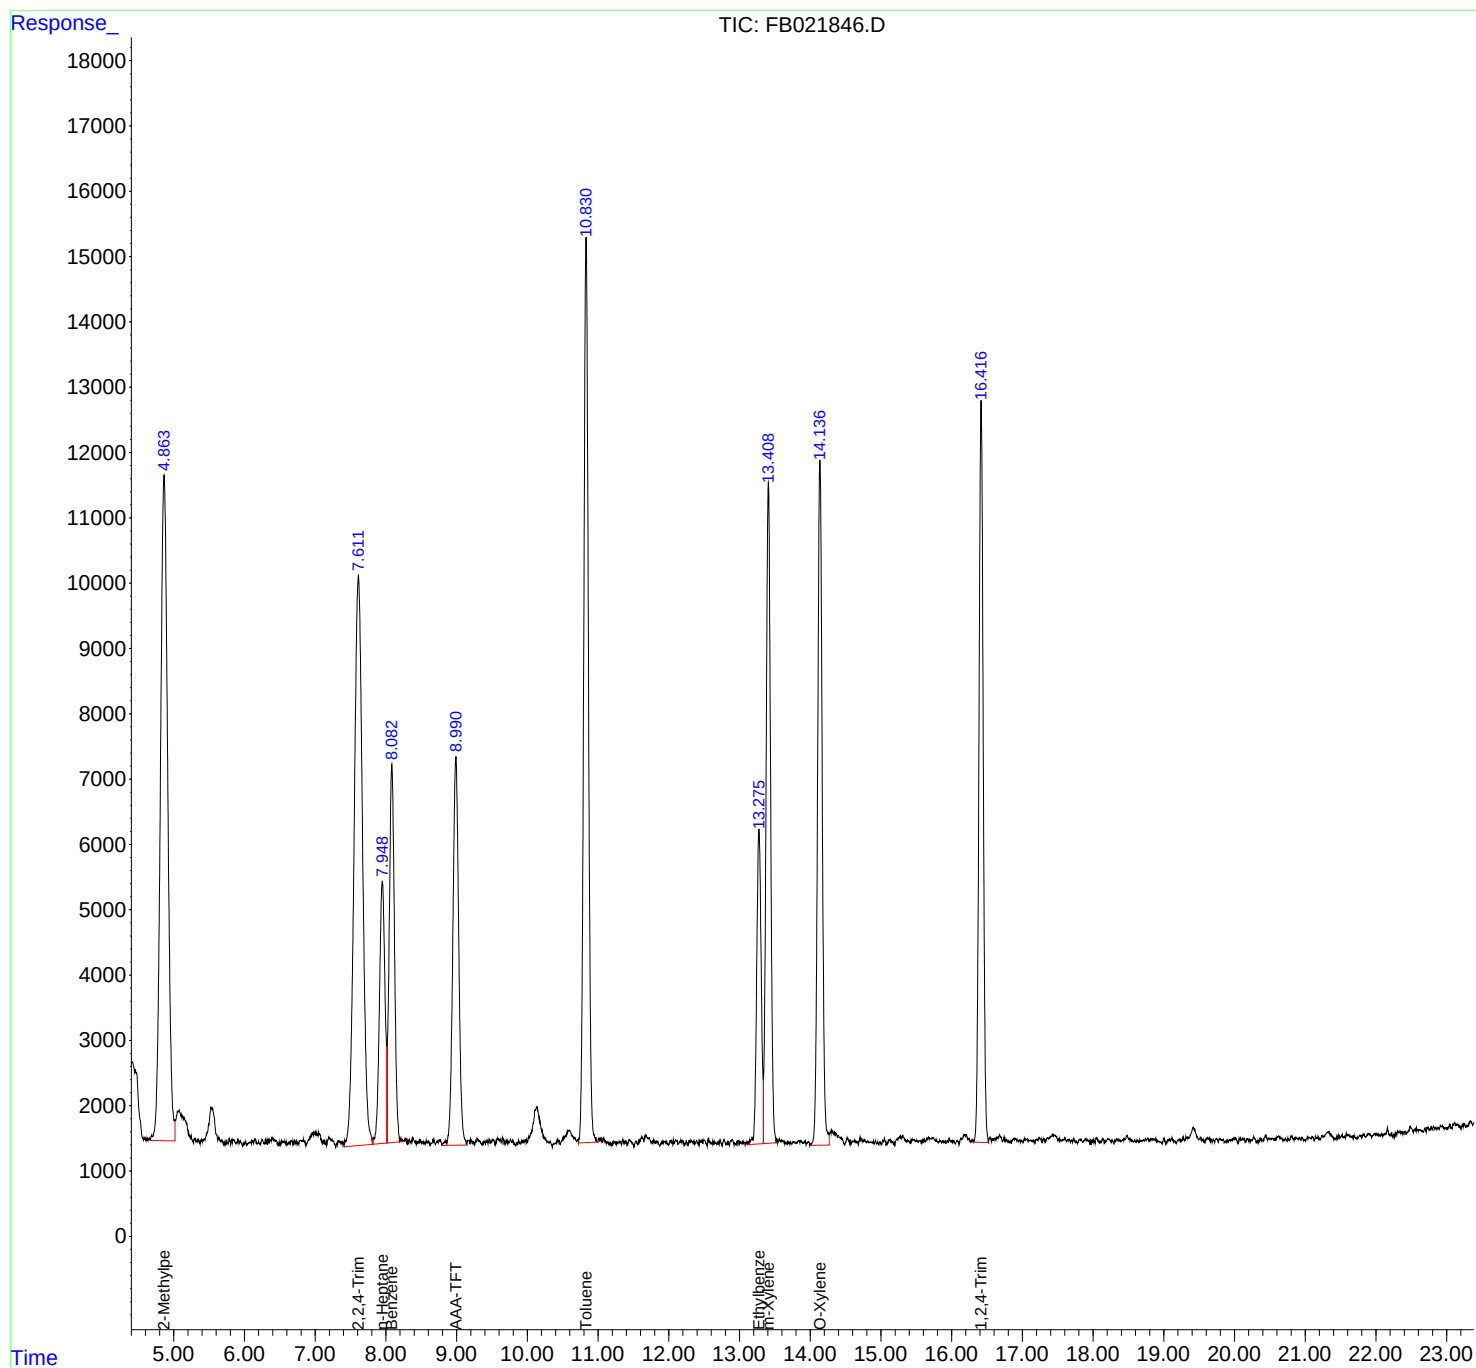

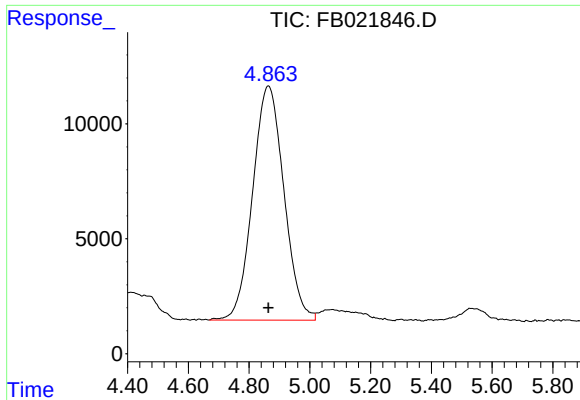


#1 2-Methylpentane

R.T.: 4.864 min
Delta R.T.: 0.001 min
Response: 728034
Conc: 26.40 ng/ml

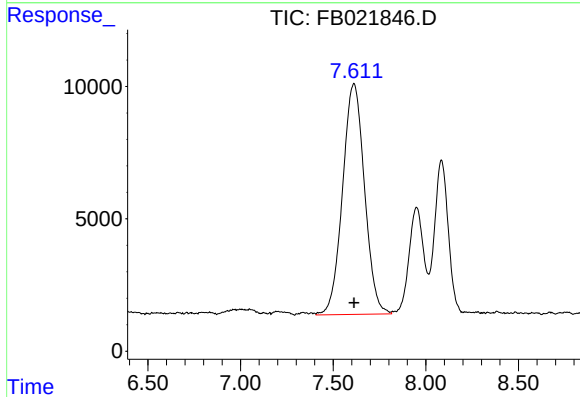


#2 2,2,4-Trimethylpentane

R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 718480
Conc: 27.18 ng/ml

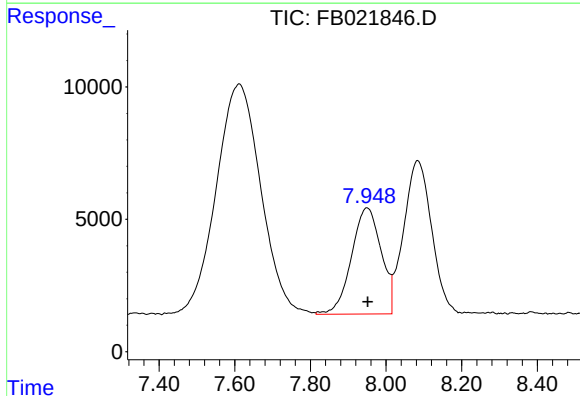


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 218707
Conc: 8.82 ng/ml

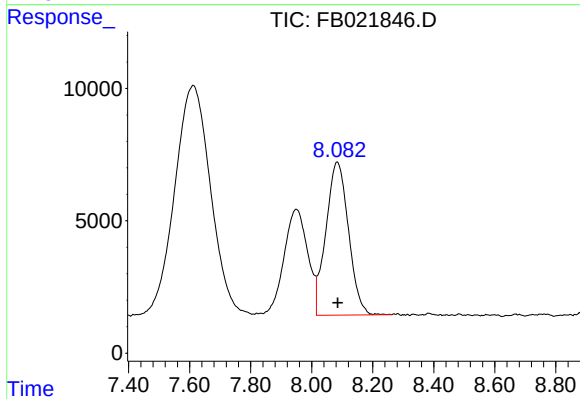


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 297438
Conc: 10.18 ng/ml

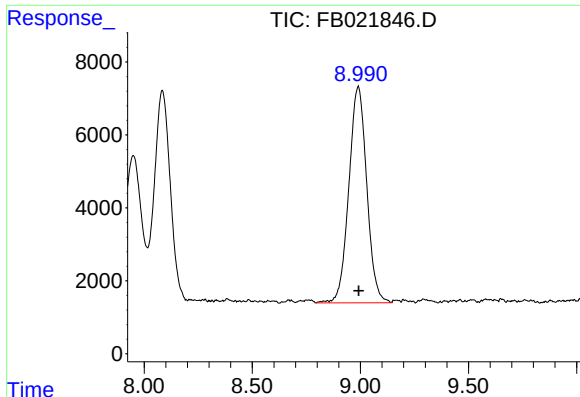


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.002 min
Response: 341476
Conc: 25.02 ng/ml

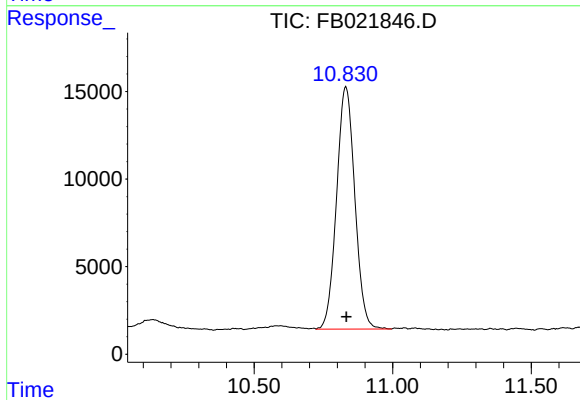


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 633316
Conc: 30.78 ng/ml

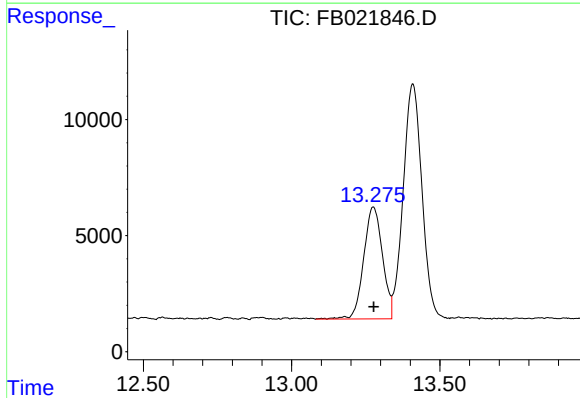


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.002 min
Response: 211964
Conc: 10.19 ng/ml

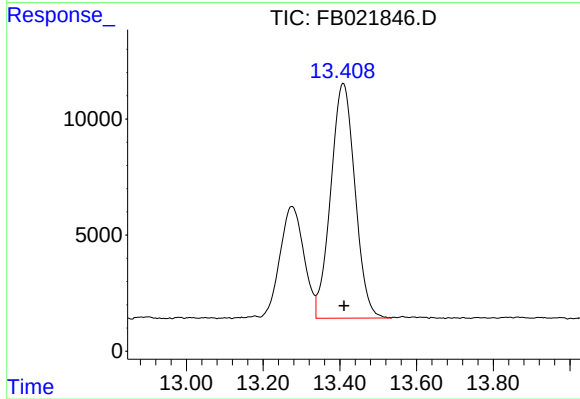


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 444073
Conc: 19.99 ng/ml

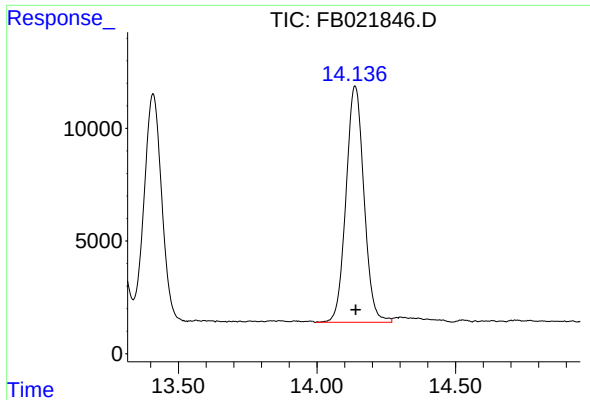

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.002 min
Response: 472144
Conc: 20.53 ng/ml

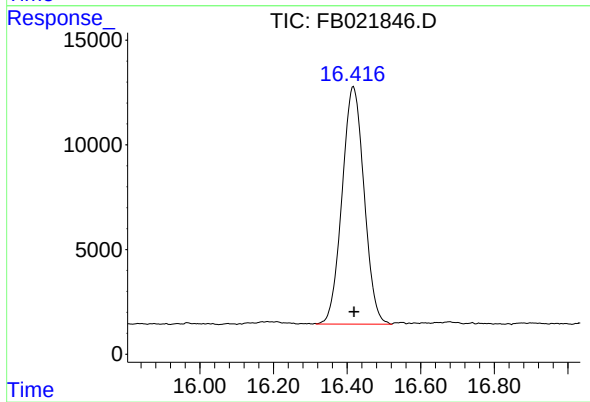

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.002 min
Response: 471156
Conc: 19.98 ng/ml