

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072922\
 Data File : FB027773.D
 Signal(s) : FID2B.CH
 Acq On : 29 Jul 2022 14:05
 Operator : AJ/MA
 Sample : BSF0729S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0729S1

Integration File: Calibration.e
 Quant Time: Jul 29 22:44:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	232573	19.983 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	616805	29.288 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	675744	32.563 ng/ml
3) t n-Heptane	7.753	223451	10.869 ng/ml
4) t Benzene	7.890	258575	11.019 ng/ml
6) t Toluene	10.624	750832	33.624 ng/ml
7) t Ethylbenzene	13.061	230469	10.999 ng/ml
8) t m-Xylene	13.194	460274	21.983 ng/ml
9) t O-Xylene	13.921	445476	21.771 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	443499	21.341 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072922\
Data File : FB027773.D
Signal(s) : FID2B.CH
Acq On : 29 Jul 2022 14:05
Operator : AJ/MA
Sample : BSF0729S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0729S1

Integration File: Calibration.e
Quant Time: Jul 29 22:44:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

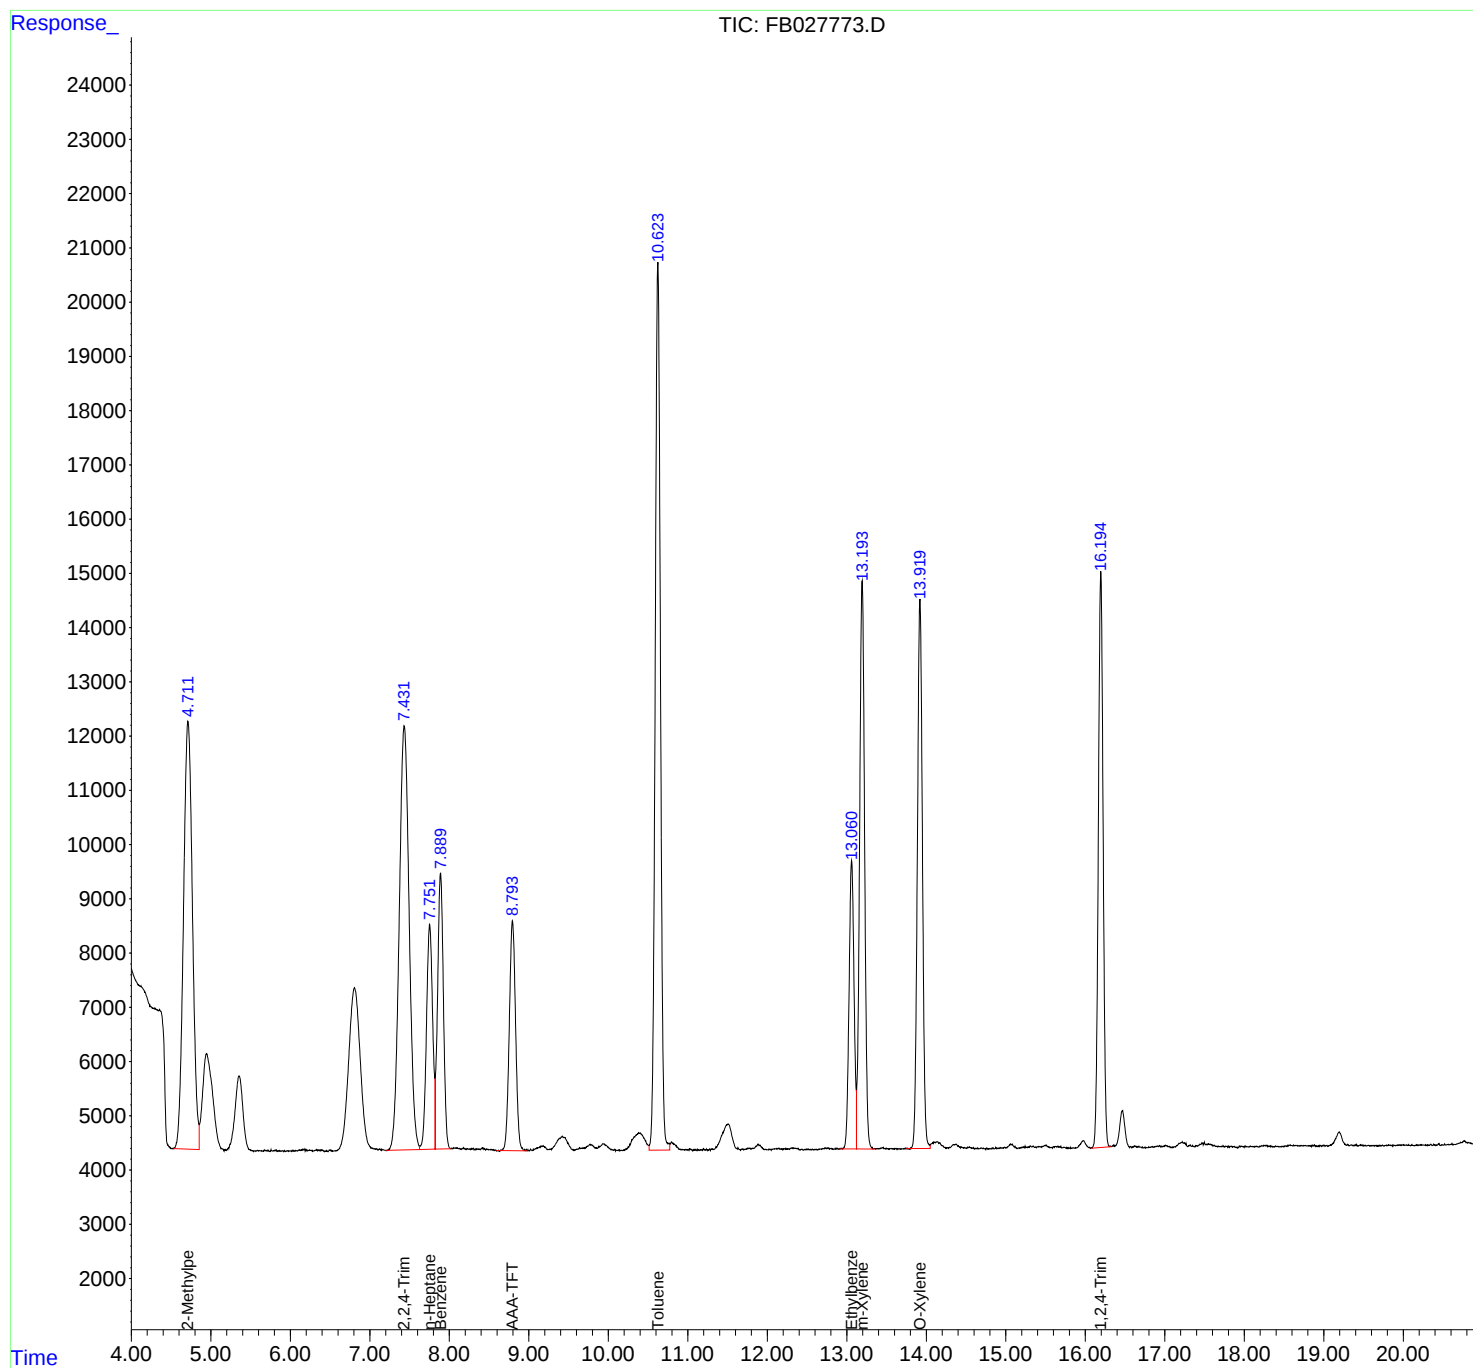


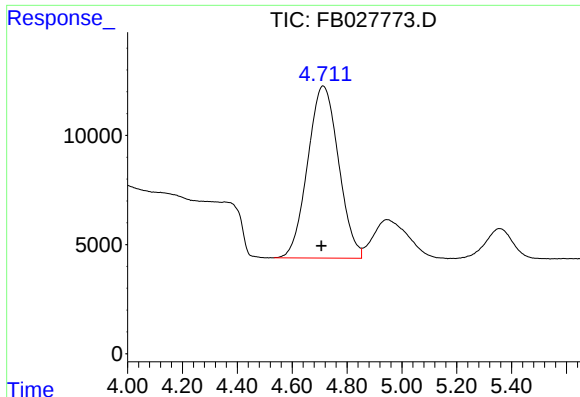

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.006 min
Response: 616805
Conc: 29.29 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0729S1

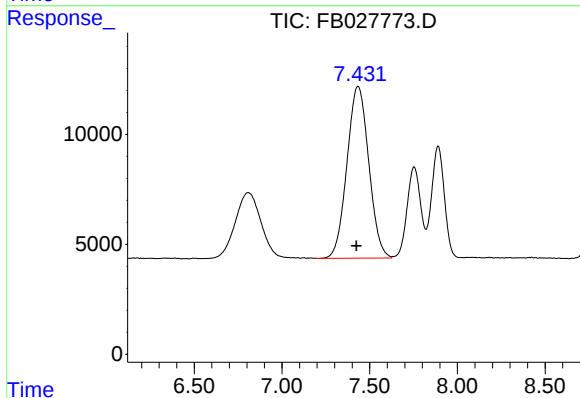


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: 0.008 min
Response: 675744
Conc: 32.56 ng/ml

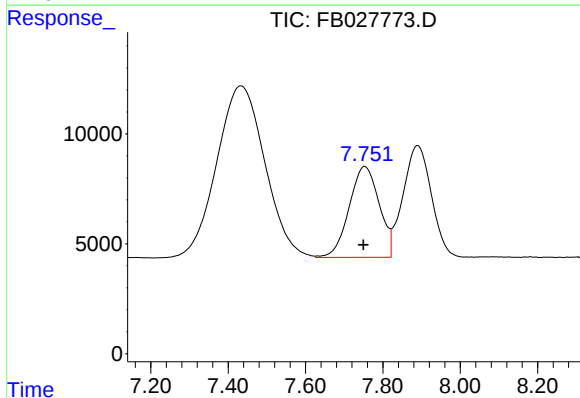


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.003 min
Response: 223451
Conc: 10.87 ng/ml

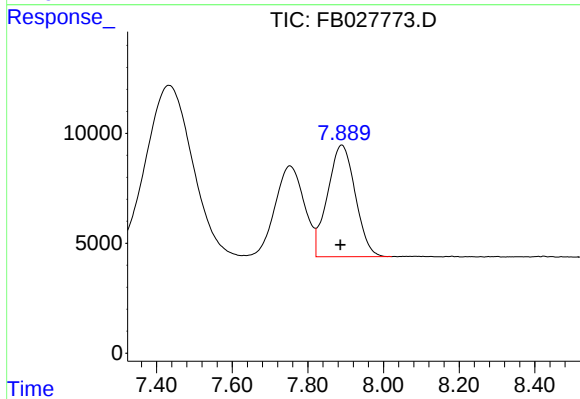

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.004 min
Response: 258575
Conc: 11.02 ng/ml

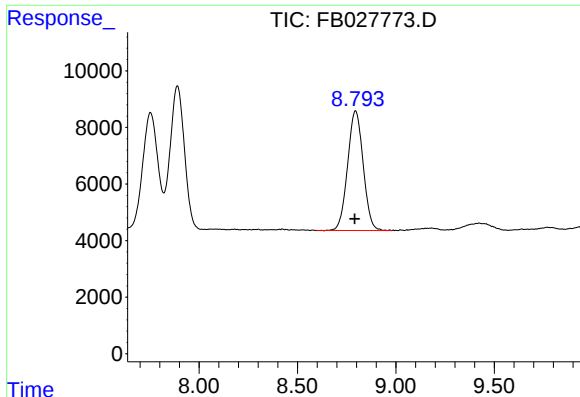

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 232573
Conc: 19.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0729S1

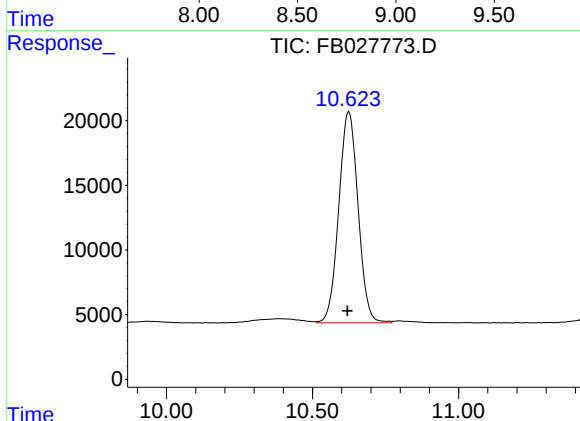


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.005 min
Response: 750832
Conc: 33.62 ng/ml

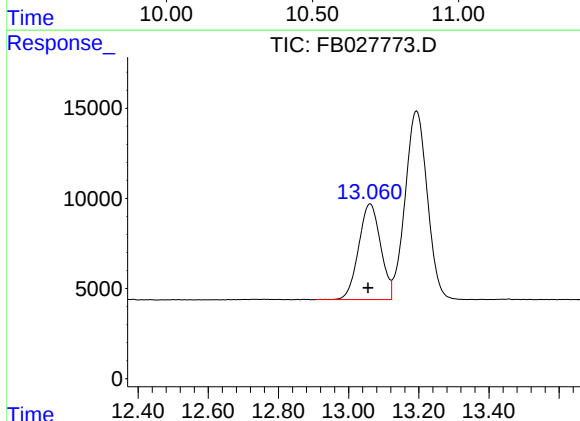


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.006 min
Response: 230469
Conc: 11.00 ng/ml

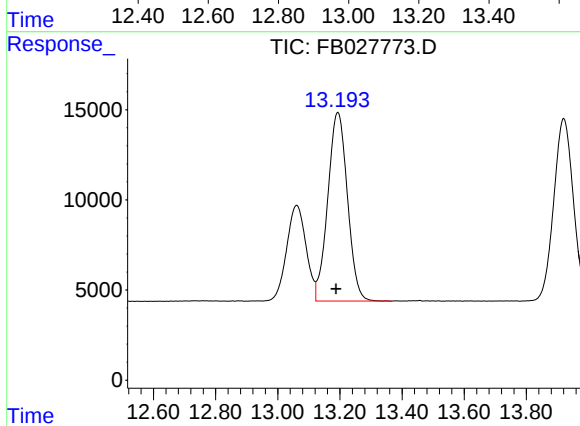

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.006 min
Response: 460274
Conc: 21.98 ng/ml

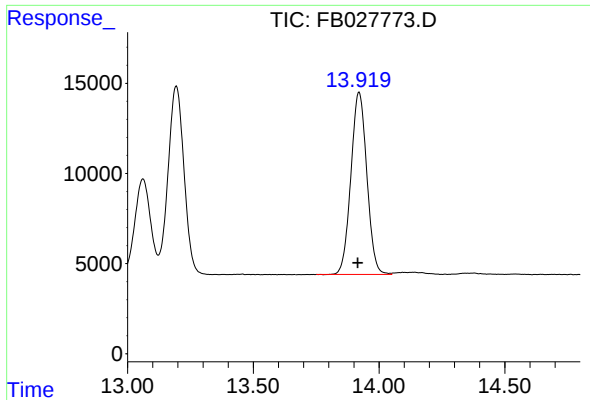

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.006 min
Response: 445476
Conc: 21.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0729S1

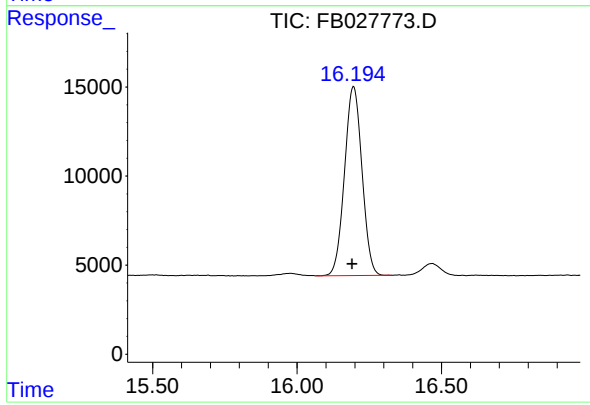

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.006 min
Response: 443499
Conc: 21.34 ng/ml