

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
 Data File : FB017001.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jul 2018 20:19
 Operator : MJ/SJ
 Sample : J4234-02 MS
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 10 09:57:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.113	158409	20.016 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.964	333184	23.082 ng/ml
2) t 2,2,4-Trimethylpentane	7.732	234812	16.786 ng/ml
3) t n-Heptane	8.067	78374	5.574 ng/ml
4) t Benzene	8.208	169558	9.652 ng/ml
6) t Toluene	10.962	415619	30.265 ng/ml
7) t Ethylbenzene	13.411	134732	9.880 ng/ml
8) t m-Xylene	13.544	285247	19.826 ng/ml
9) t O-Xylene	14.276	298858	19.596 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	320167	17.347 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
Data File : FB017001.D
Signal(s) : FID2B.CH
Acq On : 30 Jul 2018 20:19
Operator : MJ/SJ
Sample : J4234-02 MS
Misc : 5.02g/5.00mL DI Water
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 10 09:57:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

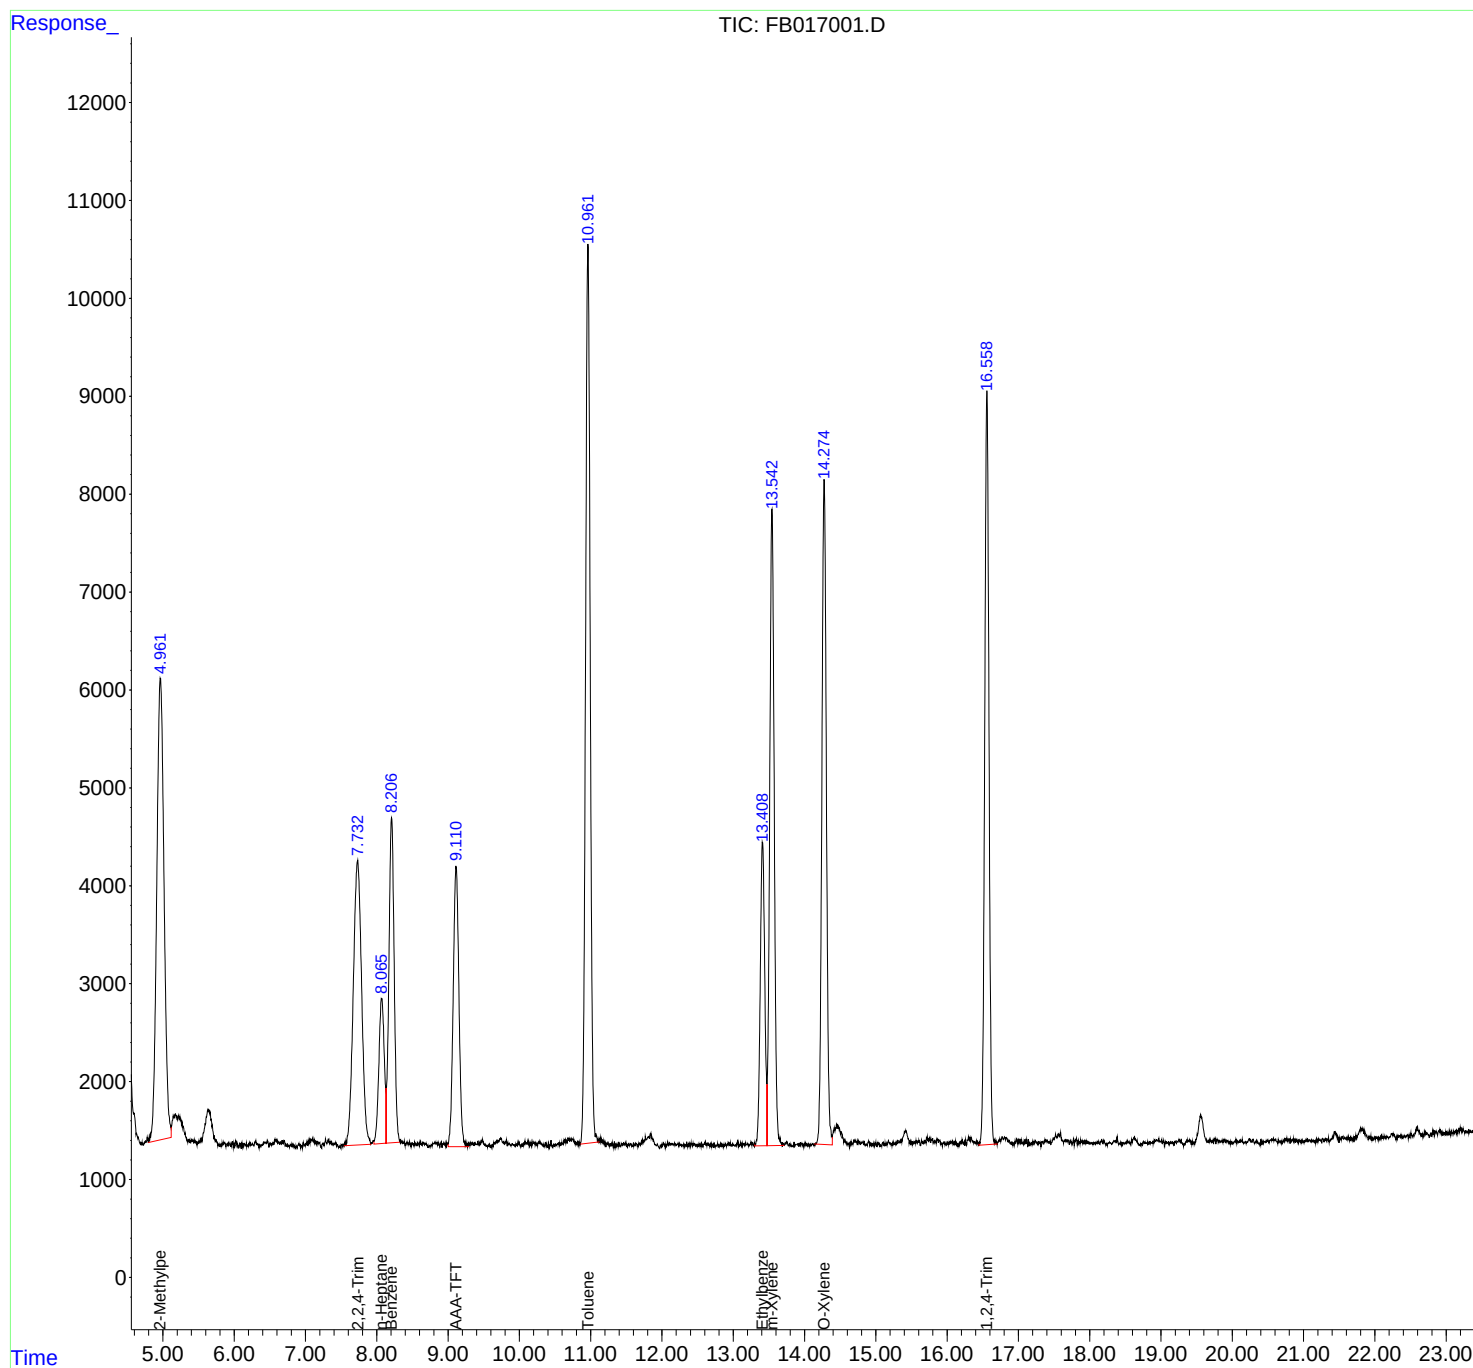


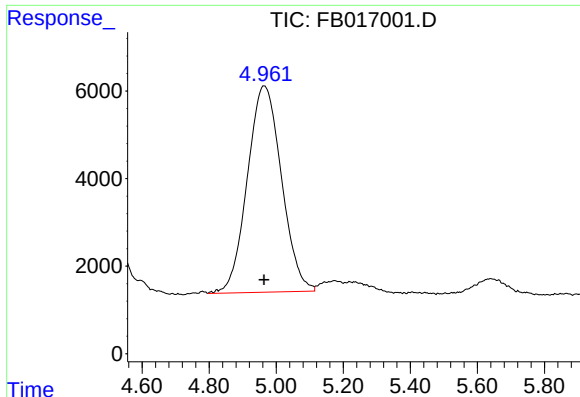

#1 2-Methylpentane


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 333184
Conc: 23.08 ng/ml

Instrument :
FID_B
ClientSampleId :

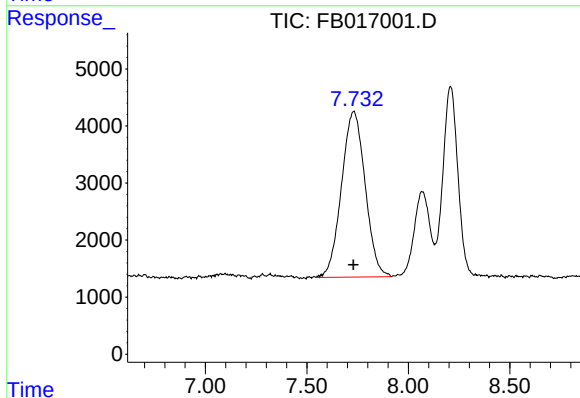


#2 2,2,4-Trimethylpentane

R.T.: 7.732 min
Delta R.T.: 0.002 min
Response: 234812
Conc: 16.79 ng/ml

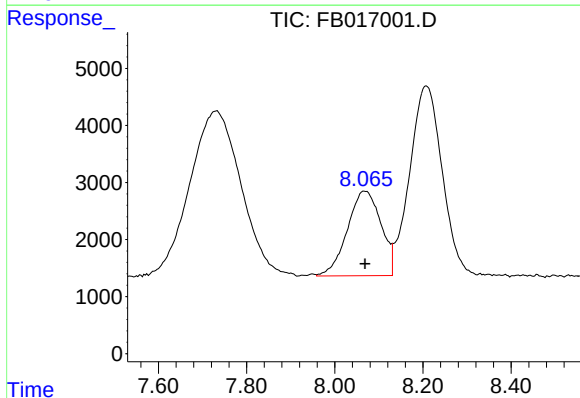


#3 n-Heptane

R.T.: 8.067 min
Delta R.T.: -0.001 min
Response: 78374
Conc: 5.57 ng/ml

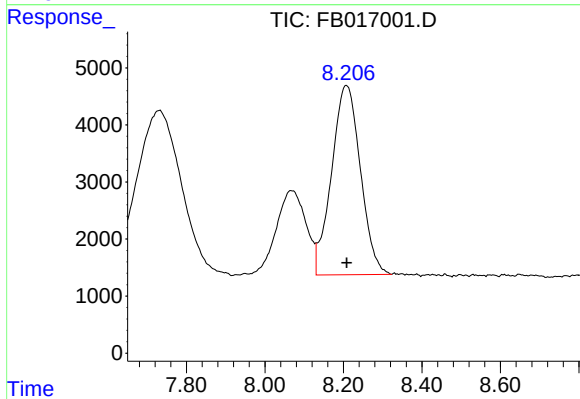

#4 Benzene


R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 169558
Conc: 9.65 ng/ml

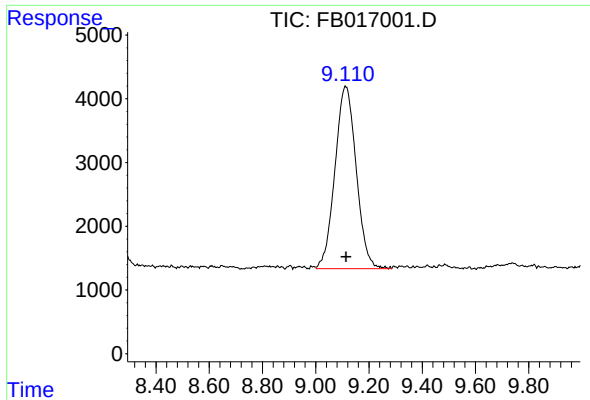

#5 AAA-TFT


R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 158409
Conc: 20.02 ng/ml

Instrument :
FID_B
ClientSampleId :

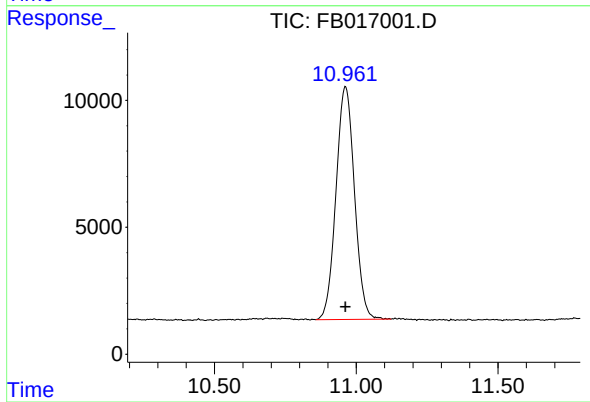


#6 Toluene

R.T.: 10.962 min
Delta R.T.: 0.000 min
Response: 415619
Conc: 30.26 ng/ml

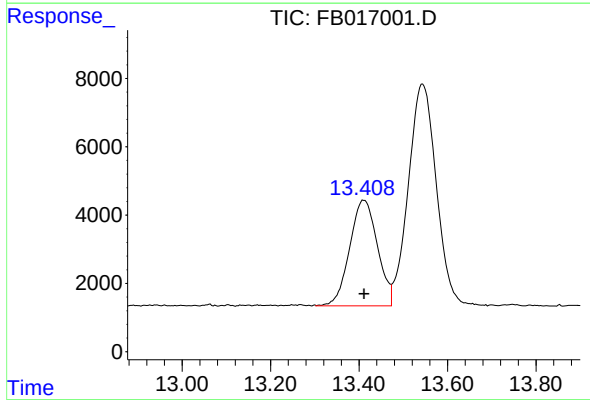


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 134732
Conc: 9.88 ng/ml

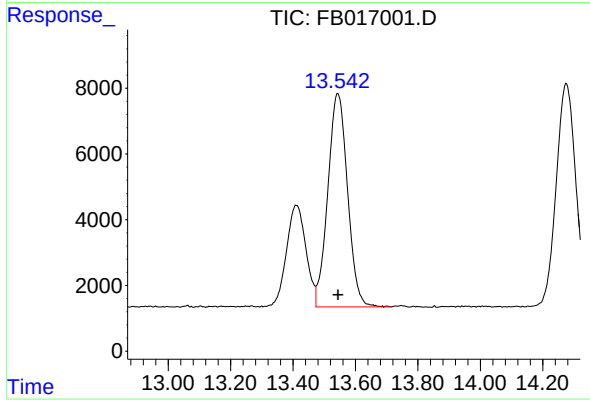

#8 m-Xylene


R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 285247
Conc: 19.83 ng/ml

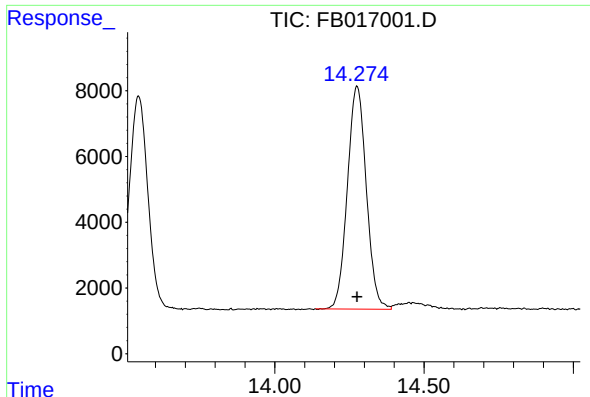

#9 O-Xylene

R.T.: 14.276 min
Delta R.T.: 0.000 min
Response: 298858
Conc: 19.60 ng/ml

Instrument :
FID_B
ClientSampleId :

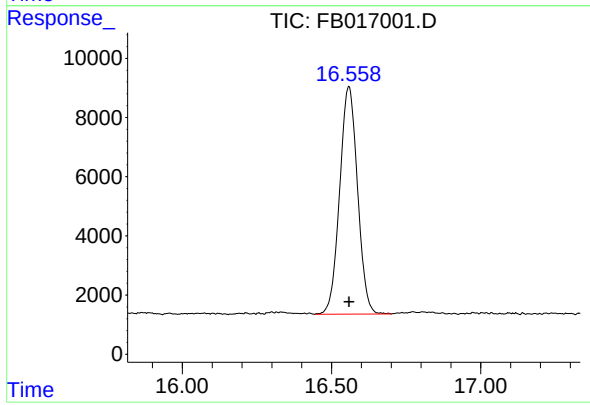

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.000 min
Response: 320167
Conc: 17.35 ng/ml