

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
 Data File : FB017002.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jul 2018 20:50
 Operator : MJ/SJ
 Sample : J4234-02 MSD
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 10 09:57:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.111	153067	19.341 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.964	329303	22.813 ng/ml
2) t 2,2,4-Trimethylpentane	7.729	232268	16.604 ng/ml
3) t n-Heptane	8.069	79922	5.684 ng/ml
4) t Benzene	8.207	169923	9.673 ng/ml
6) t Toluene	10.961	404041	29.422 ng/ml
7) t Ethylbenzene	13.411	131080	9.613 ng/ml
8) t m-Xylene	13.544	267822	18.615 ng/ml
9) t O-Xylene	14.275	285675	18.732 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	304414	16.493 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
Data File : FB017002.D
Signal(s) : FID2B.CH
Acq On : 30 Jul 2018 20:50
Operator : MJ/SJ
Sample : J4234-02 MSD
Misc : 5.01g/5.00mL DI Water
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 10 09:57:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

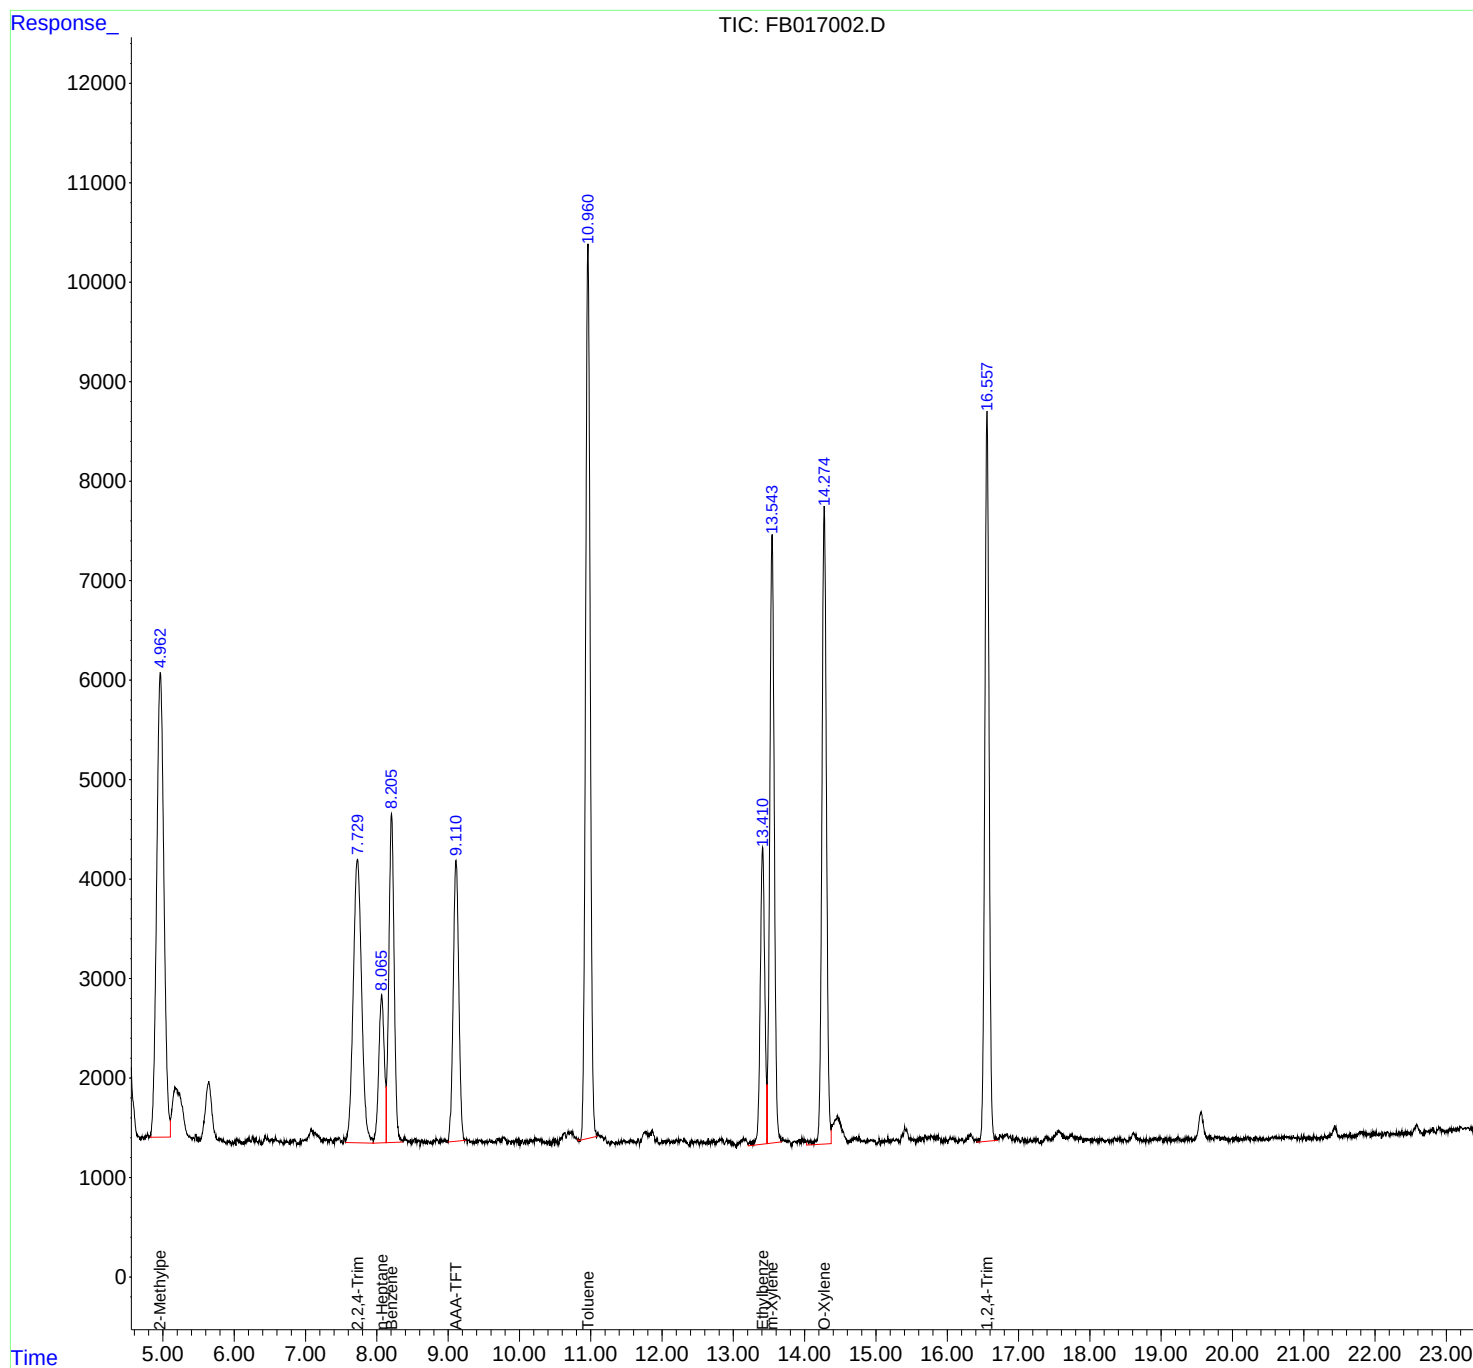


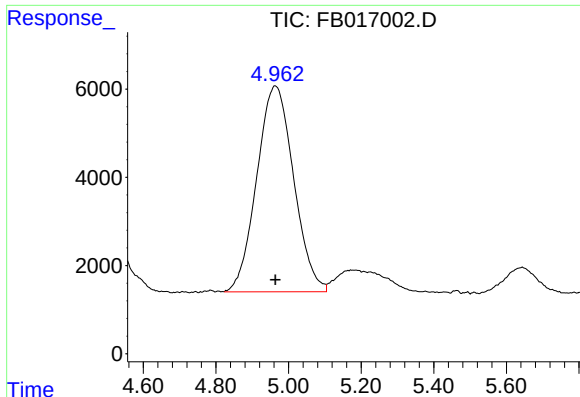

#1 2-Methylpentane


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 329303
Conc: 22.81 ng/ml

Instrument :
FID_B
ClientSampleId :

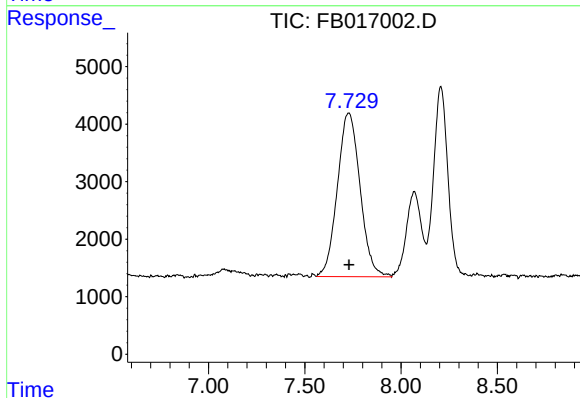


#2 2,2,4-Trimethylpentane

R.T.: 7.729 min
Delta R.T.: -0.001 min
Response: 232268
Conc: 16.60 ng/ml

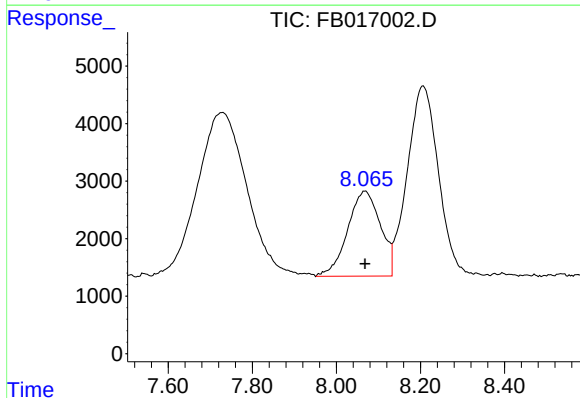


#3 n-Heptane

R.T.: 8.069 min
Delta R.T.: 0.000 min
Response: 79922
Conc: 5.68 ng/ml

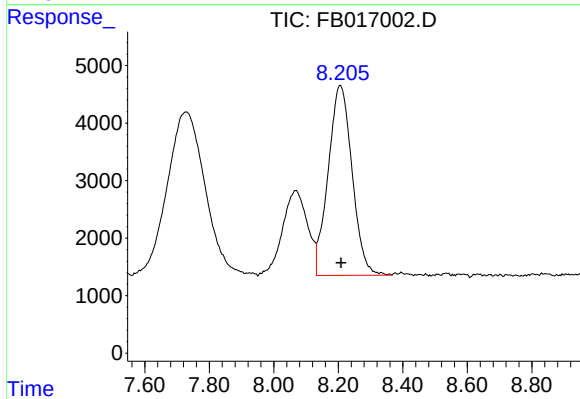

#4 Benzene


R.T.: 8.207 min
Delta R.T.: -0.002 min
Response: 169923
Conc: 9.67 ng/ml

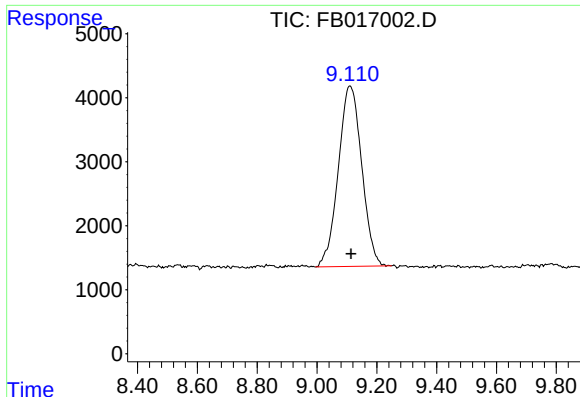

#5 AAA-TFT


R.T.: 9.111 min
Delta R.T.: -0.003 min
Response: 153067
Conc: 19.34 ng/ml

Instrument :
FID_B
ClientSampleId :

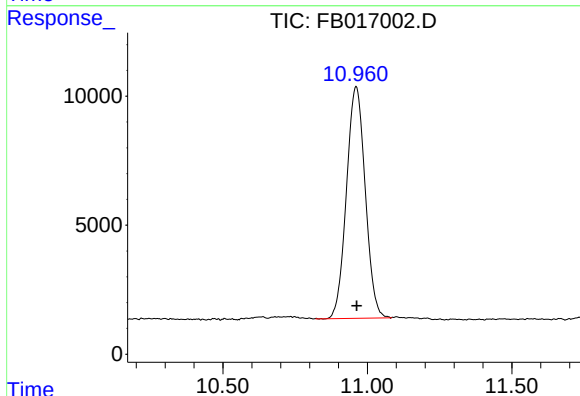


#6 Toluene

R.T.: 10.961 min
Delta R.T.: -0.001 min
Response: 404041
Conc: 29.42 ng/ml

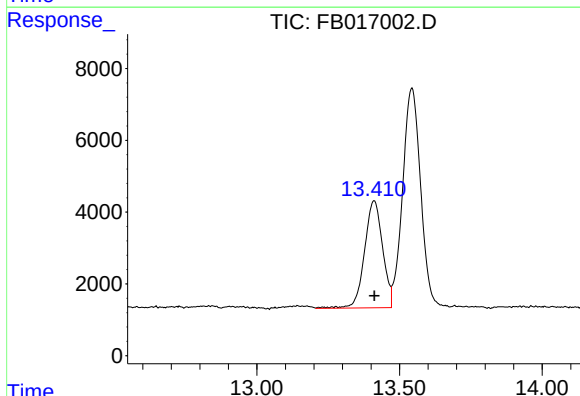


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 131080
Conc: 9.61 ng/ml

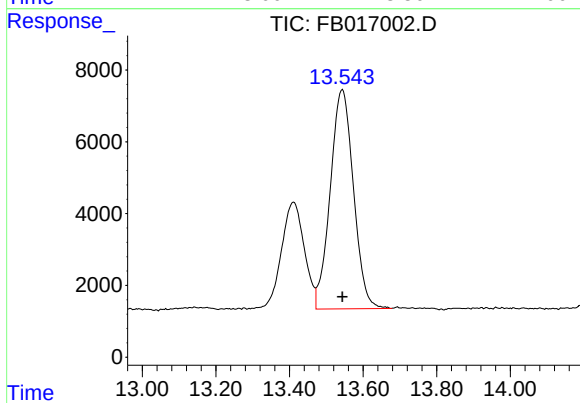

#8 m-Xylene


R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 267822
Conc: 18.62 ng/ml

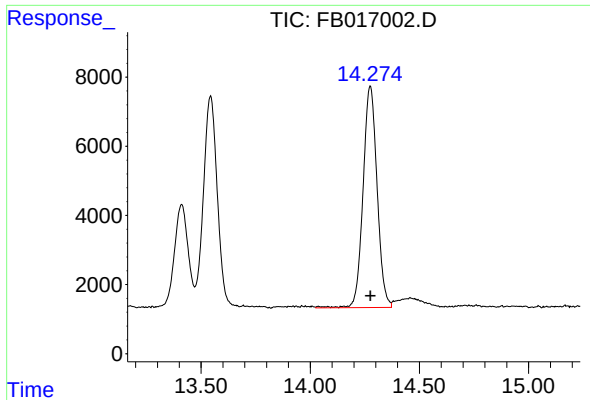

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: 0.000 min
Response: 285675
Conc: 18.73 ng/ml

Instrument :
FID_B
ClientSampleId :

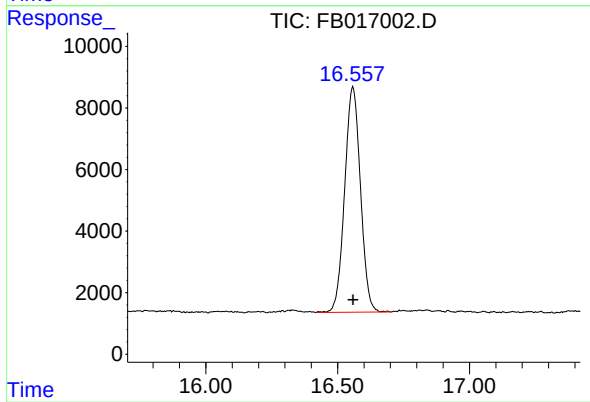

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.000 min
Response: 304414
Conc: 16.49 ng/ml