

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
 Data File : FB017005.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jul 2018 22:51
 Operator : MJ/SJ
 Sample : J4231-21
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 10 09:58:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.113	149069	18.836 ng/ml
Target Compounds			
4) t Benzene	8.225	5089	0.290 ng/ml
6) t Toluene	10.952	6278	0.457 ng/ml
7) t Ethylbenzene	13.411	34045	2.497 ng/ml
8) t m-Xylene	13.538	16223	1.128 ng/ml
9) t O-Xylene	14.278	12974	0.851 ng/ml
10) t 1,2,4-Trimethylbenzene	16.560	39545	2.143 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
Data File : FB017005.D
Signal(s) : FID2B.CH
Acq On : 30 Jul 2018 22:51
Operator : MJ/SJ
Sample : J4231-21
Misc : 5.00g/5.00mL DI Water
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 10 09:58:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

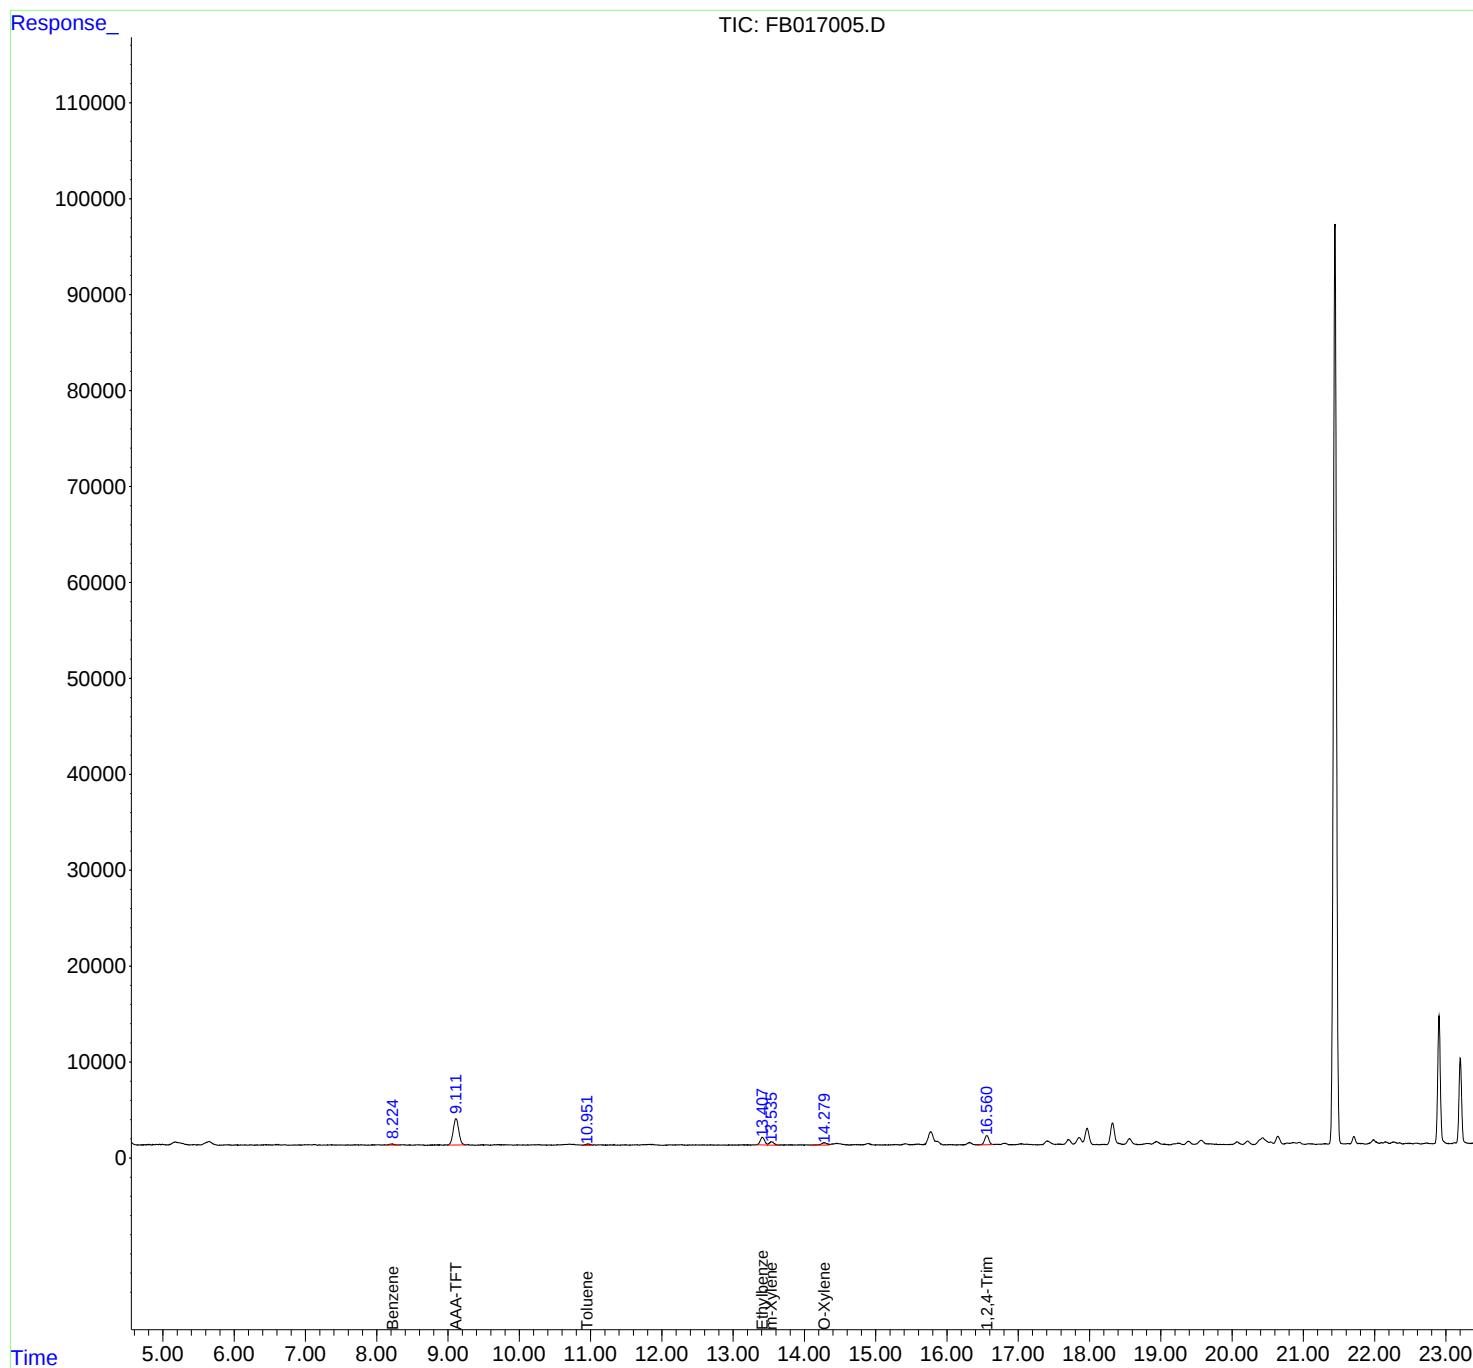


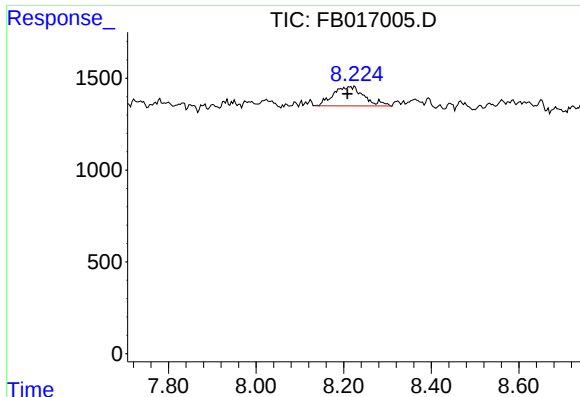

#4 Benzene


R.T.: 8.225 min
Delta R.T.: 0.016 min
Response: 5089
Conc: 0.29 ng/ml

Instrument :
FID_B
ClientSampleId :

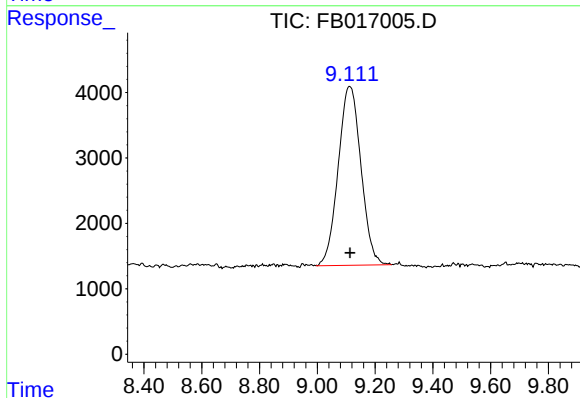


#5 AAA-TFT

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 149069
Conc: 18.84 ng/ml

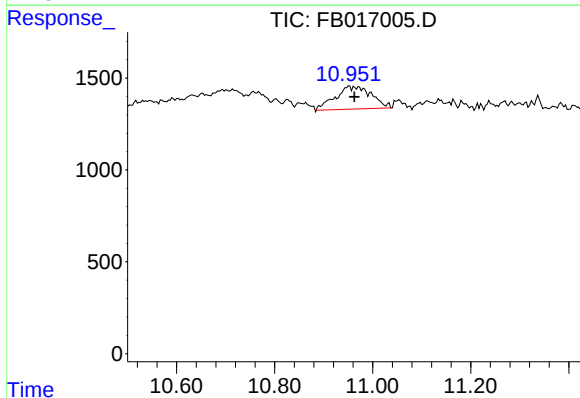


#6 Toluene

R.T.: 10.952 min
Delta R.T.: -0.011 min
Response: 6278
Conc: 0.46 ng/ml

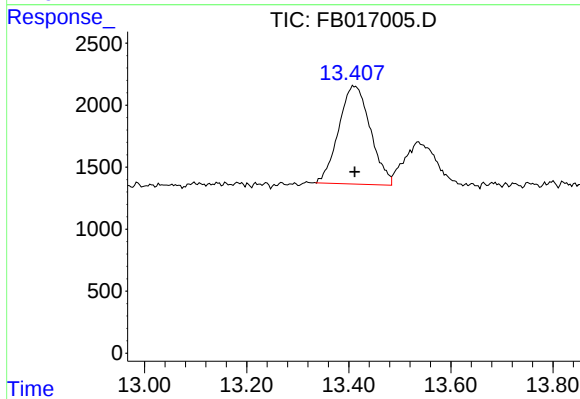

#7 Ethylbenzene


R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 34045
Conc: 2.50 ng/ml

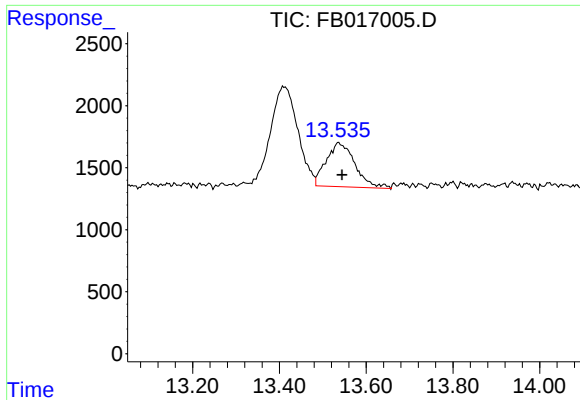

#8 m-Xylene


R.T.: 13.538 min
Delta R.T.: -0.007 min
Response: 16223
Conc: 1.13 ng/ml

Instrument :
FID_B
ClientSampleId :

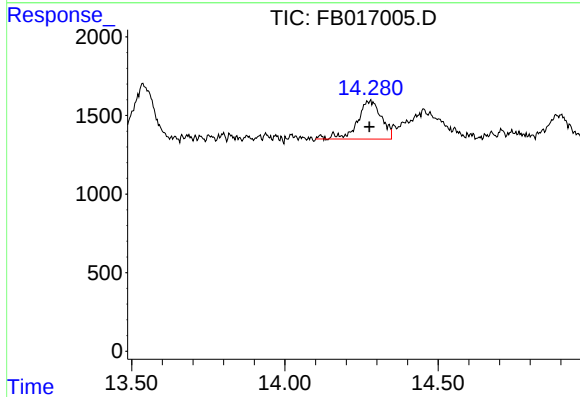

#9 O-Xylene

R.T.: 14.278 min
Delta R.T.: 0.002 min
Response: 12974
Conc: 0.85 ng/ml

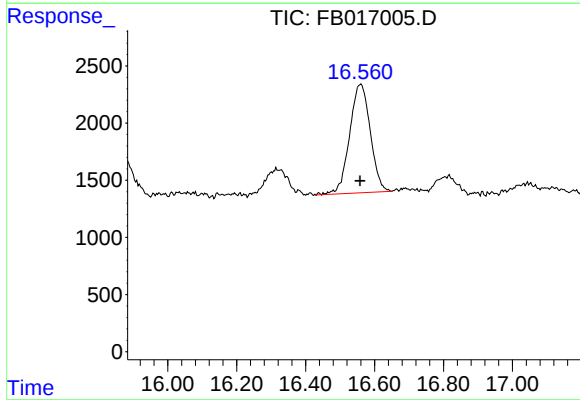

#10 1,2,4-Trimethylbenzene

R.T.: 16.560 min
Delta R.T.: 0.001 min
Response: 39545
Conc: 2.14 ng/ml