

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
 Data File : FB017009.D
 Signal(s) : FID2B.CH
 Acq On : 31 Jul 2018 1:53
 Operator : MJ/SJ
 Sample : J4231-05
 Misc : 5.00g/5.00ml DI water
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 31 07:50:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	146377	18.398 ng/ml
Target Compounds			
4) t Benzene	8.212	3310	0.189 ng/ml
6) t Toluene	10.960	27783	2.048 ng/ml
7) t Ethylbenzene	13.411	480970	35.048 ng/ml
8) t m-Xylene	13.541	152828	10.535 ng/ml
9) t O-Xylene	14.276	84113	5.467 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	193472	10.373 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
Data File : FB017009.D
Signal(s) : FID2B.CH
Acq On : 31 Jul 2018 1:53
Operator : MJ/SJ
Sample : J4231-05
Misc : 5.00g/5.00ml DI water
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 31 07:50:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

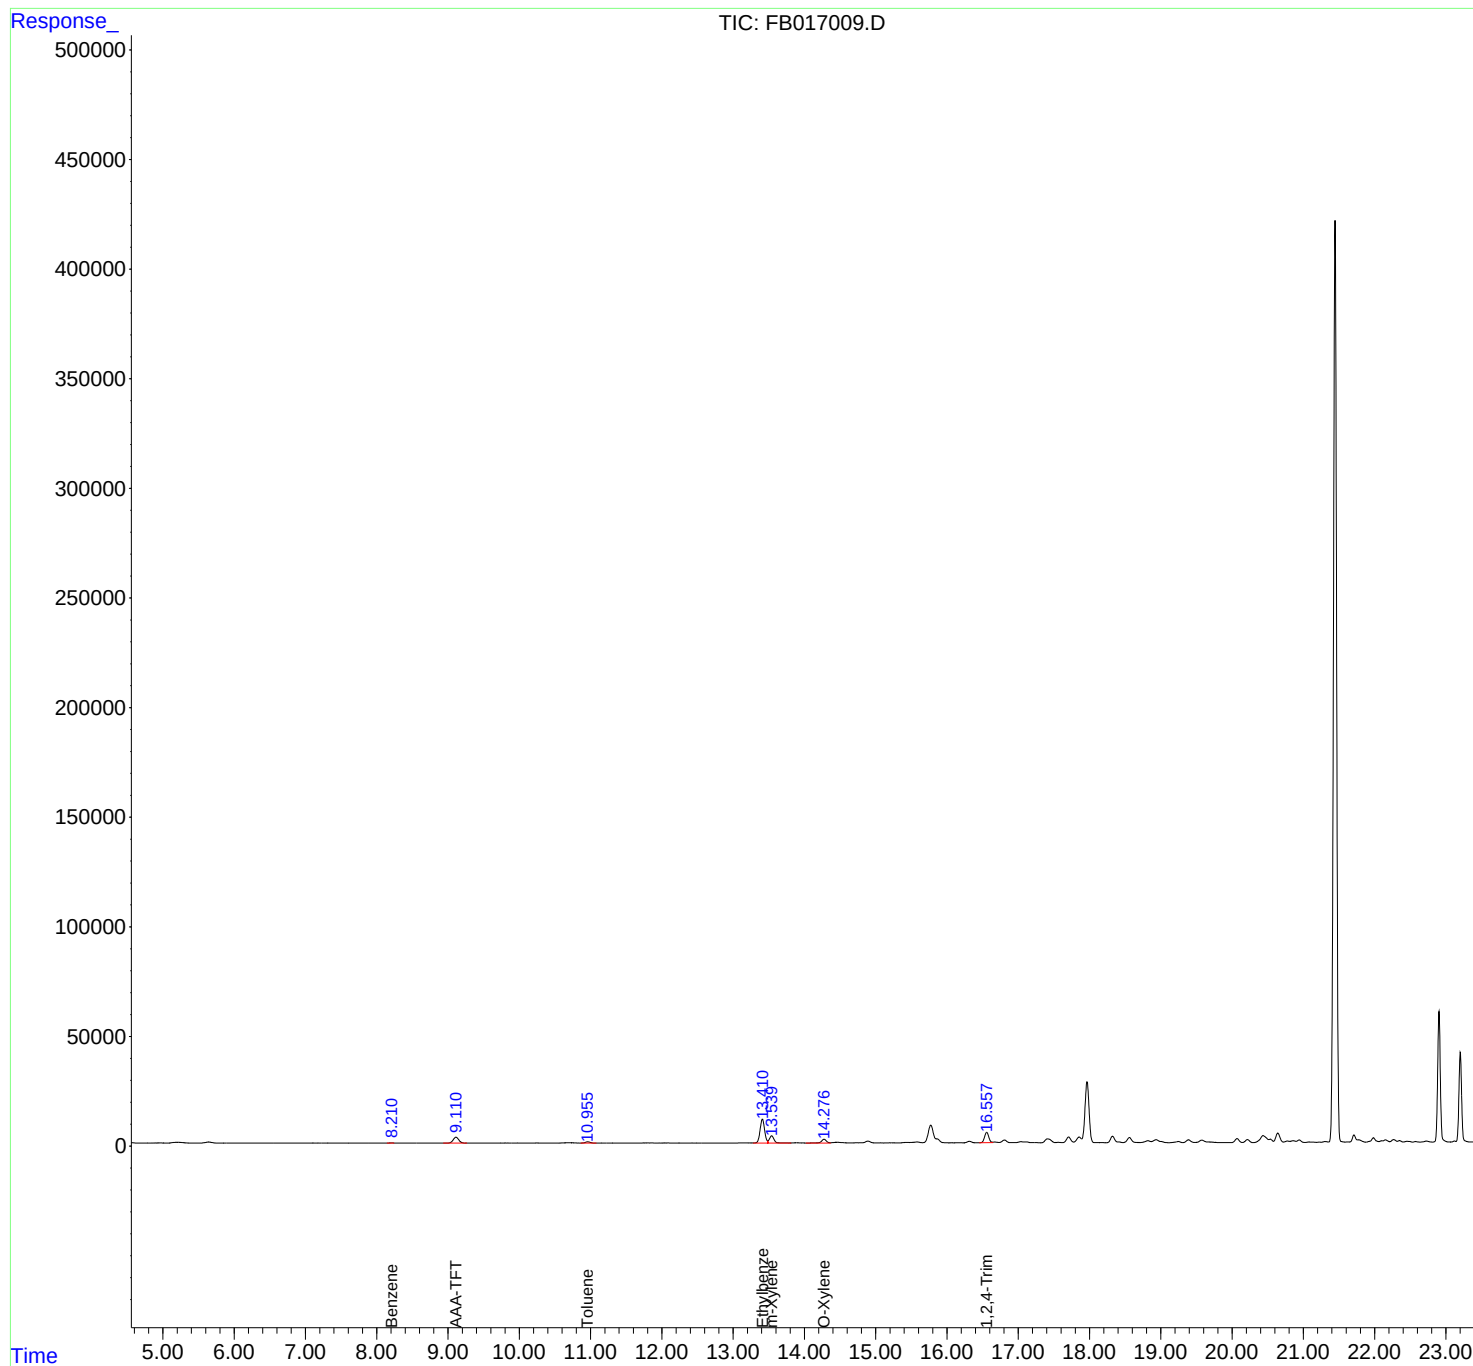


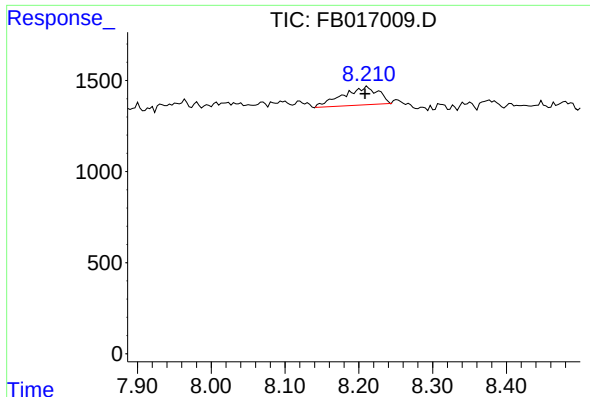

#4 Benzene


R.T.: 8.212 min
Delta R.T.: 0.003 min
Response: 3310
Conc: 0.19 ng/ml

Instrument :
FID_B
ClientSampleId :

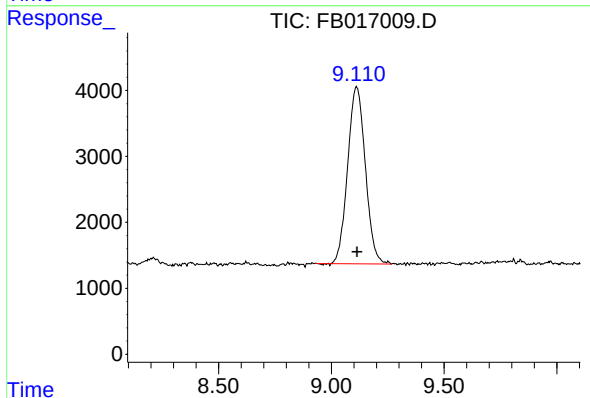


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: -0.002 min
Response: 146377
Conc: 18.40 ng/ml

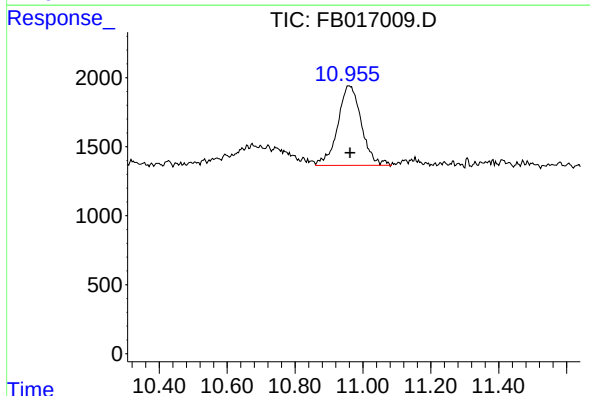


#6 Toluene

R.T.: 10.960 min
Delta R.T.: -0.002 min
Response: 27783
Conc: 2.05 ng/ml

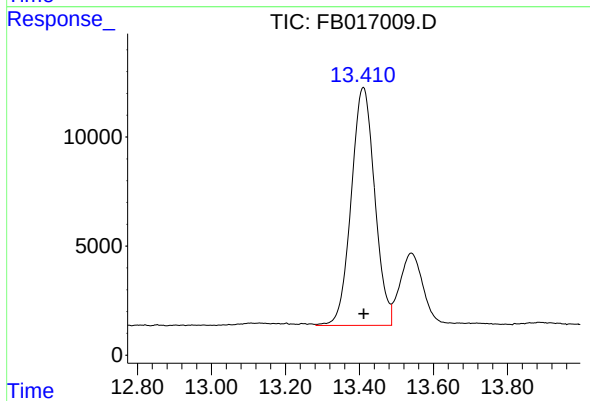

#7 Ethylbenzene


R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 480970
Conc: 35.05 ng/ml

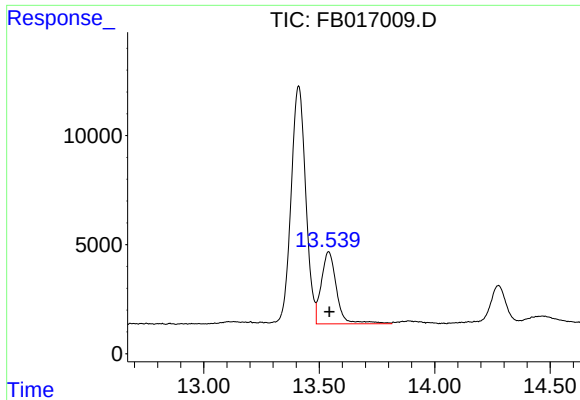

#8 m-Xylene


R.T.: 13.541 min
Delta R.T.: -0.003 min
Response: 152828
Conc: 10.53 ng/ml

Instrument :
FID_B
ClientSampleId :

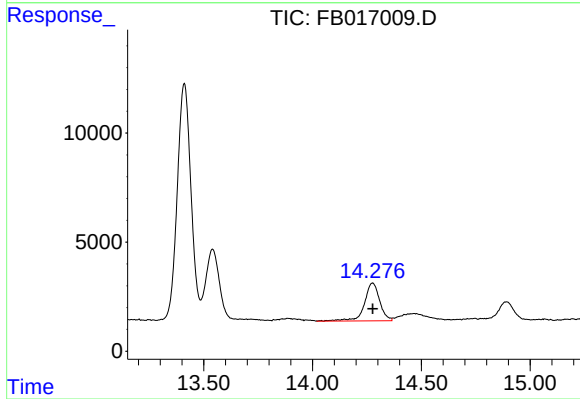

#9 O-Xylene

R.T.: 14.276 min
Delta R.T.: 0.000 min
Response: 84113
Conc: 5.47 ng/ml

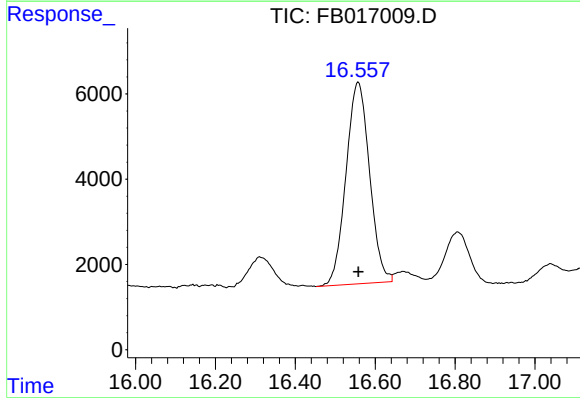

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.000 min
Response: 193472
Conc: 10.37 ng/ml