

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
 Data File : FB017011.D
 Signal(s) : FID2B.CH
 Acq On : 31 Jul 2018 3:55
 Operator : MJ/SJ
 Sample : J4231-09
 Misc : 4.99g/5.00mL DI Water
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 10 09:58:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	118153	14.929 ng/ml
Target Compounds			
4) t Benzene	8.194	436	0.025 ng/ml
6) t Toluene	10.976	6328	0.461 ng/ml
7) t Ethylbenzene	13.411	51133	3.750 ng/ml
8) t m-Xylene	13.543	21205	1.474 ng/ml
9) t O-Xylene	14.285	14870	0.975 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	133724	7.245 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
Data File : FB017011.D
Signal(s) : FID2B.CH
Acq On : 31 Jul 2018 3:55
Operator : MJ/SJ
Sample : J4231-09
Misc : 4.99g/5.00mL DI Water
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 10 09:58:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

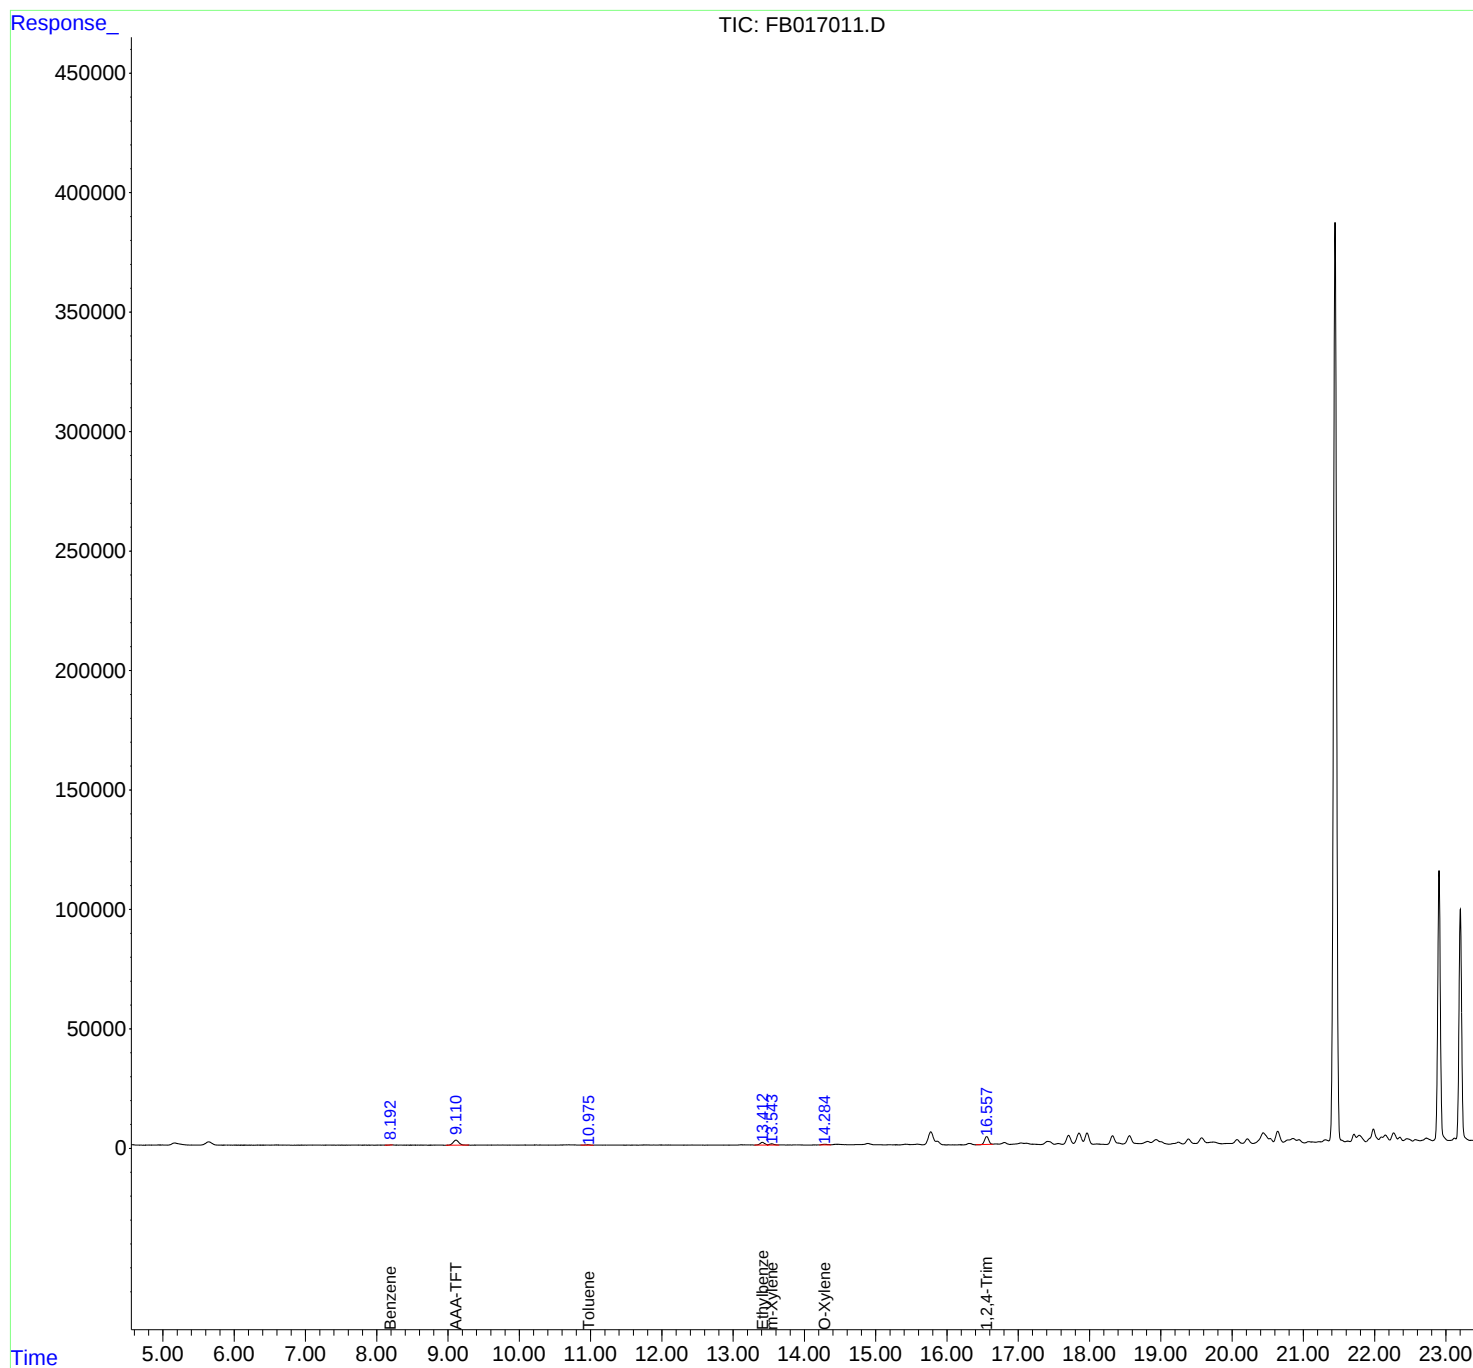


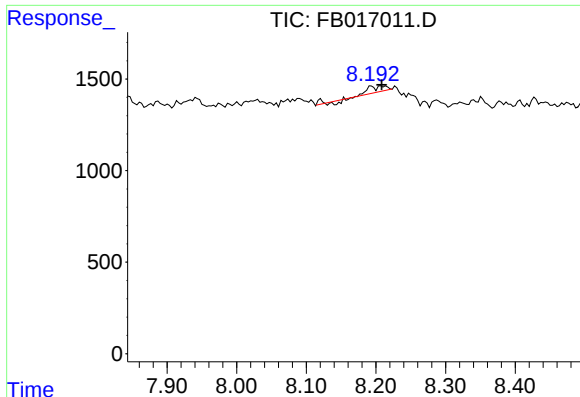

#4 Benzene


R.T.: 8.194 min
Delta R.T.: -0.014 min
Response: 436
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :

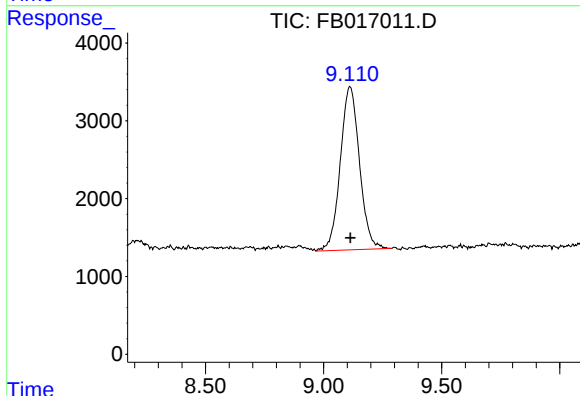


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: -0.002 min
Response: 118153
Conc: 14.93 ng/ml

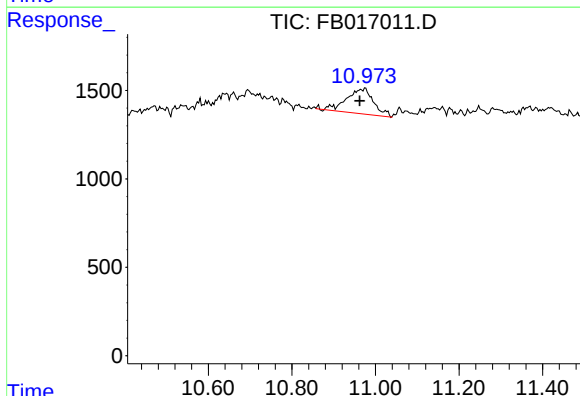


#6 Toluene

R.T.: 10.976 min
Delta R.T.: 0.013 min
Response: 6328
Conc: 0.46 ng/ml

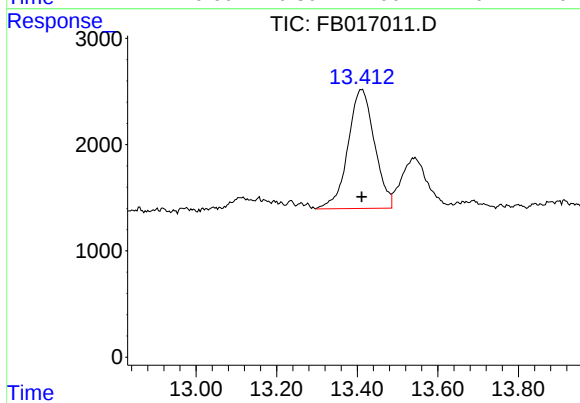

#7 Ethylbenzene


R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 51133
Conc: 3.75 ng/ml

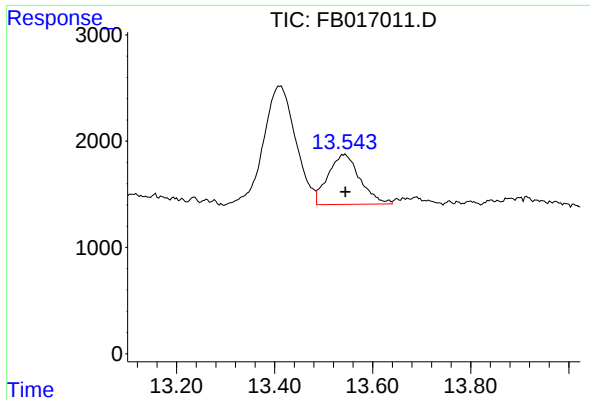

#8 m-Xylene


R.T.: 13.543 min
Delta R.T.: -0.001 min
Response: 21205
Conc: 1.47 ng/ml

Instrument :
FID_B
ClientSampleId :

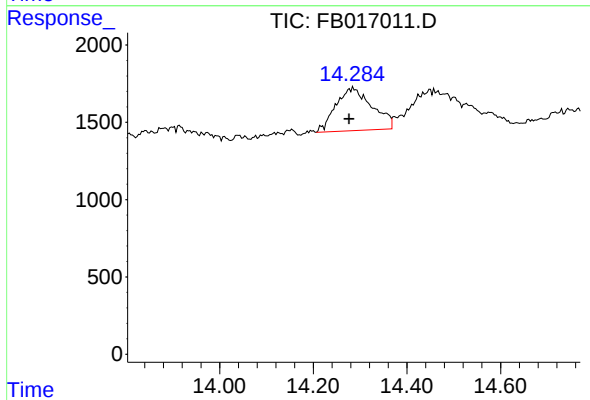

#9 O-Xylene

R.T.: 14.285 min
Delta R.T.: 0.010 min
Response: 14870
Conc: 0.98 ng/ml

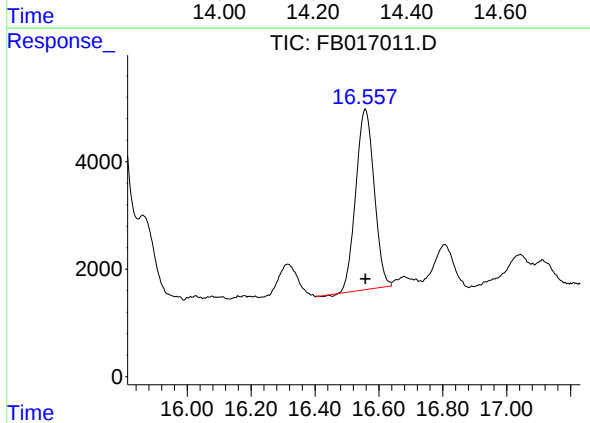

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.000 min
Response: 133724
Conc: 7.25 ng/ml