

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
 Data File : FB017012.D
 Signal(s) : FID2B.CH
 Acq On : 31 Jul 2018 4:56
 Operator : MJ/SJ
 Sample : J4231-15
 Misc : 4.99g/5.00mL DI Water
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 10 09:58:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.113	129196	16.325 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.965	2875	0.199 ng/ml
2) t 2,2,4-Trimethylpentane	7.753	3839	0.274 ng/ml
3) t n-Heptane	8.067	13812	0.982 ng/ml
4) t Benzene	8.207	52221	2.973 ng/ml
6) t Toluene	10.960	104208	7.588 ng/ml
7) t Ethylbenzene	13.410	3300065	242.006 ng/ml
8) t m-Xylene	13.540	949611	66.003 ng/ml
9) t O-Xylene	14.275	624747	40.965 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	2627191	142.342 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
Data File : FB017012.D
Signal(s) : FID2B.CH
Acq On : 31 Jul 2018 4:56
Operator : MJ/SJ
Sample : J4231-15
Misc : 4.99g/5.00mL DI Water
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 10 09:58:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

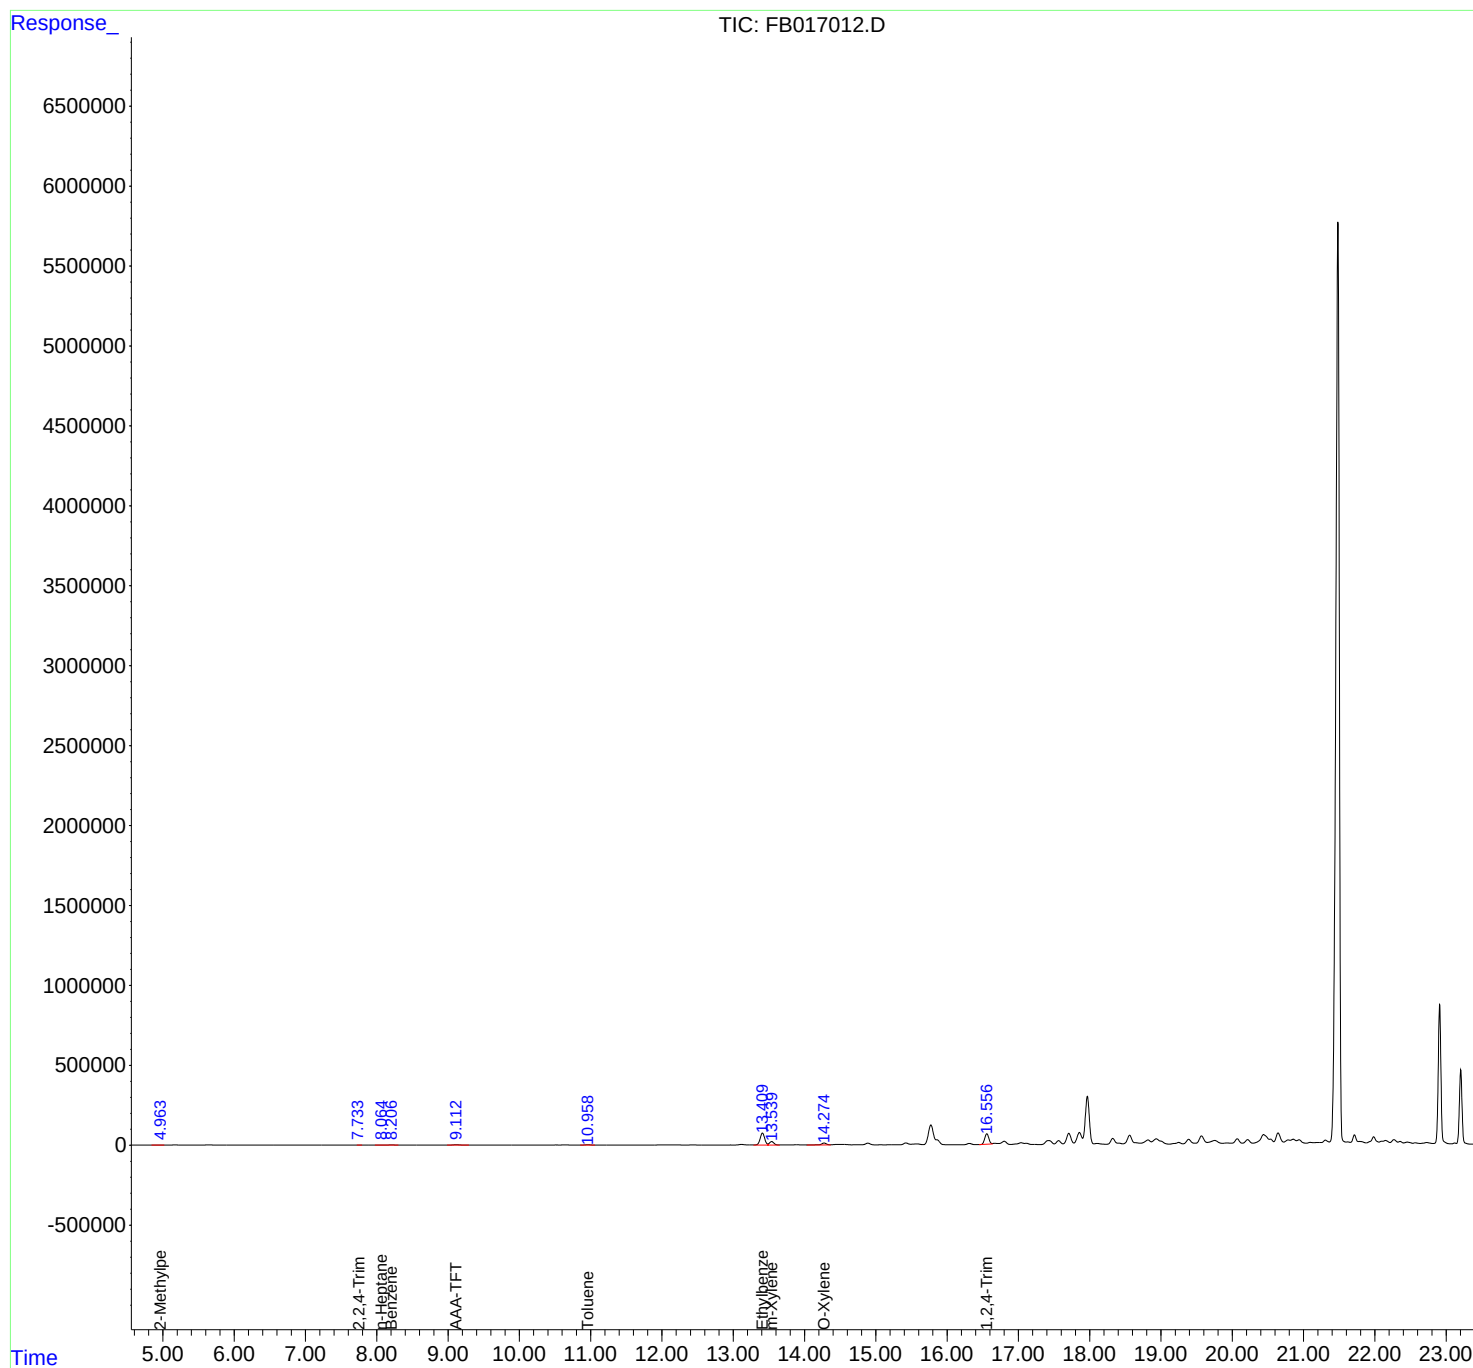


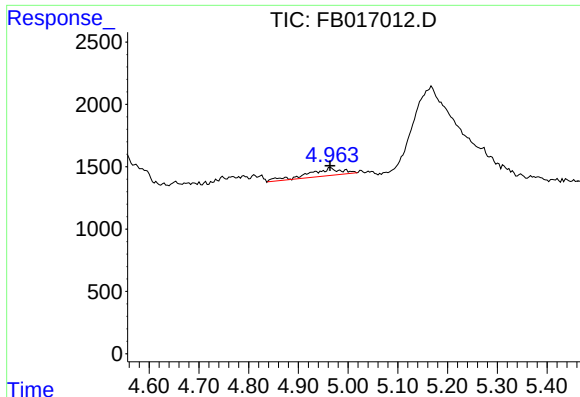

#1 2-Methylpentane


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 2875
Conc: 0.20 ng/ml

Instrument :
FID_B
ClientSampleId :

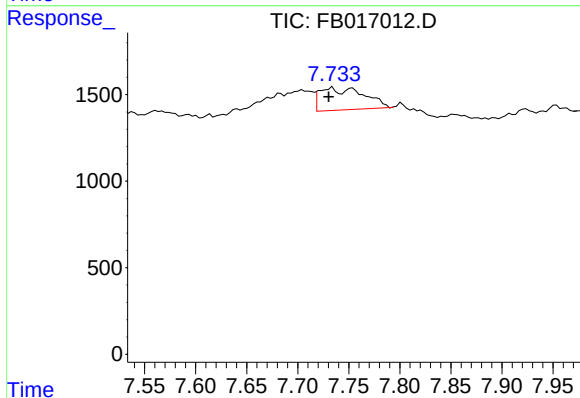


#2 2,2,4-Trimethylpentane

R.T.: 7.753 min
Delta R.T.: 0.023 min
Response: 3839
Conc: 0.27 ng/ml

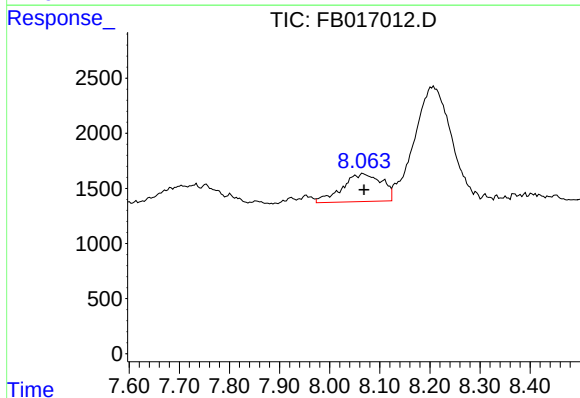


#3 n-Heptane

R.T.: 8.067 min
Delta R.T.: -0.002 min
Response: 13812
Conc: 0.98 ng/ml

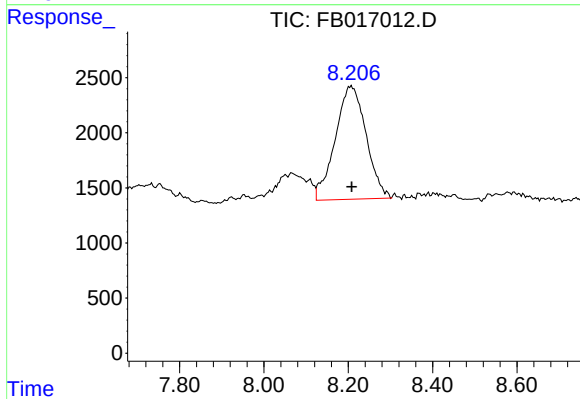

#4 Benzene


R.T.: 8.207 min
Delta R.T.: -0.002 min
Response: 52221
Conc: 2.97 ng/ml

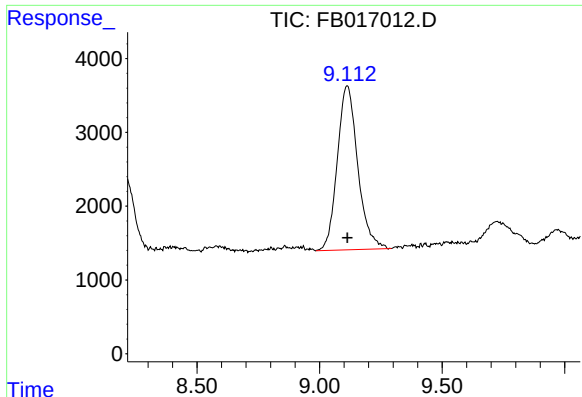

#5 AAA-TFT


R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 129196
Conc: 16.32 ng/ml

Instrument :
FID_B
ClientSampleId :

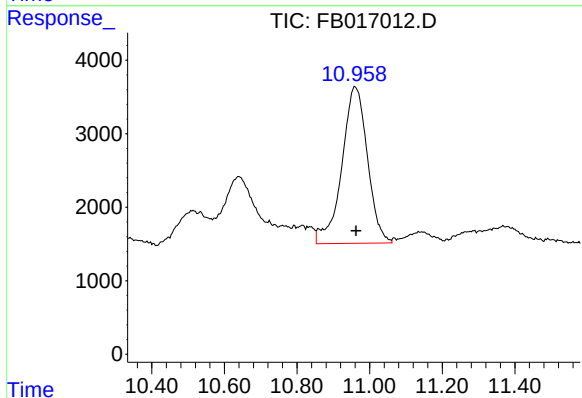


#6 Toluene

R.T.: 10.960 min
Delta R.T.: -0.003 min
Response: 104208
Conc: 7.59 ng/ml

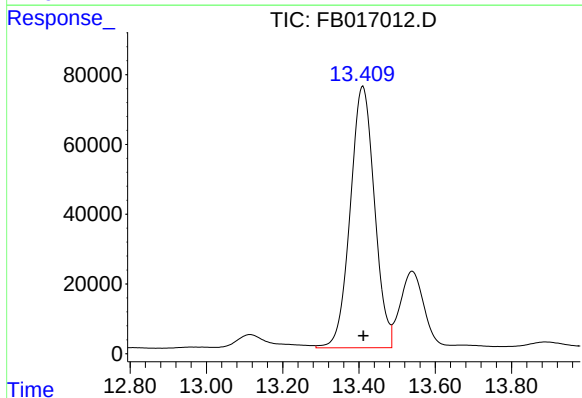


#7 Ethylbenzene

R.T.: 13.410 min
Delta R.T.: -0.001 min
Response: 3300065
Conc: 242.01 ng/ml

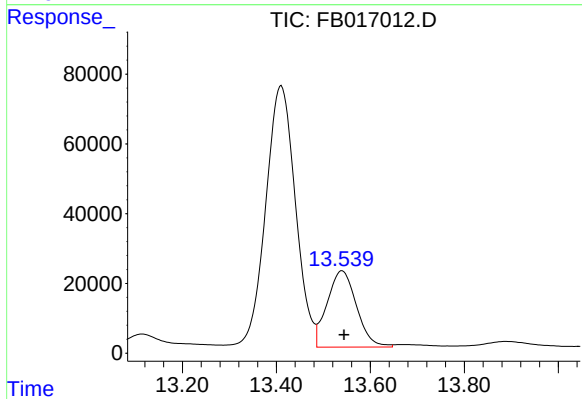

#8 m-Xylene


R.T.: 13.540 min
Delta R.T.: -0.004 min
Response: 949611
Conc: 66.00 ng/ml

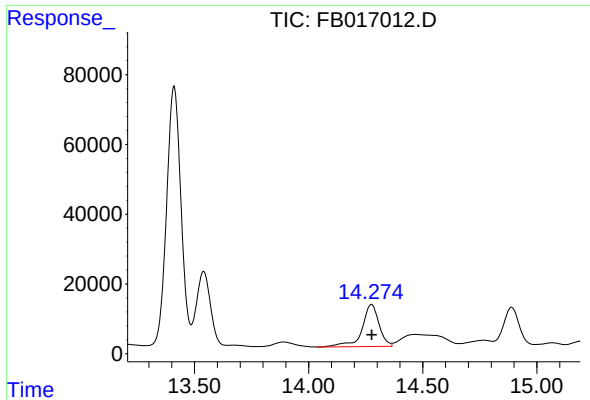

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: 0.000 min
Response: 624747
Conc: 40.97 ng/ml

Instrument :
FID_B
ClientSampleId :

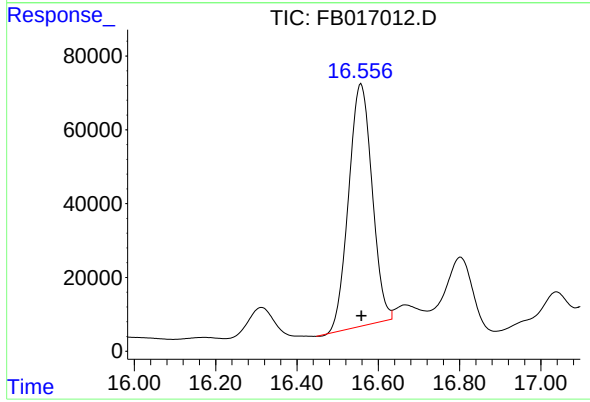

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.000 min
Response: 2627191
Conc: 142.34 ng/ml