

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
 Data File : FB016992.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jul 2018 11:18
 Operator : MJ/SJ
 Sample : BSF0730S1
 Misc : 5.01g/5.00ml DI water
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0730S1

Integration File: Calibration.e
 Quant Time: Jul 31 09:04:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.113	159755	20.186 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.965	447842	31.025 ng/ml
2) t 2,2,4-Trimethylpentane	7.728	429408	30.696 ng/ml
3) t n-Heptane	8.068	139428	9.915 ng/ml
4) t Benzene	8.208	177827	10.122 ng/ml
6) t Toluene	10.961	428179	31.180 ng/ml
7) t Ethylbenzene	13.411	144430	10.592 ng/ml
8) t m-Xylene	13.544	306263	21.287 ng/ml
9) t O-Xylene	14.275	320788	21.034 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	380329	20.606 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
Data File : FB016992.D
Signal(s) : FID2B.CH
Acq On : 30 Jul 2018 11:18
Operator : MJ/SJ
Sample : BSF0730S1
Misc : 5.01g/5.00ml DI water
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0730S1

Integration File: Calibration.e
Quant Time: Jul 31 09:04:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

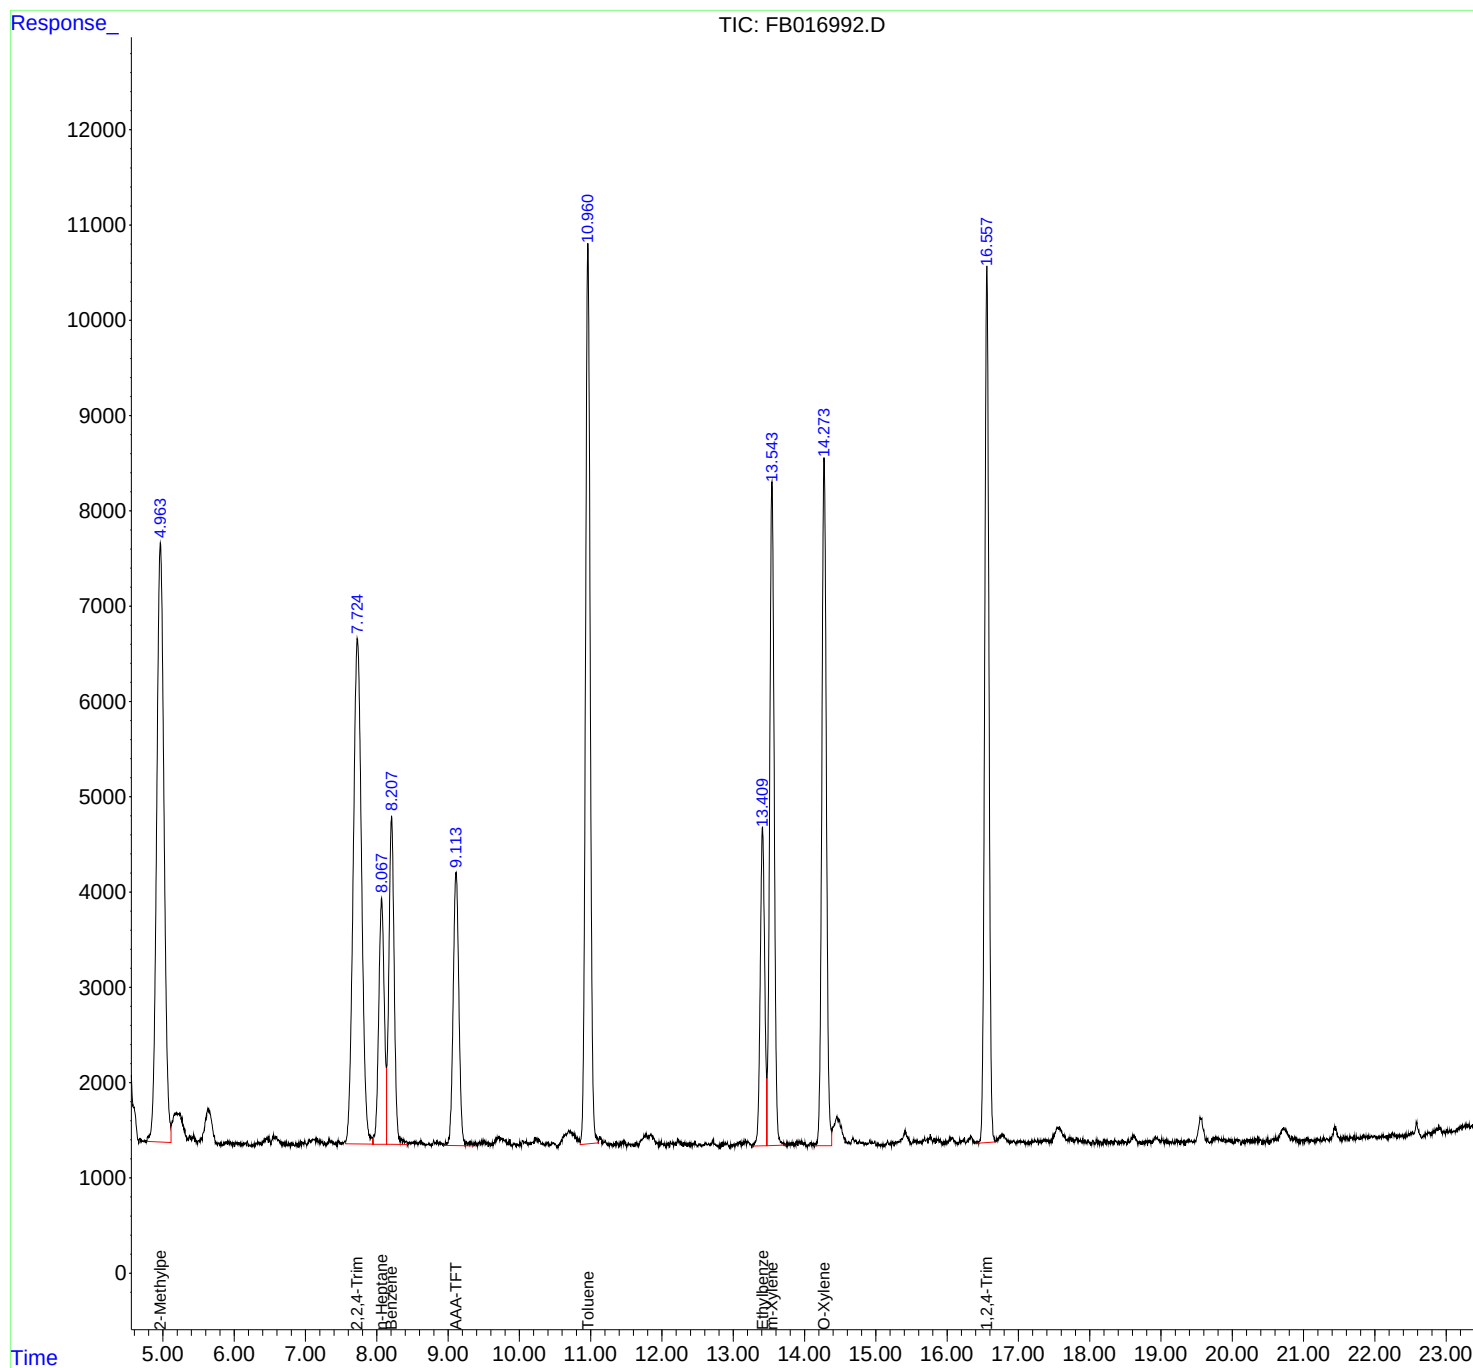


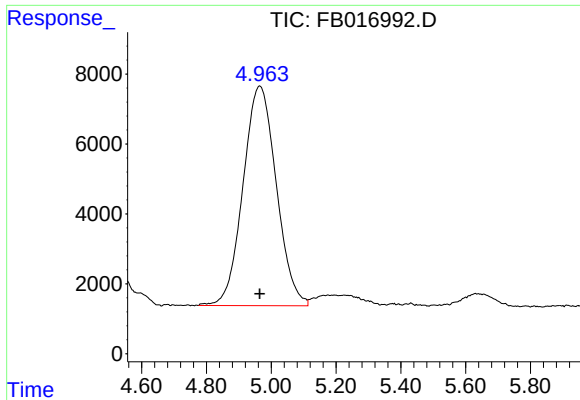

#1 2-Methylpentane


R.T.: 4.965 min
Delta R.T.: 0.001 min
Response: 447842
Conc: 31.02 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0730S1

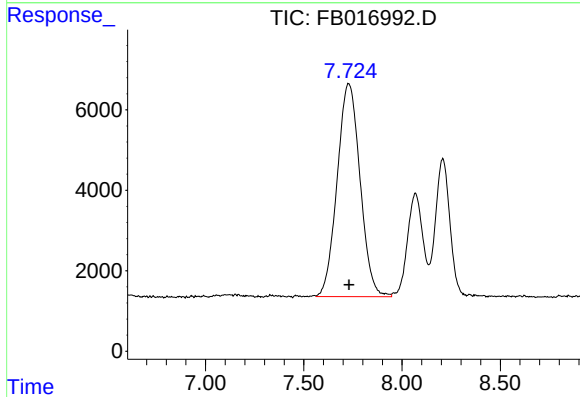


#2 2,2,4-Trimethylpentane

R.T.: 7.728 min
Delta R.T.: -0.003 min
Response: 429408
Conc: 30.70 ng/ml

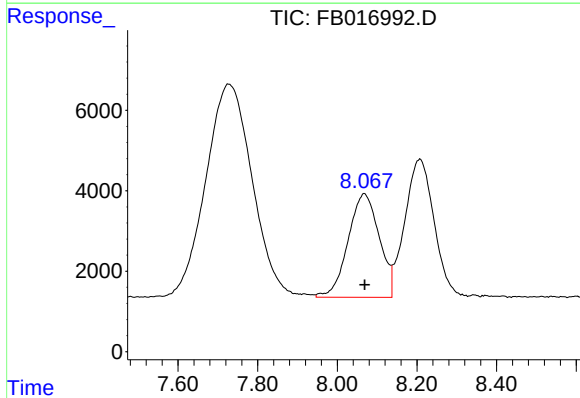


#3 n-Heptane

R.T.: 8.068 min
Delta R.T.: 0.000 min
Response: 139428
Conc: 9.92 ng/ml

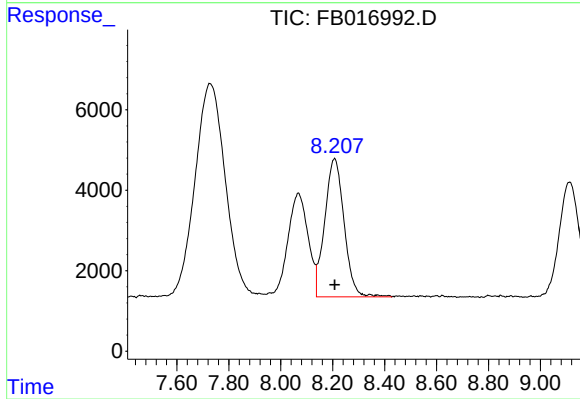

#4 Benzene


R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 177827
Conc: 10.12 ng/ml

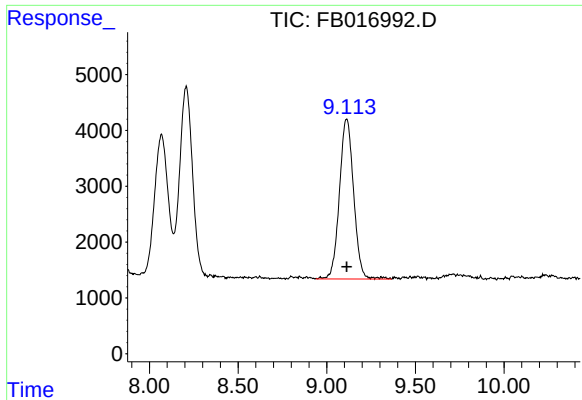

#5 AAA-TFT


R.T.: 9.113 min
Delta R.T.: -0.001 min
Response: 159755
Conc: 20.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0730S1

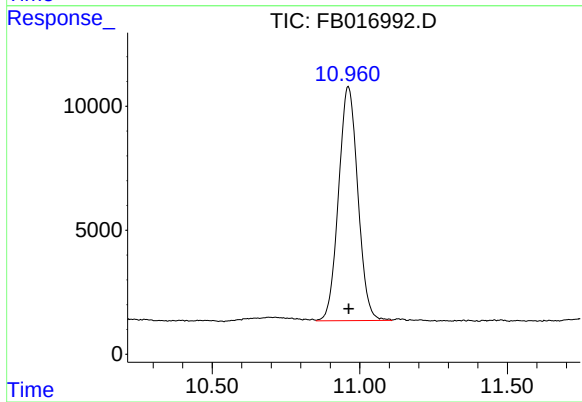


#6 Toluene

R.T.: 10.961 min
Delta R.T.: -0.001 min
Response: 428179
Conc: 31.18 ng/ml

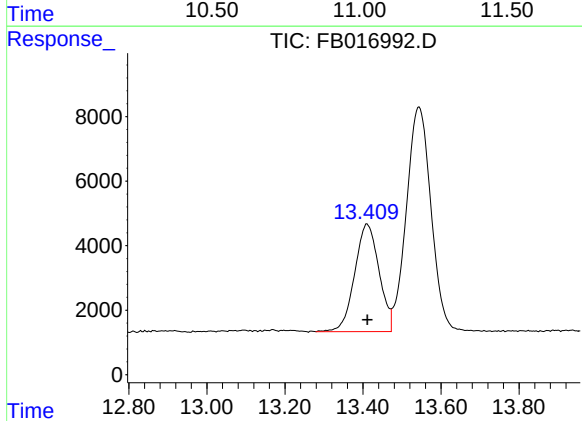


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 144430
Conc: 10.59 ng/ml

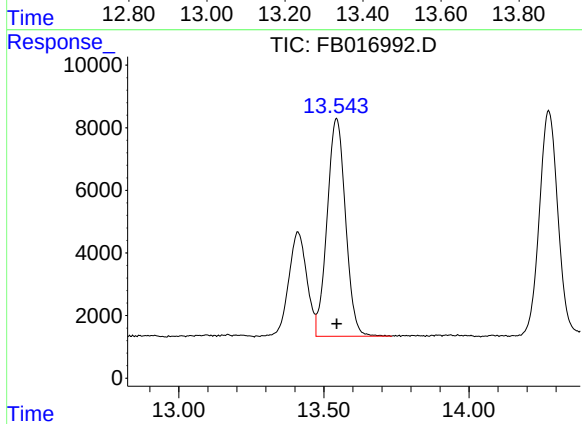

#8 m-Xylene


R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 306263
Conc: 21.29 ng/ml

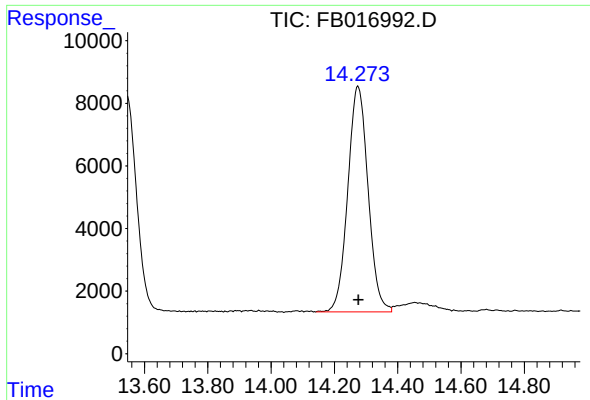

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: 0.000 min
Response: 320788
Conc: 21.03 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0730S1

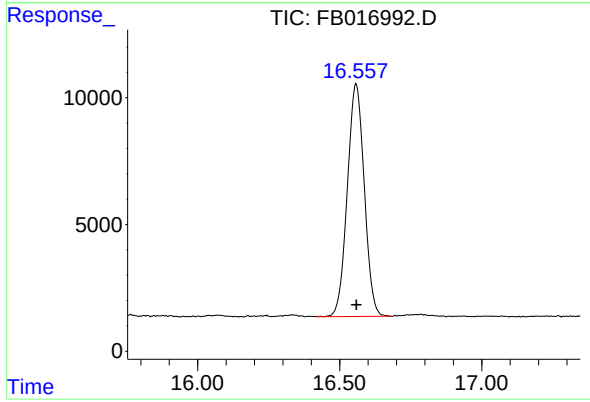

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.000 min
Response: 380329
Conc: 20.61 ng/ml