

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
Data File : FB017008.D
Signal(s) : FID2B.CH
Acq On : 31 Jul 2018 00:52
Operator : MJ/SJ
Sample : J4231-13
Misc : 5.00g/5.00ml DI water
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-7

Integration File: Calibration.e
Quant Time: Jul 31 09:07:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	135073	16.978 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073018\
Data File : FB017008.D
Signal(s) : FID2B.CH
Acq On : 31 Jul 2018 00:52
Operator : MJ/SJ
Sample : J4231-13
Misc : 5.00g/5.00ml DI water
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-7

Integration File: Calibration.e
Quant Time: Jul 31 09:07:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

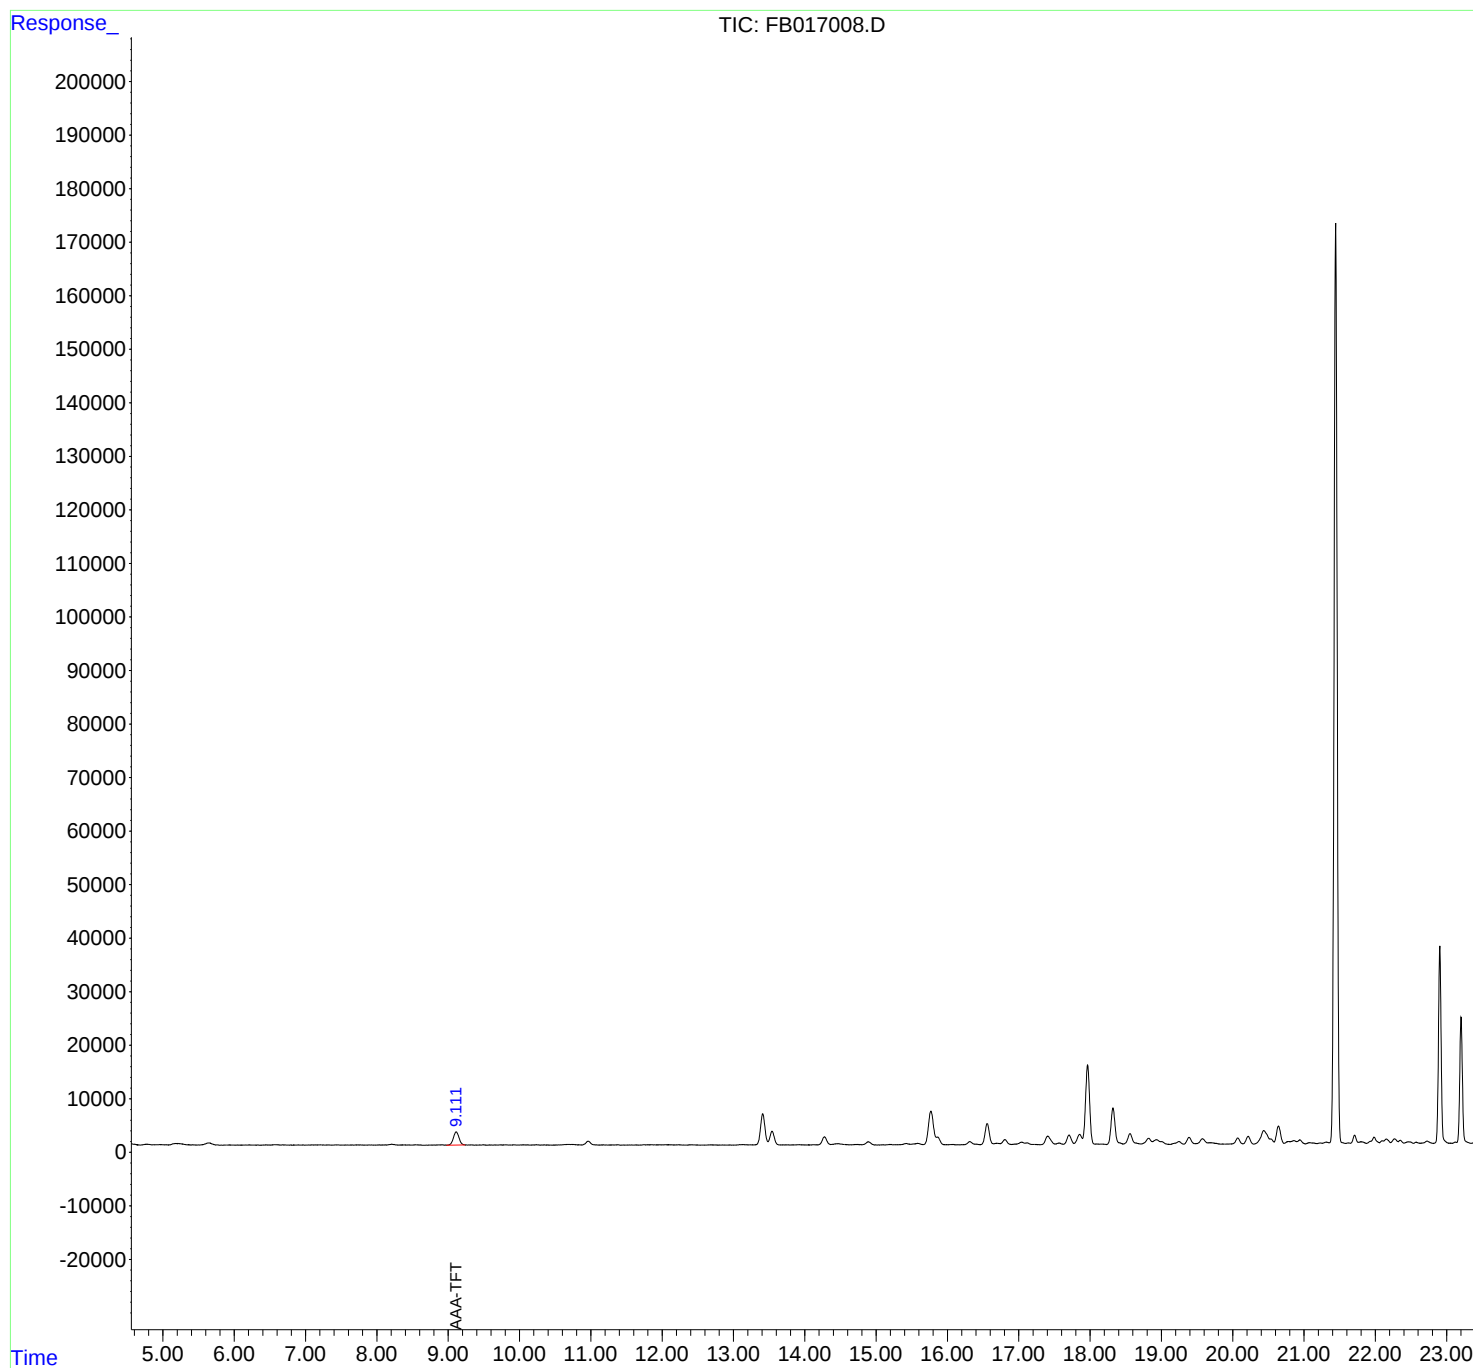

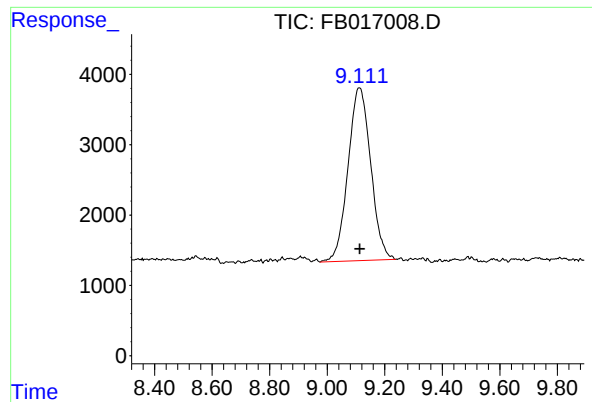

#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: -0.002 min
Response: 135073
Conc: 16.98 ng/ml

Instrument :
FID_B
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-7