

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073019\
 Data File : FB021859.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jul 2019 9:02
 Operator : DD/AJ
 Sample : BSF0730S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Jul 31 00:50:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.989	270217	19.801 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.862	725110	26.295 ng/ml
2) t	2,2,4-Trimethylpentane	7.609	718491	27.180 ng/ml
3) t	n-Heptane	7.948	218760	8.823 ng/ml
4) t	Benzene	8.082	282805	9.680 ng/ml
6) t	Toluene	10.830	622389	30.248 ng/ml
7) t	Ethylbenzene	13.275	225342	10.831 ng/ml
8) t	m-Xylene	13.407	480515	21.630 ng/ml
9) t	O-Xylene	14.137	488191	21.223 ng/ml
10) t	1,2,4-Trimethylbenzene	16.416	500589	21.232 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073019\
Data File : FB021859.D
Signal(s) : FID2B.CH
Acq On : 30 Jul 2019 9:02
Operator : DD/AJ
Sample : BSF0730S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Jul 31 00:50:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

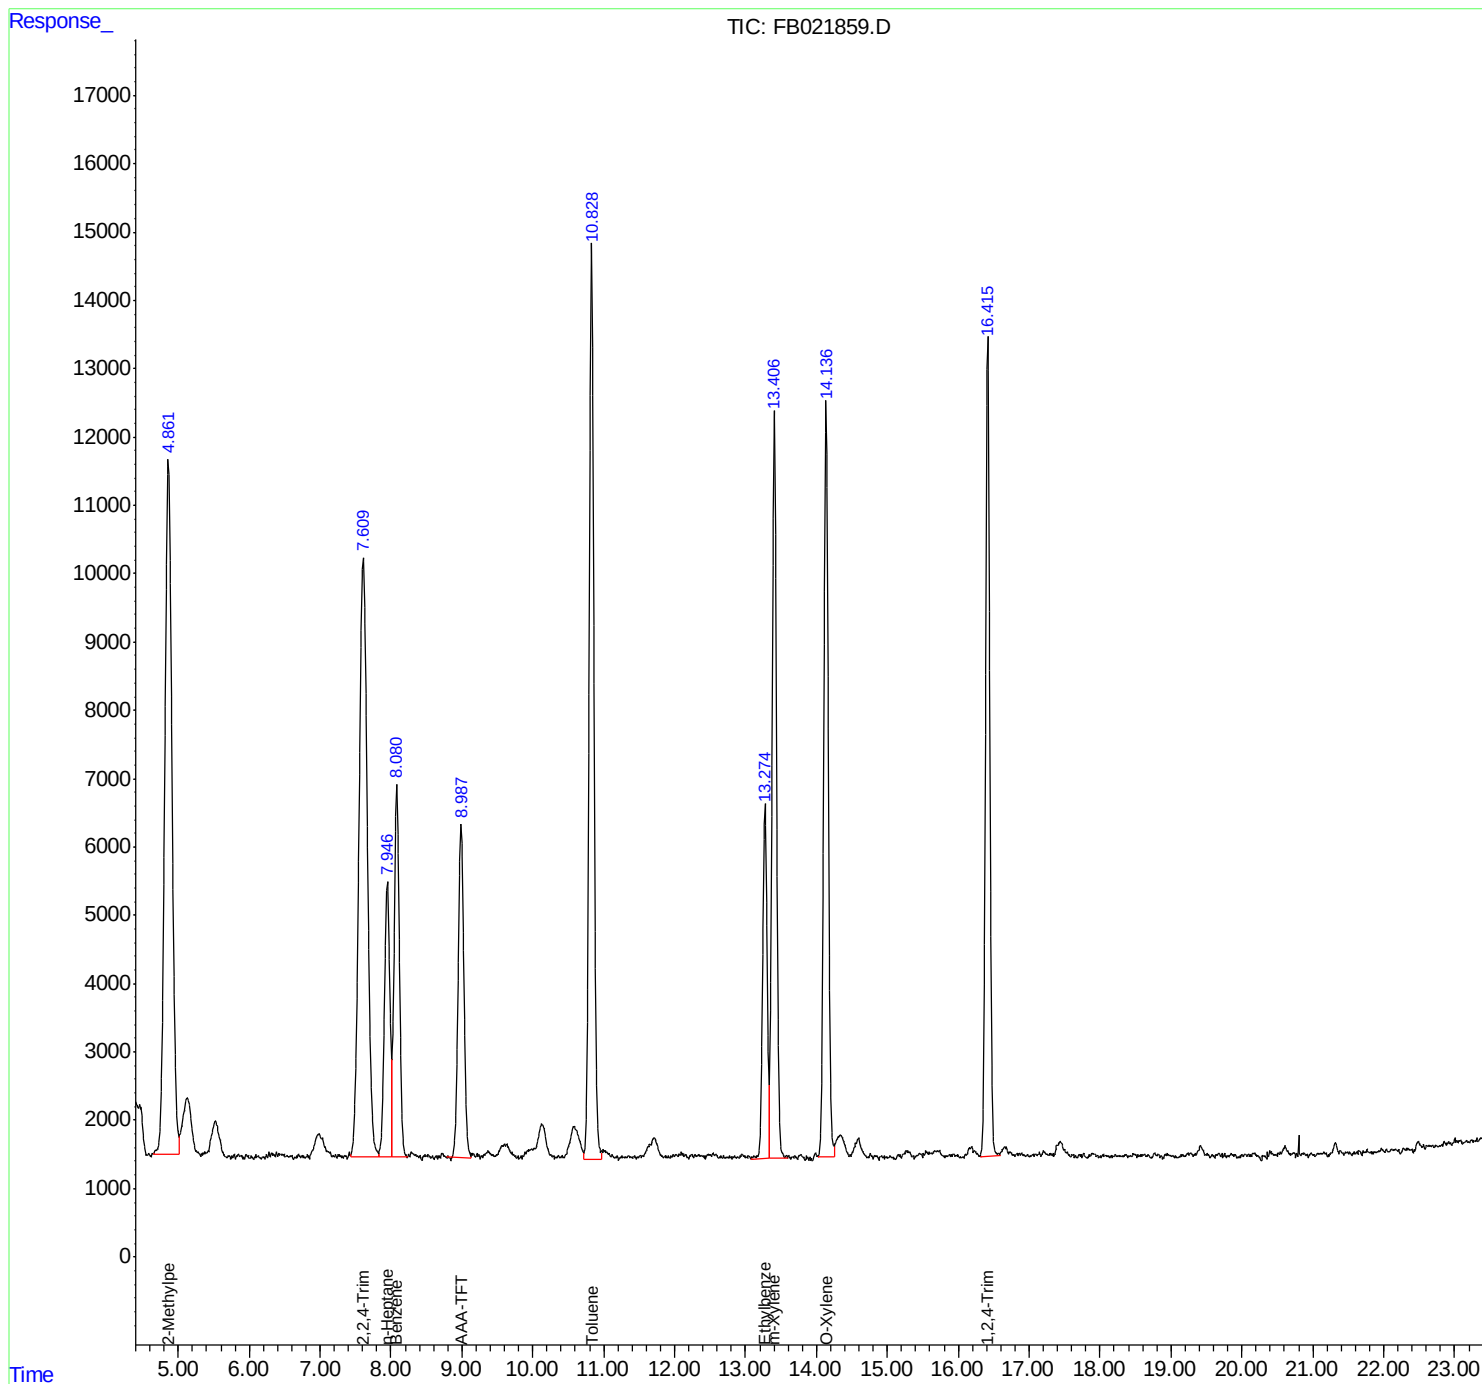

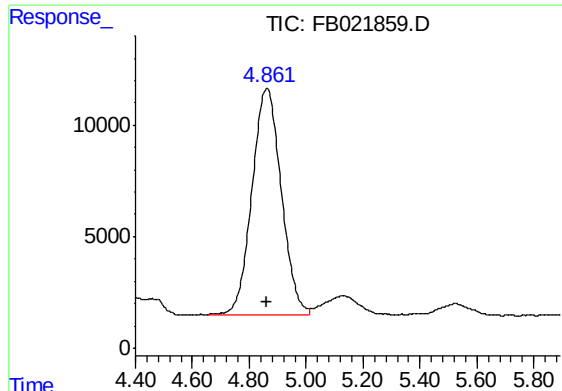


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 725110
Conc: 26.29 ng/ml

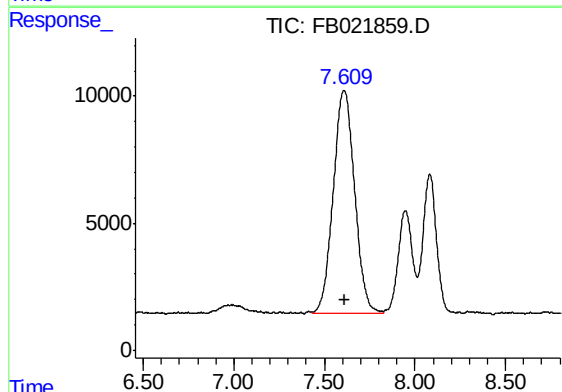


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.004 min
Response: 718491
Conc: 27.18 ng/ml

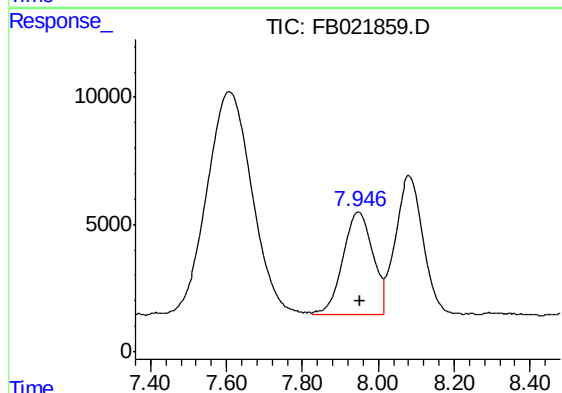


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: -0.004 min
Response: 218760
Conc: 8.82 ng/ml

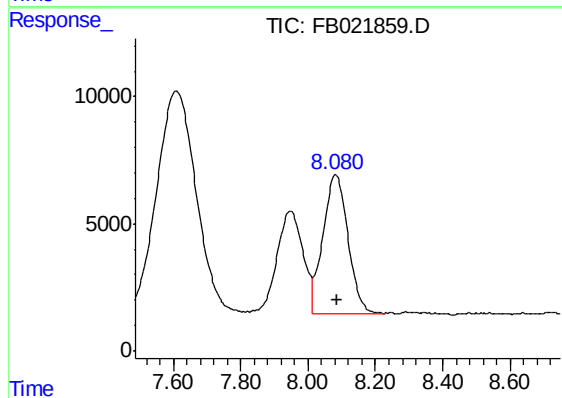


#4 Benzene

R.T.: 8.082 min
Delta R.T.: -0.004 min
Response: 282805
Conc: 9.68 ng/ml

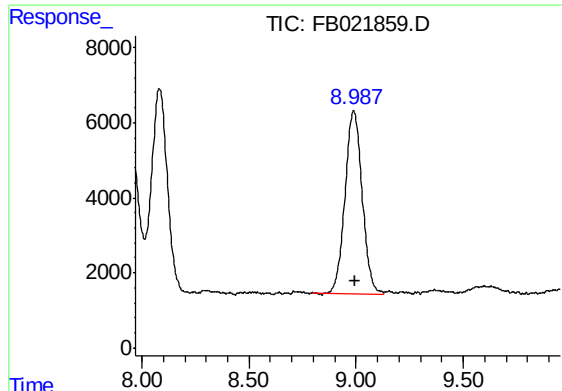


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.003 min
Response: 270217
Conc: 19.80 ng/ml

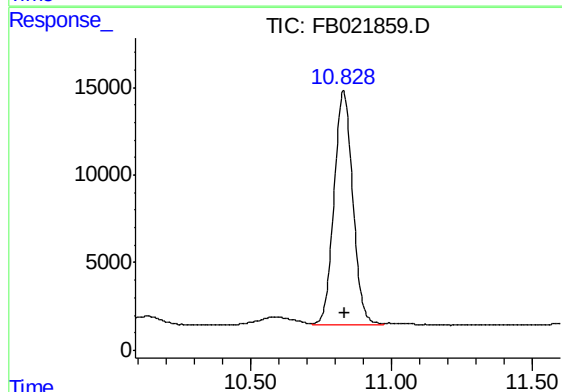


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.004 min
Response: 622389
Conc: 30.25 ng/ml

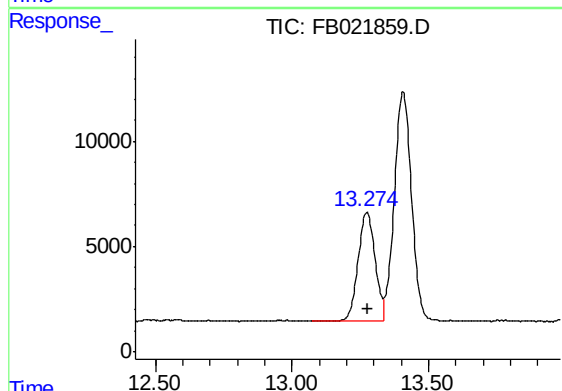


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: -0.003 min
Response: 225342
Conc: 10.83 ng/ml

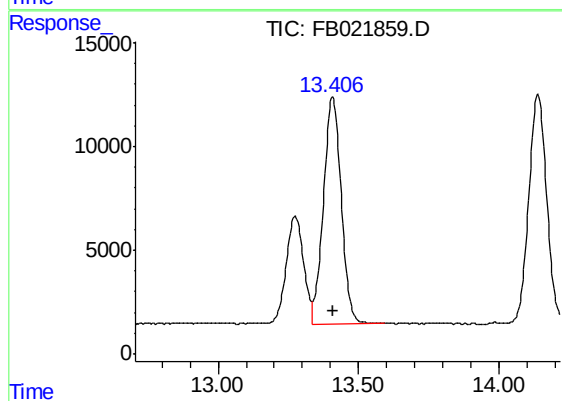


#8 m-Xylene

R.T.: 13.407 min
Delta R.T.: -0.003 min
Response: 480515
Conc: 21.63 ng/ml

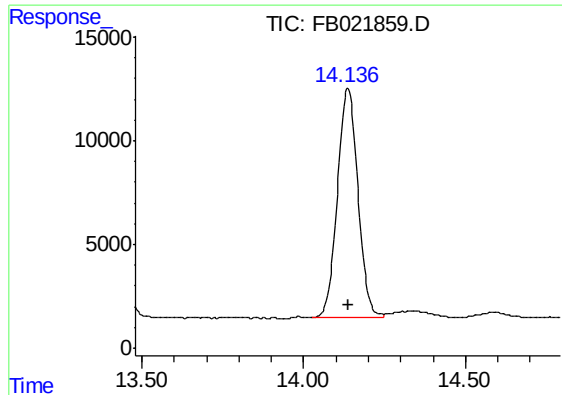

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: -0.003 min
Response: 488191
Conc: 21.22 ng/ml

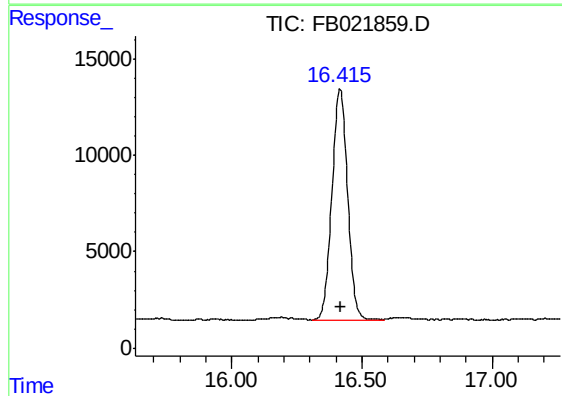

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: -0.003 min
Response: 500589
Conc: 21.23 ng/ml