

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073019\
 Data File : FB021861.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jul 2019 11:48
 Operator : DD/AJ
 Sample : K3621-07MS
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Jul 31 00:50:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.990	301998	22.130 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.862	637942	23.134 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	613317	23.202 ng/ml
3) t n-Heptane	7.949	185606	7.486 ng/ml
4) t Benzene	8.084	288311	9.869 ng/ml
6) t Toluene	10.831	573780	27.885 ng/ml
7) t Ethylbenzene	13.276	186364	8.958 ng/ml
8) t m-Xylene	13.409	389997	17.555 ng/ml
9) t O-Xylene	14.138	412260	17.922 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	407075	17.266 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073019\
Data File : FB021861.D
Signal(s) : FID2B.CH
Acq On : 30 Jul 2019 11:48
Operator : DD/AJ
Sample : K3621-07MS
Misc : 5.02/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Jul 31 00:50:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

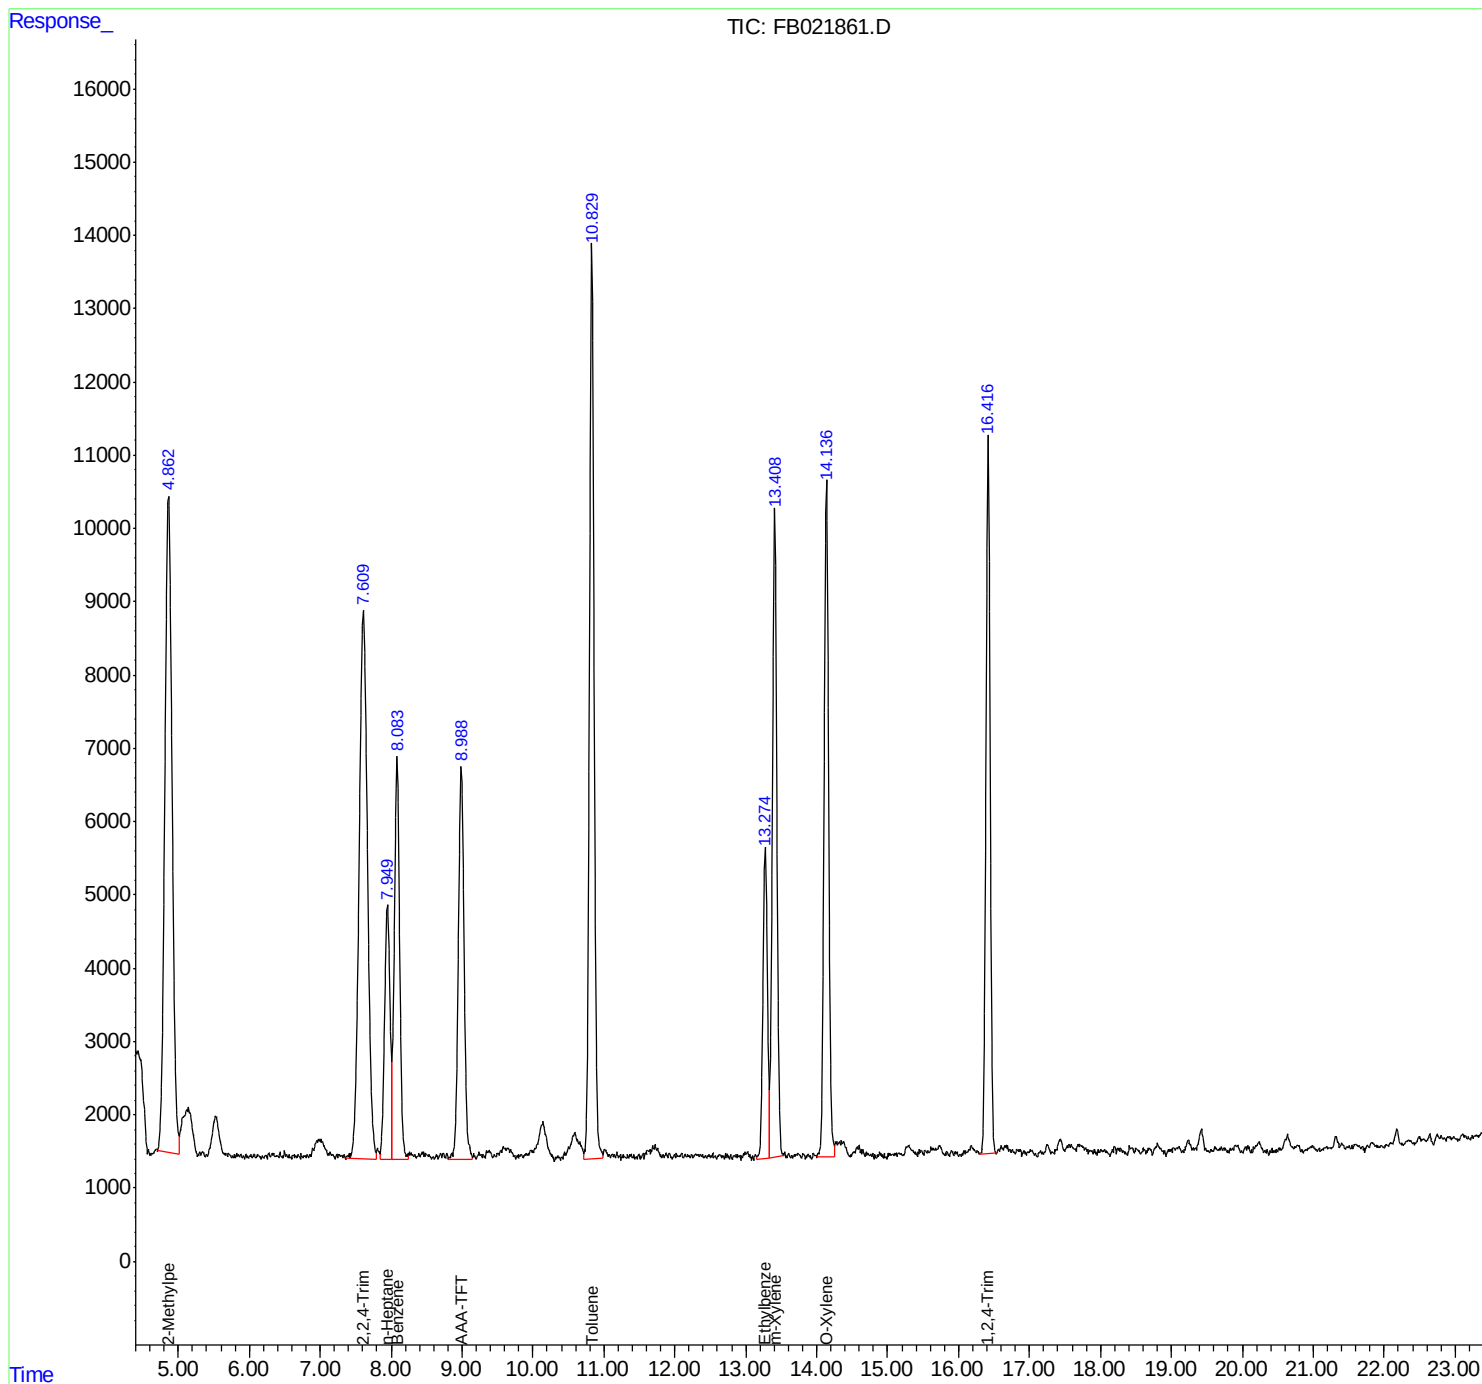

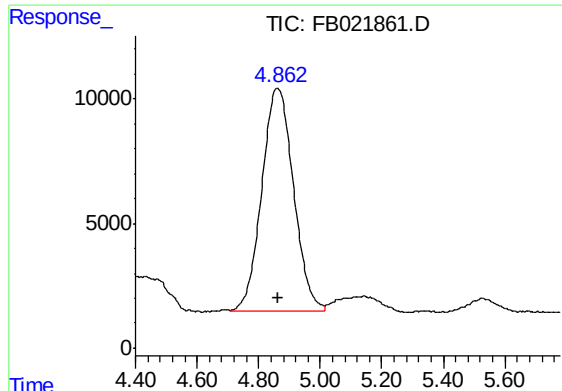


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 637942
Conc: 23.13 ng/ml

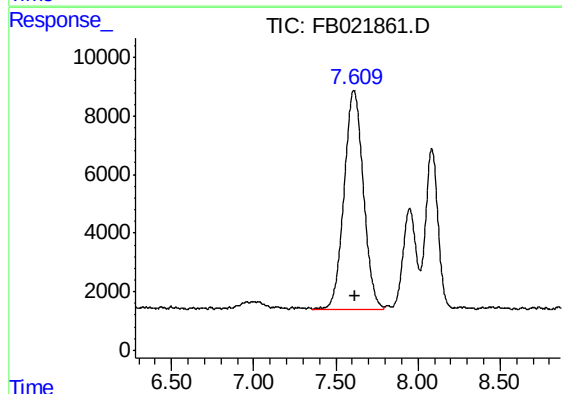


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.003 min
Response: 613317
Conc: 23.20 ng/ml

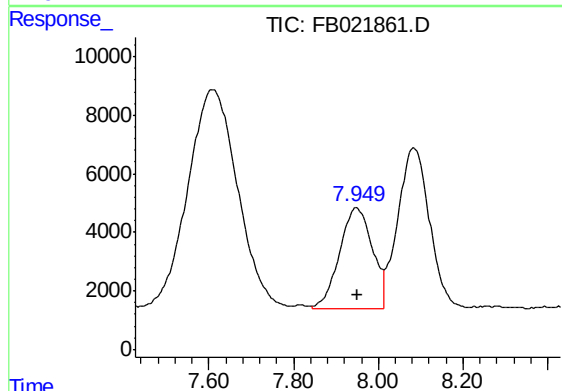


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 185606
Conc: 7.49 ng/ml

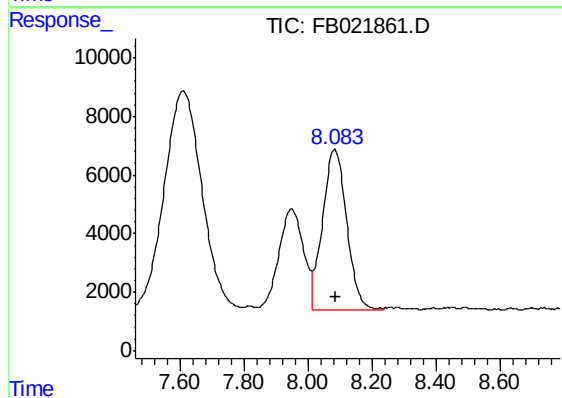


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 288311
Conc: 9.87 ng/ml

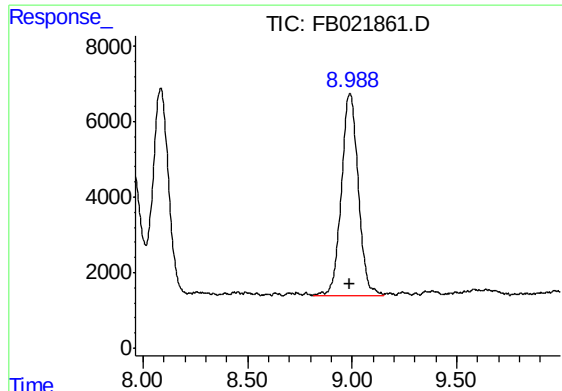


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.002 min
Response: 301998
Conc: 22.13 ng/ml

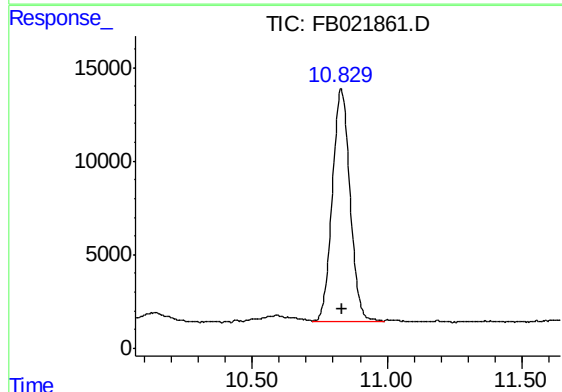


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.003 min
Response: 573780
Conc: 27.89 ng/ml

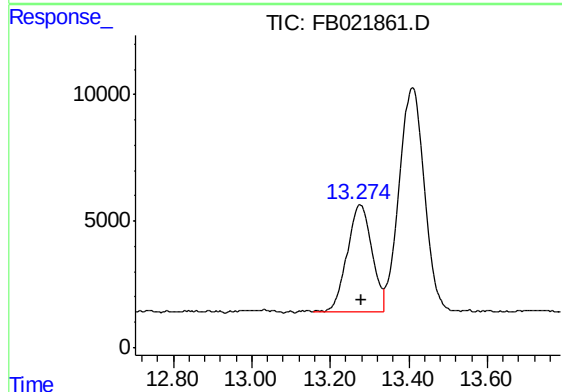


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.002 min
Response: 186364
Conc: 8.96 ng/ml

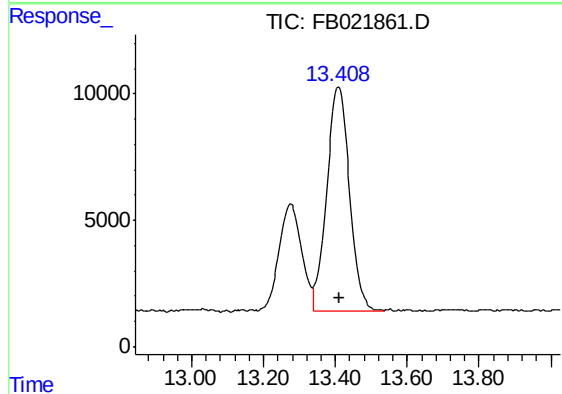


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 389997
Conc: 17.56 ng/ml

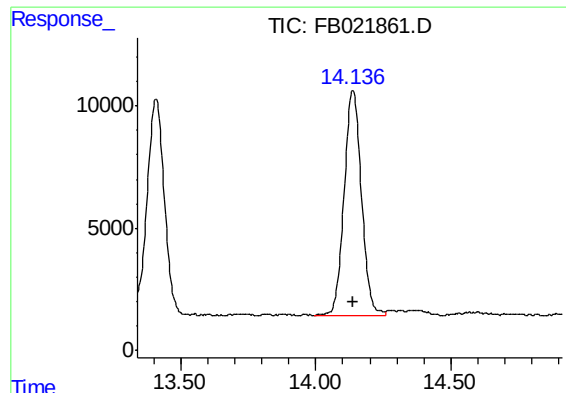

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.003 min
Response: 412260
Conc: 17.92 ng/ml

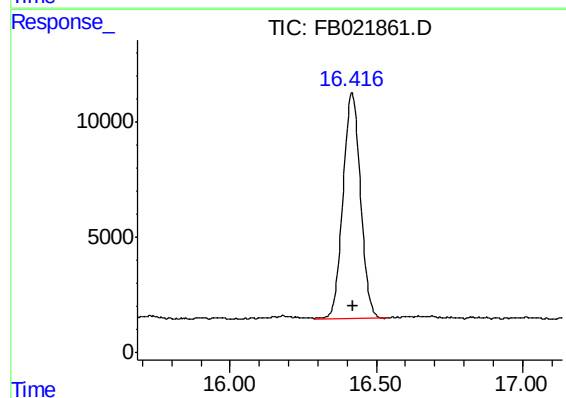

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.002 min
Response: 407075
Conc: 17.27 ng/ml