

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073019\
 Data File : FB021862.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jul 2019 12:18
 Operator : DD/AJ
 Sample : K3621-07MSD
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Jul 31 00:50:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.991	267194	19.579 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.863	587894	21.319 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	526628	19.922 ng/ml
3) t n-Heptane	7.949	159110	6.417 ng/ml
4) t Benzene	8.085	271251	9.285 ng/ml
6) t Toluene	10.832	540876	26.286 ng/ml
7) t Ethylbenzene	13.276	170739	8.207 ng/ml
8) t m-Xylene	13.409	364420	16.404 ng/ml
9) t O-Xylene	14.139	381887	16.602 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	367552	15.590 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073019\
Data File : FB021862.D
Signal(s) : FID2B.CH
Acq On : 30 Jul 2019 12:18
Operator : DD/AJ
Sample : K3621-07MSD
Misc : 5.03/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Jul 31 00:50:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

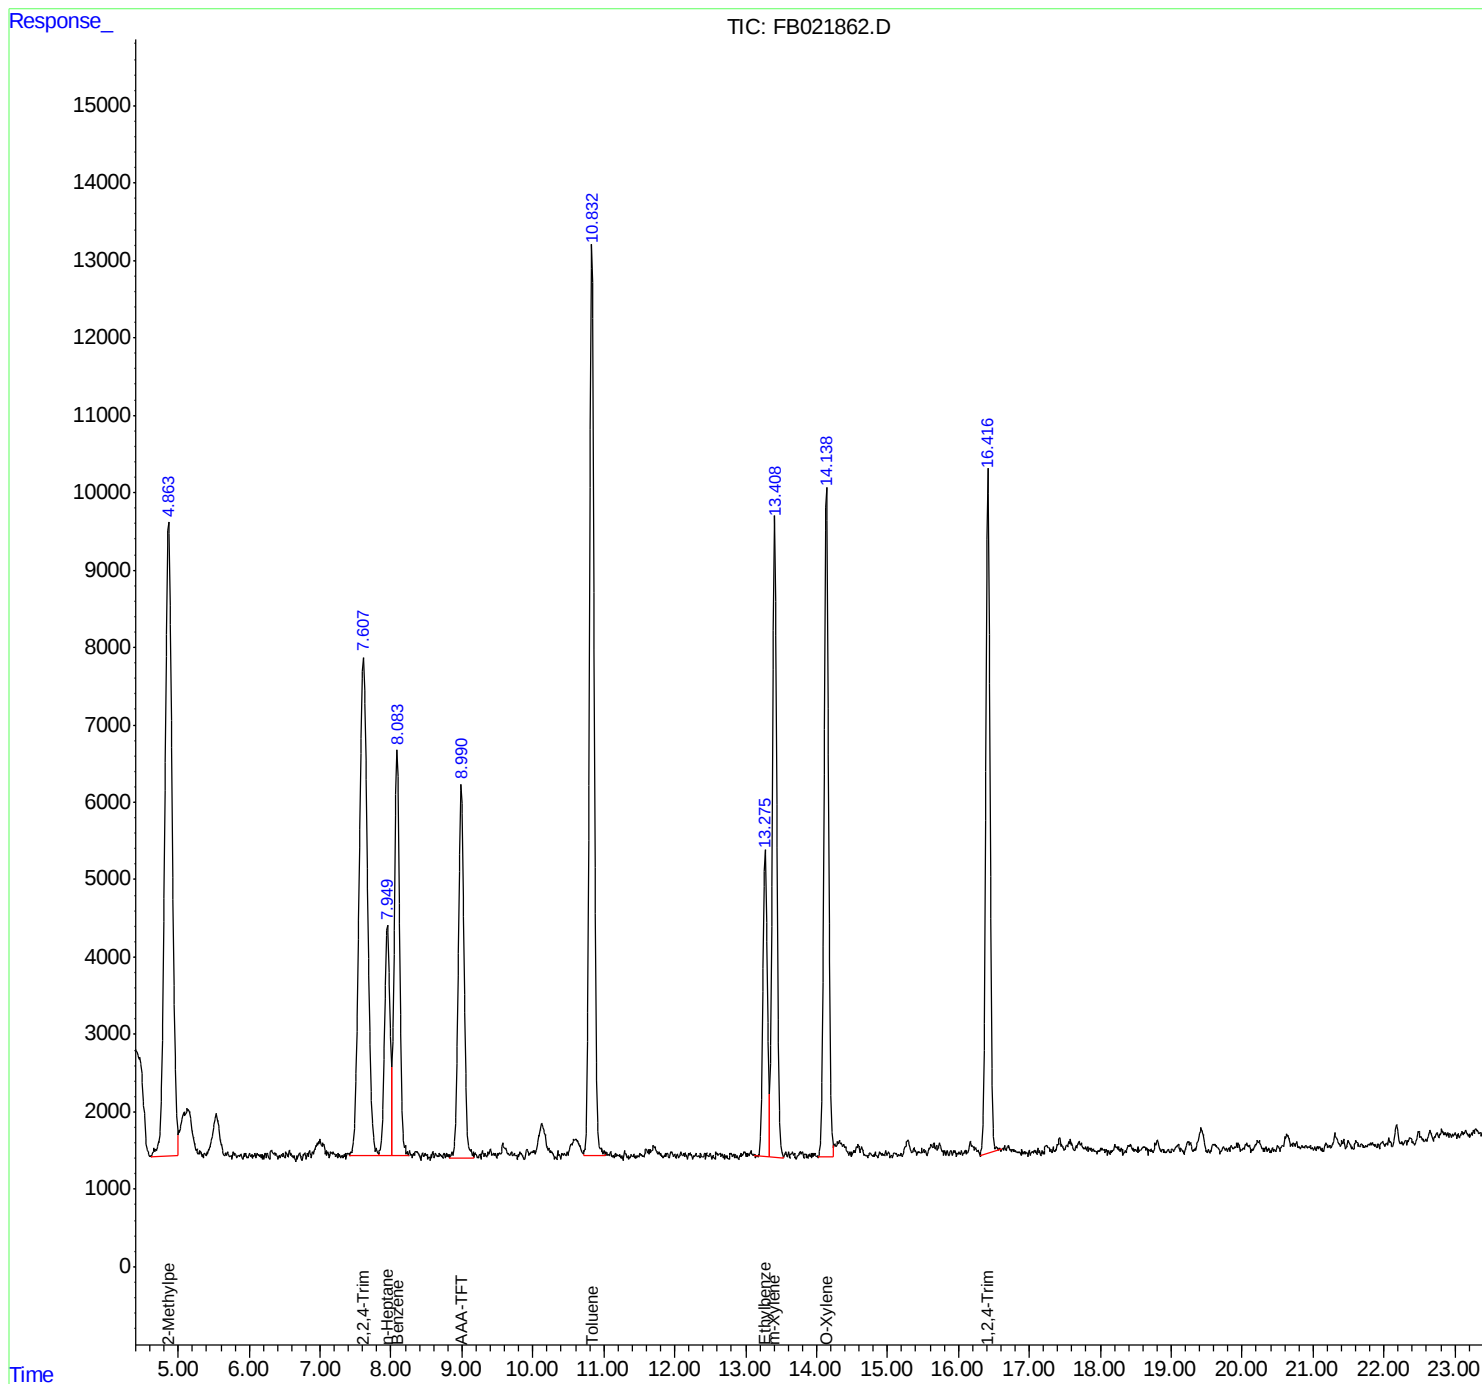

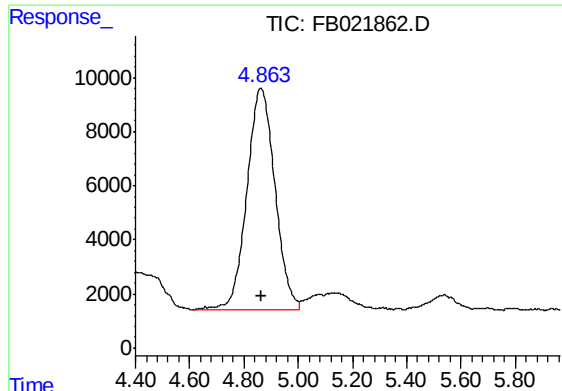


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 587894
Conc: 21.32 ng/ml

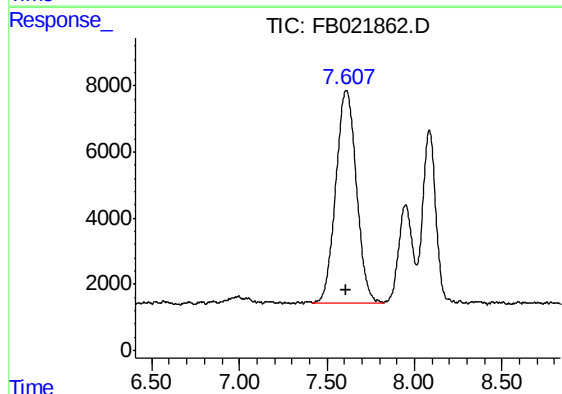


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.003 min
Response: 526628
Conc: 19.92 ng/ml

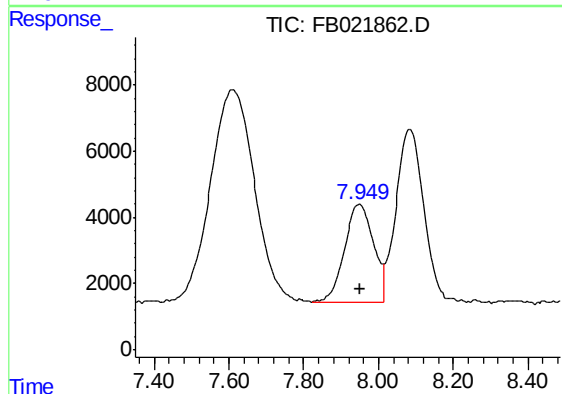


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 159110
Conc: 6.42 ng/ml

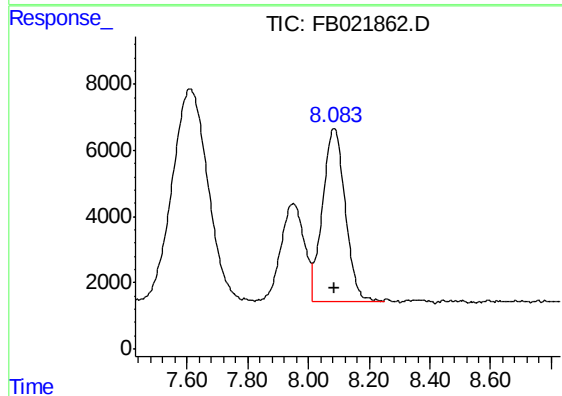


#4 Benzene

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 271251
Conc: 9.28 ng/ml

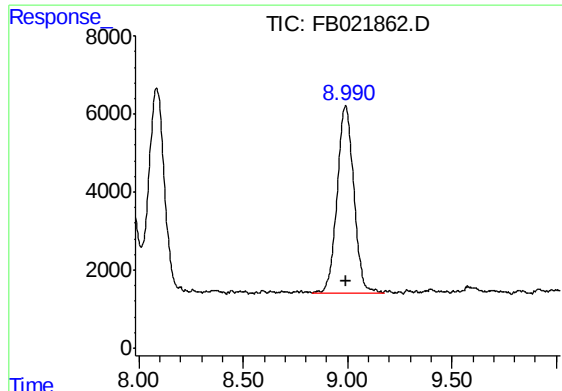


#5 AAA-TFT

R.T.: 8.991 min
Delta R.T.: -0.002 min
Response: 267194
Conc: 19.58 ng/ml

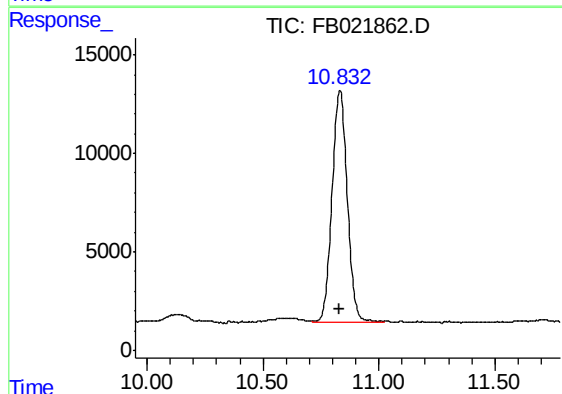


#6 Toluene

R.T.: 10.832 min
Delta R.T.: 0.000 min
Response: 540876
Conc: 26.29 ng/ml

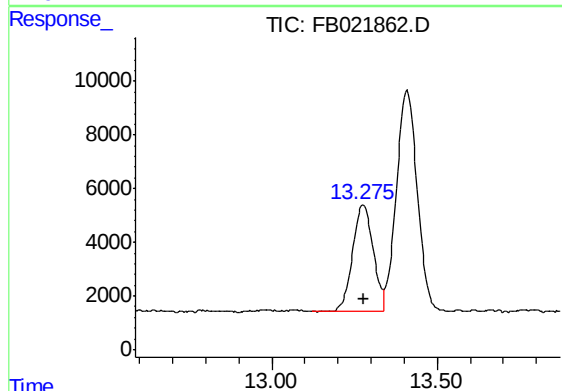


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.002 min
Response: 170739
Conc: 8.21 ng/ml

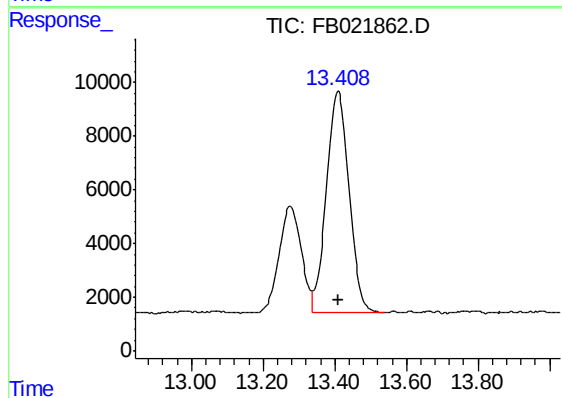


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 364420
Conc: 16.40 ng/ml

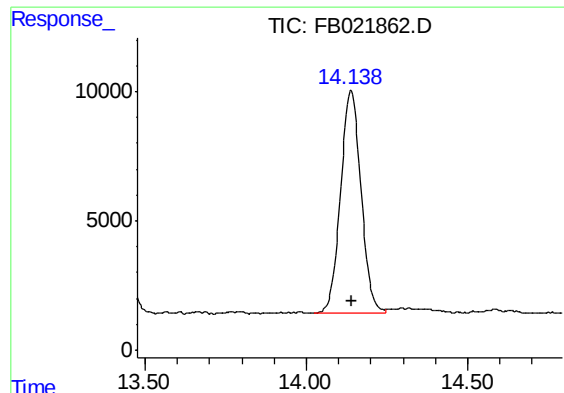

#9 O-Xylene

R.T.: 14.139 min
Delta R.T.: -0.002 min
Response: 381887
Conc: 16.60 ng/ml

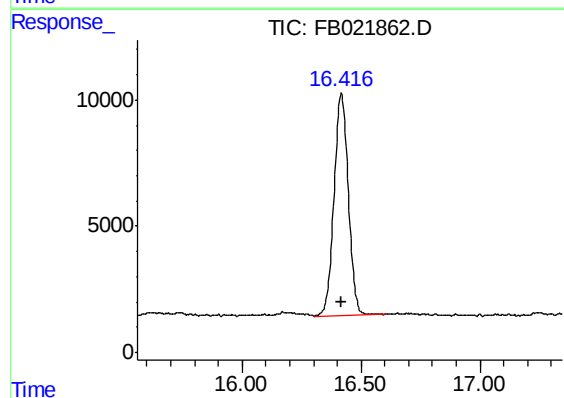

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: -0.002 min
Response: 367552
Conc: 15.59 ng/ml