

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073020\
 Data File : FB024701.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jul 2020 12:10
 Operator : DD/AJ
 Sample : BSF0730S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 31 01:29:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.801	452070	19.625 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	865640	29.251 ng/ml
2) t	2,2,4-Trimethylpentane	7.420	945210	30.192 ng/ml
3) t	n-Heptane	7.759	311566	10.021 ng/ml
4) t	Benzene	7.894	372794	9.780 ng/ml
6) t	Toluene	10.633	1072949	29.344 ng/ml
7) t	Ethylbenzene	13.072	321142	9.402 ng/ml
8) t	m-Xylene	13.205	634221	18.794 ng/ml
9) t	O-Xylene	13.933	624939	19.014 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	532973	19.758 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073020\
Data File : FB024701.D
Signal(s) : FID2B.CH
Acq On : 30 Jul 2020 12:10
Operator : DD/AJ
Sample : BSF0730S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 31 01:29:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

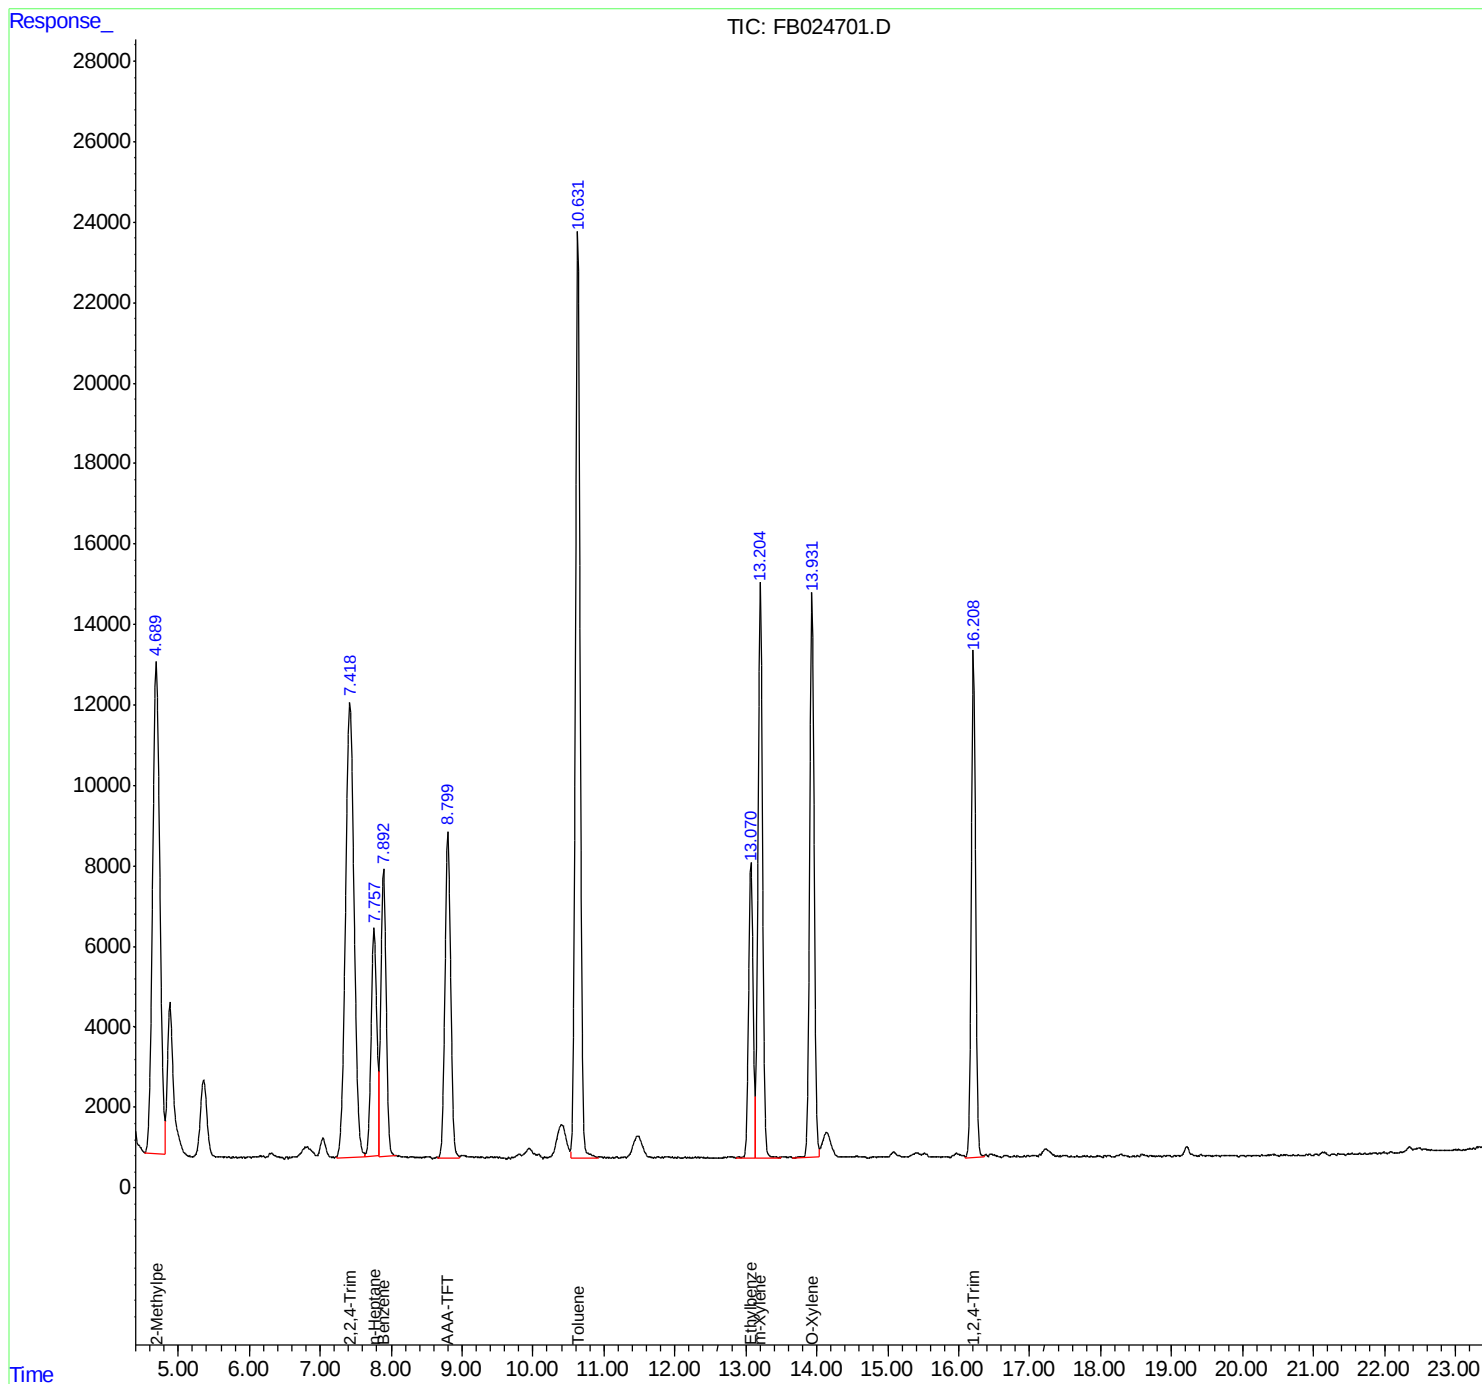

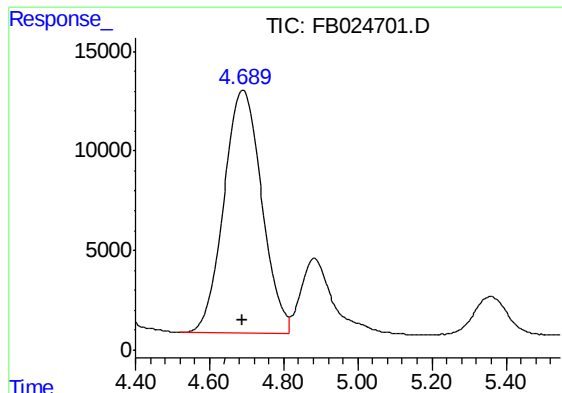


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.002 min
Response: 865640
Conc: 29.25 ng/ml

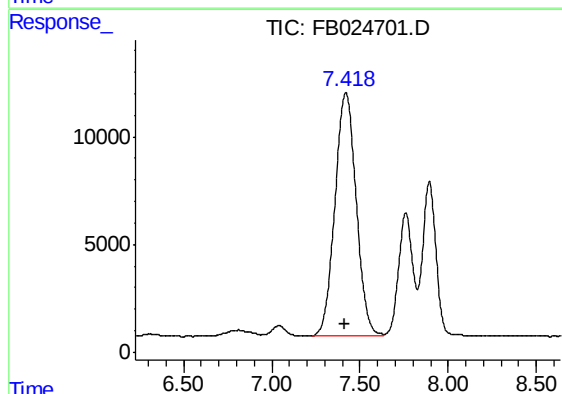


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.004 min
Response: 945210
Conc: 30.19 ng/ml

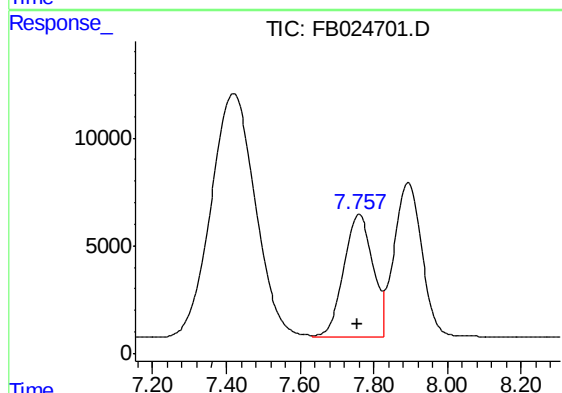


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.003 min
Response: 311566
Conc: 10.02 ng/ml

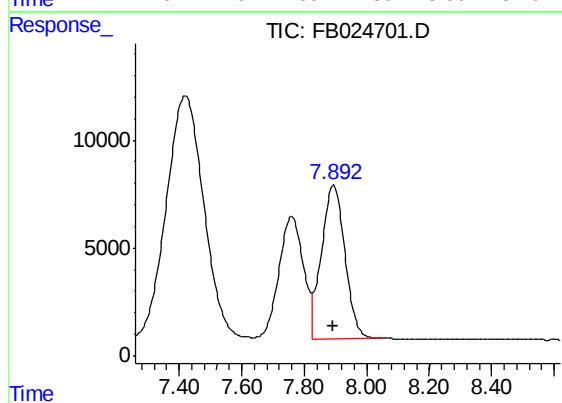


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 372794
Conc: 9.78 ng/ml

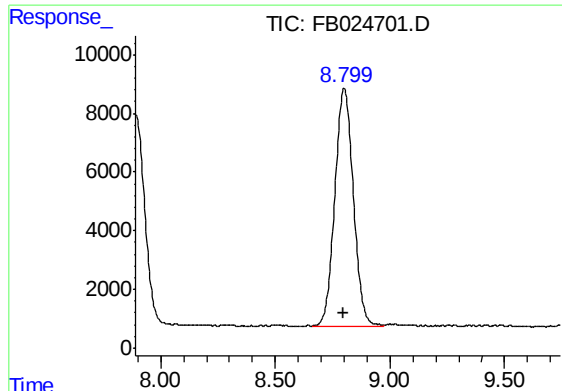


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.003 min
Response: 452070
Conc: 19.63 ng/ml

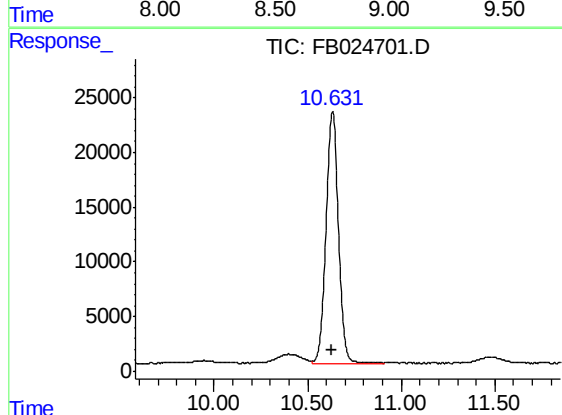


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.003 min
Response: 1072949
Conc: 29.34 ng/ml

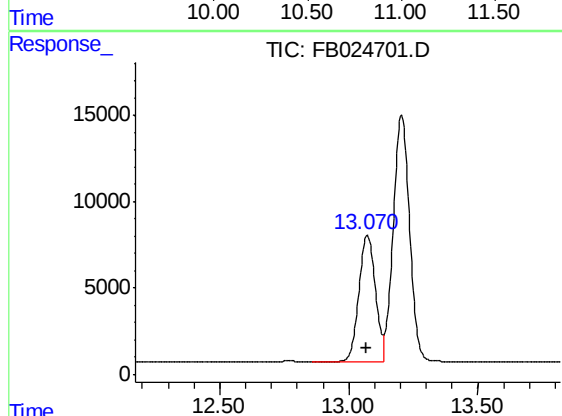


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.003 min
Response: 321142
Conc: 9.40 ng/ml

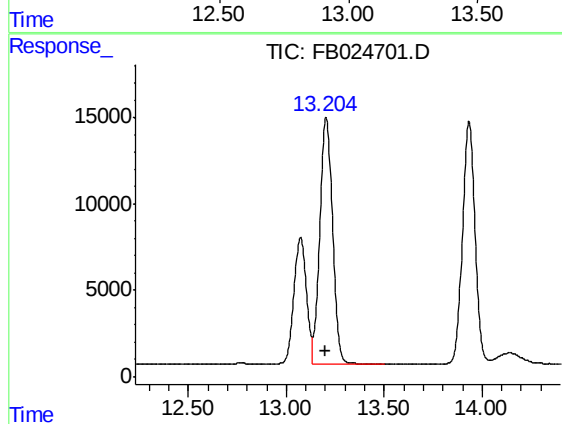


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.004 min
Response: 634221
Conc: 18.79 ng/ml

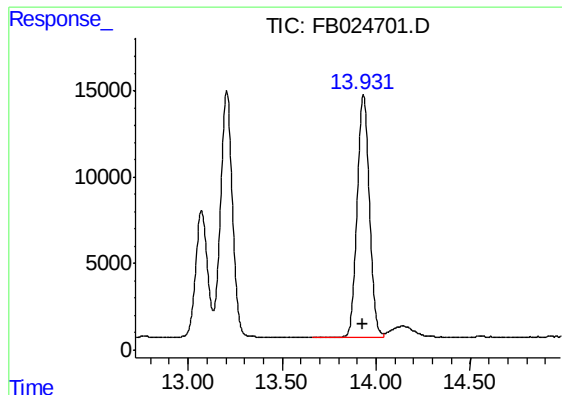

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.004 min
Response: 624939
Conc: 19.01 ng/ml

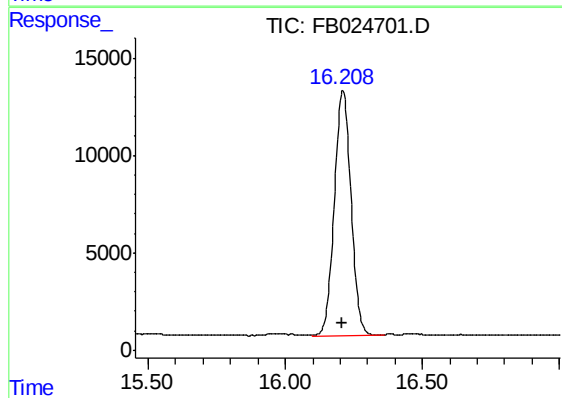

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.003 min
Response: 532973
Conc: 19.76 ng/ml