

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073024\
Data File : FB030845.D
Signal(s) : FID2B.CH
Acq On : 30 Jul 2024 19:09
Operator : YP/AJ
Sample : BSF0730S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 31 06:36:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB073024.M
Quant Title :
QLast Update : Tue Jul 30 12:33:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
6) t	Toluene	10.620	9346	0.368 ng/ml
8) t	m-Xylene	13.191	4472	0.189 ng/ml
9) t	O-Xylene	13.917	7145	0.310 ng/ml
10) t	1,2,4-Trimethylbenzene	16.191	10305	0.450 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073024\
Data File : FB030845.D
Signal(s) : FID2B.CH
Acq On : 30 Jul 2024 19:09
Operator : YP/AJ
Sample : BSF0730S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 31 06:36:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB073024.M
Quant Title :
QLast Update : Tue Jul 30 12:33:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

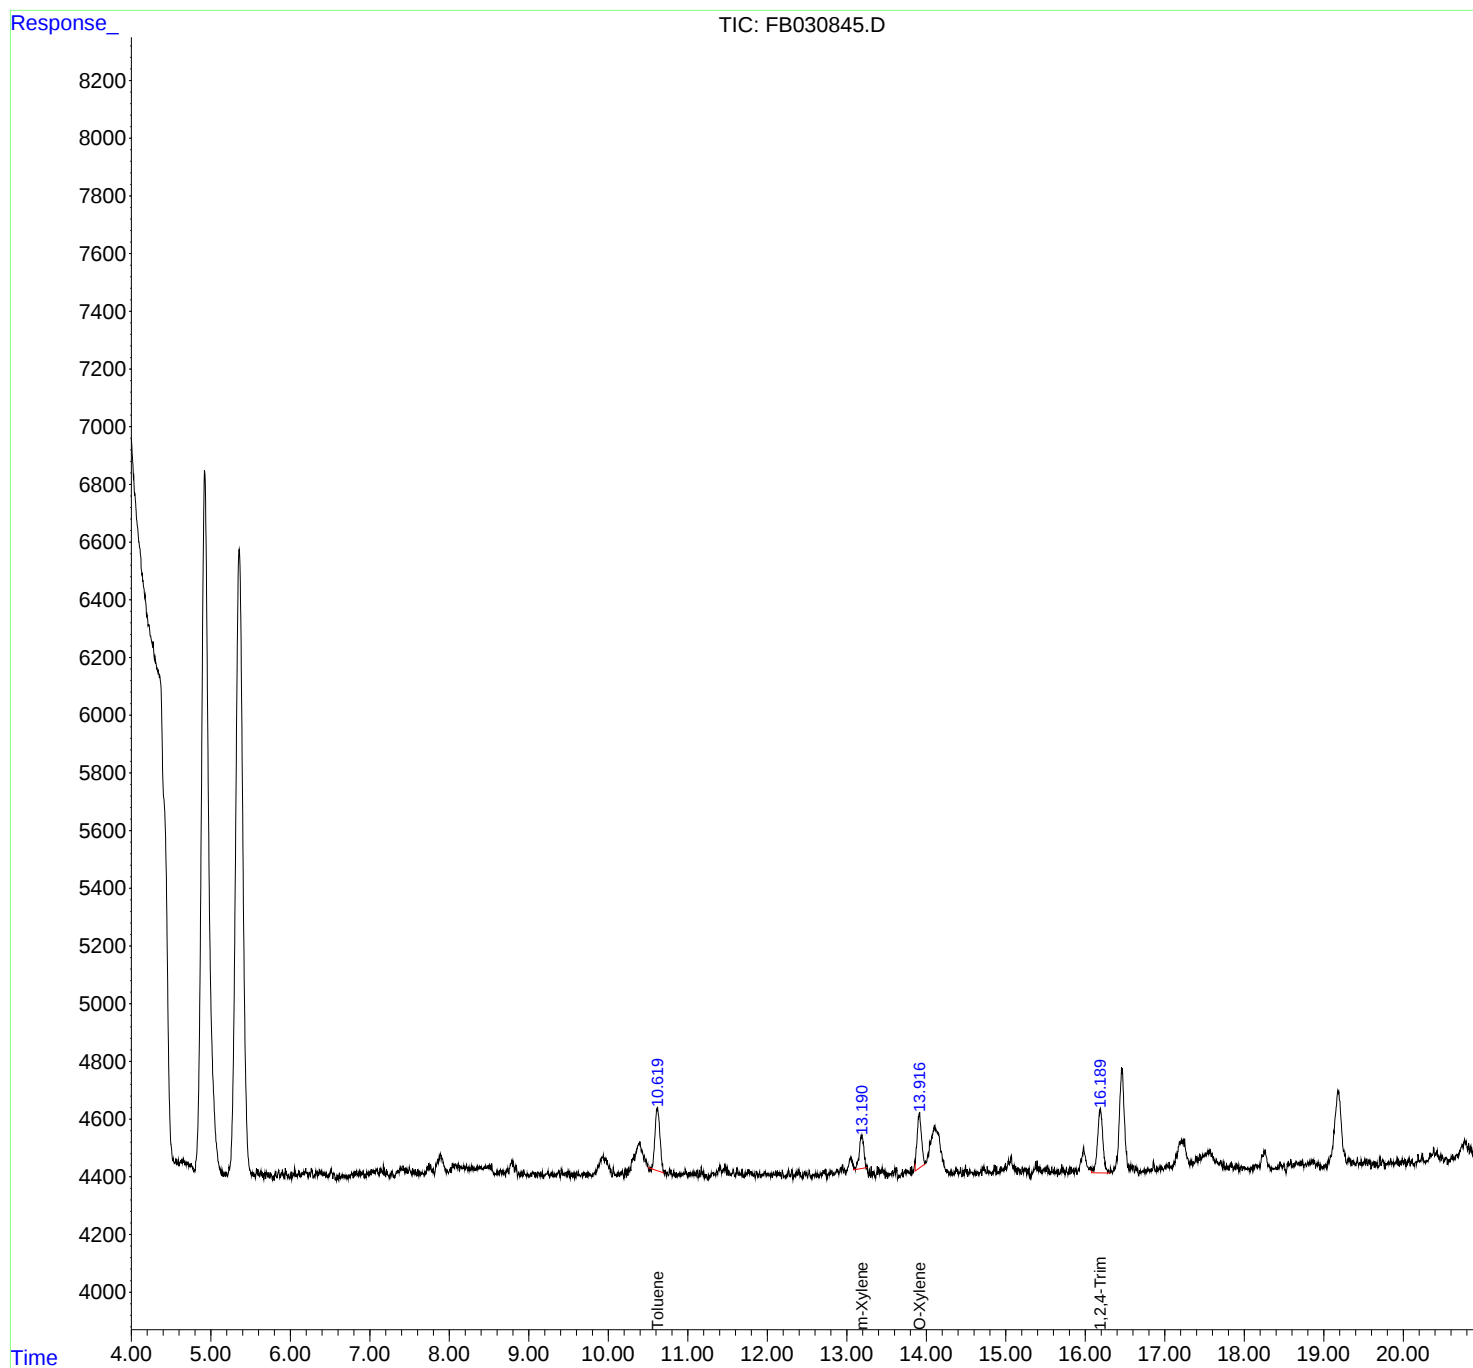


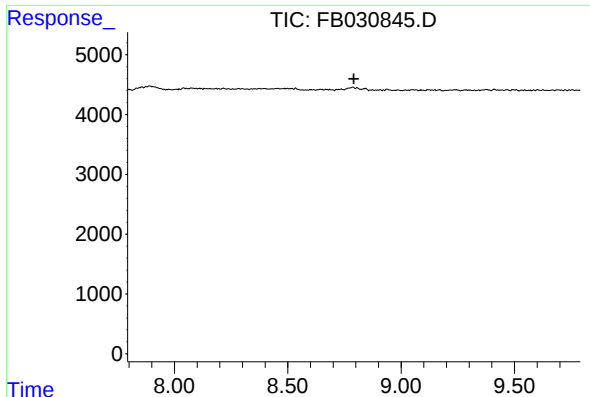

#5 AAA-TFT


R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :

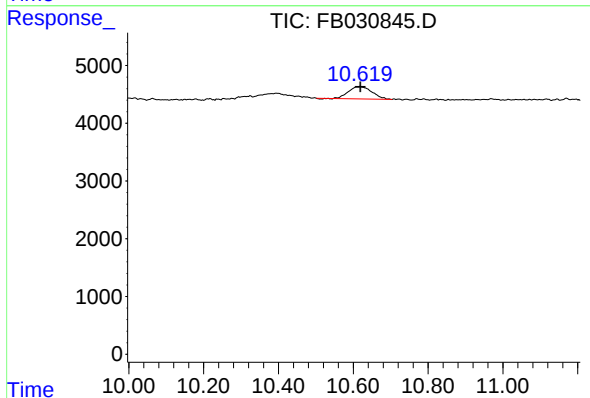


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.001 min
Response: 9346
Conc: 0.37 ng/ml

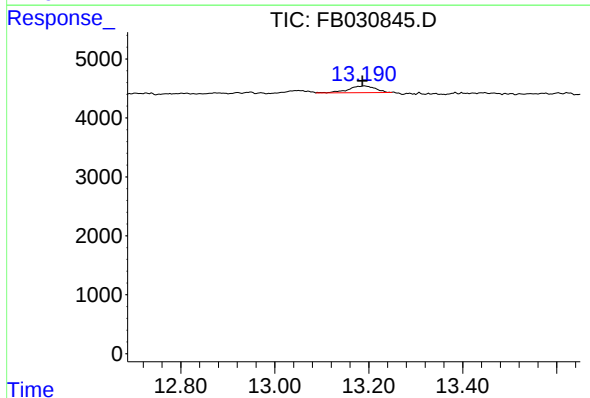


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.005 min
Response: 4472
Conc: 0.19 ng/ml

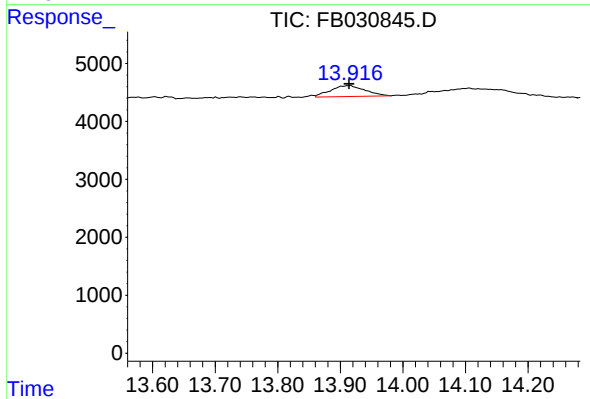

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.003 min
Response: 7145
Conc: 0.31 ng/ml

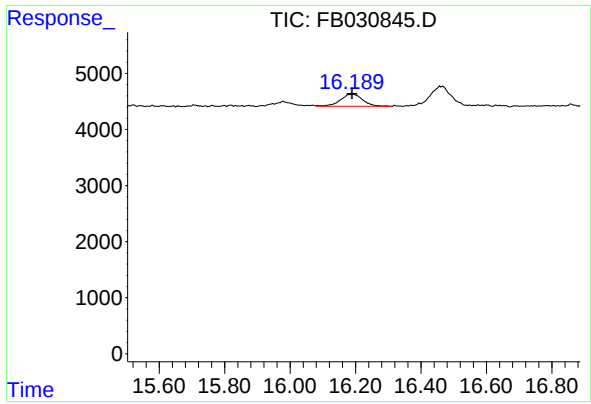

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.001 min
Response: 10305
Conc: 0.45 ng/ml

Instrument :
FID_B
ClientSampleId :